
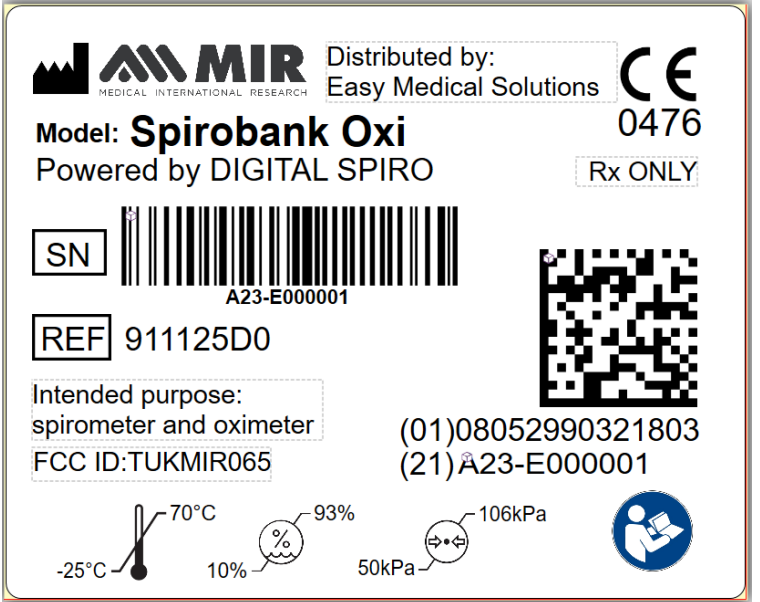
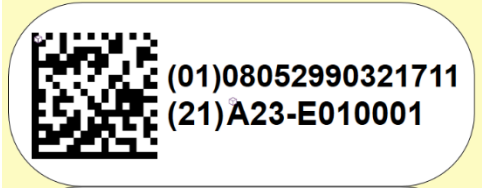
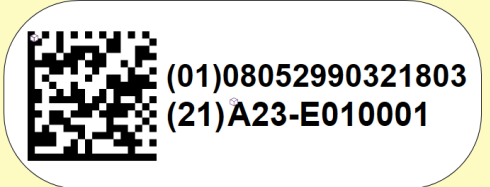


	Spirobank Oxi labeling	rev.06 15/11/2021	ST068
--	------------------------	----------------------	-------

Product name Spirobank Oxi
Product code 911125xx

DESCRIPTION	MIR CODE	LABEL
Id label	451216	
Rx Only label provided by MIR Amount needed one for each device	451294	
Manufacturing period/IFU symbol Amount needed one for each device	451293	
External label Amount needed one for each device	451216	
	460026	
	451234	

DESCRIPTION	MIR CODE	LABEL
GUDID label for USA Amount needed one for each serial number	451216	 For Spirobank OXI
	451234	 For Spirobank OXI EMS customization

The QR code in the GUDID label and in the external label must comply with the following requirements:

QR code type GS1 Datamatrix 128
 GTIN Global trade number (01)08052990321711
 Serial number (21)A23-Exxxxxx

The bar code of the serial number in the external label must comply with the following requirement:

Bar code type 128 with readable part below

REF	Description	UDI = UDI_DI + UDI_PI					
		UDI-DI	GTIN	Lot	Serial Number	Exp date	Manuf. Date
			(01)	(10)	(21)	(17)	(11)
911125	Spirobank Oxi with reusable turbine	8052990321711	X	-	X	-	-
911125B0	Spirobank Oxi without reusable turbine	8052990321711	X	-	X	-	-
911125P1	Spirobank Oxi F/V with reusable turbine	8052990321711	X	-	X	-	-
911125P0	Spirobank Oxi F/V without reusable turbine	8052990321711	X	-	X	-	-
911125S1	Spirobank Oxi F/V SVC with reusable turbine	8052990321711	X	-	X	-	-
911125S0	Spirobank Oxi F/V SVC without reusable turbine	8052990321711	X	-	X	-	-
911125D0	Spirobank Oxi F/V SVC without reusable turbine (EMS customization)	8052990321803	X	-	X	-	-

Concerning the proper application of the labeling please refer to ILC038.