

System Check_Head_2450MHz

DUT: D2450V2 - SN806

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_2450_231108 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.79$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(7.38, 7.38, 7.38); Calibrated: 2023-04-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2023-08-17
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238-; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.71 W/kg; SAR (10g) = 1.23 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.68 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 76.6 %

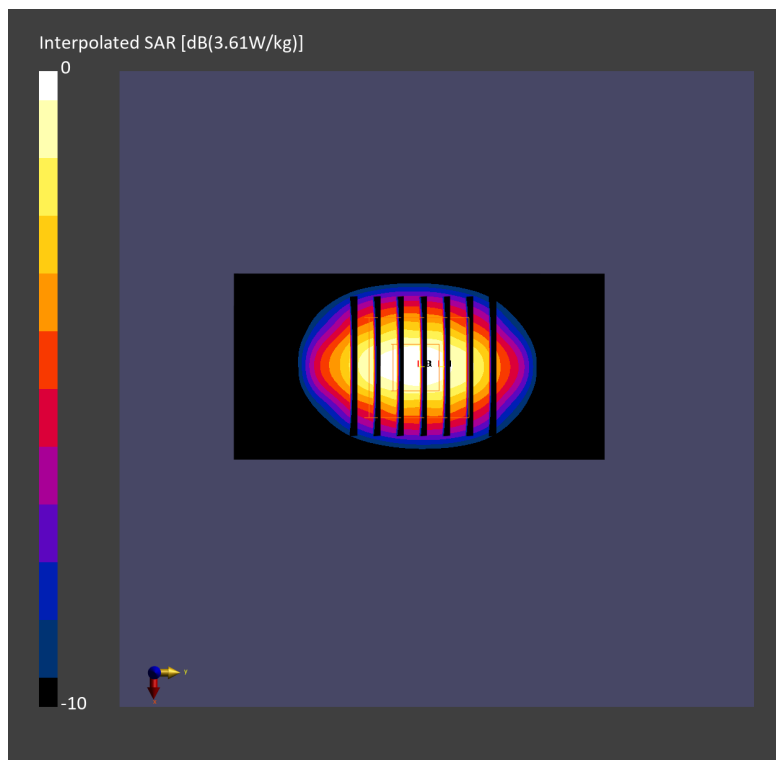

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5250_231109 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.71$ S/m; $\epsilon_r = 37.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(4.5, 4.5, 4.5); Calibrated: 2023-04-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2023-08-17
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238-; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 4.02 W/kg; SAR (10g) = 1.13 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.04 dB

SAR (1g) = 4.11 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.17 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 65.3 %

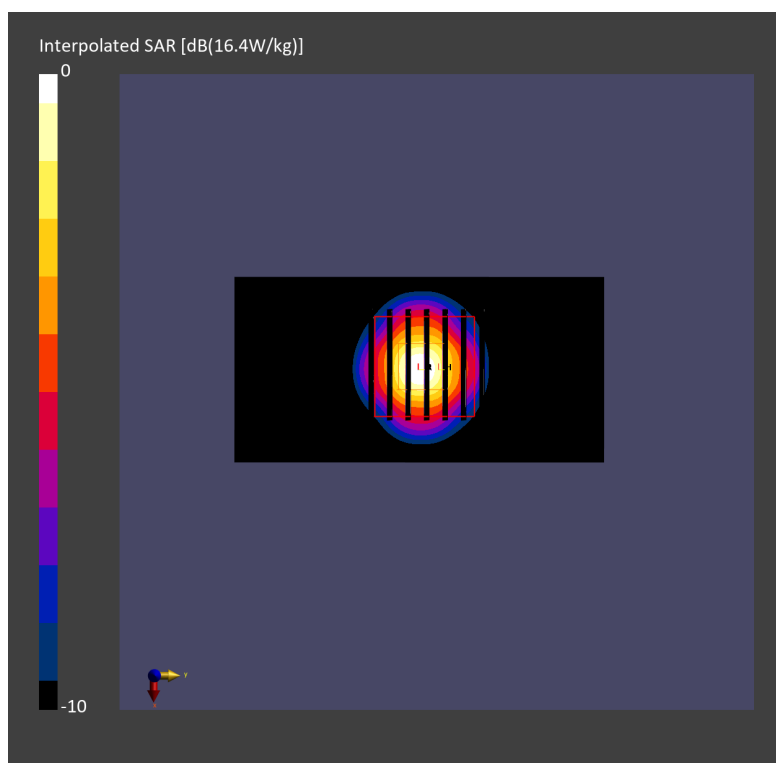

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_5600_231109 Medium parameters used: $f=5600.000$ MHz; $\sigma=5.07$ S/m; $\epsilon_r=36.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(4.11, 4.11, 4.11); Calibrated: 2023-04-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2023-08-17
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238-; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 4.28 W/kg; SAR (10g) = 1.19 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 4.39 W/kg; SAR (8g) = 1.44 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 62.5 %

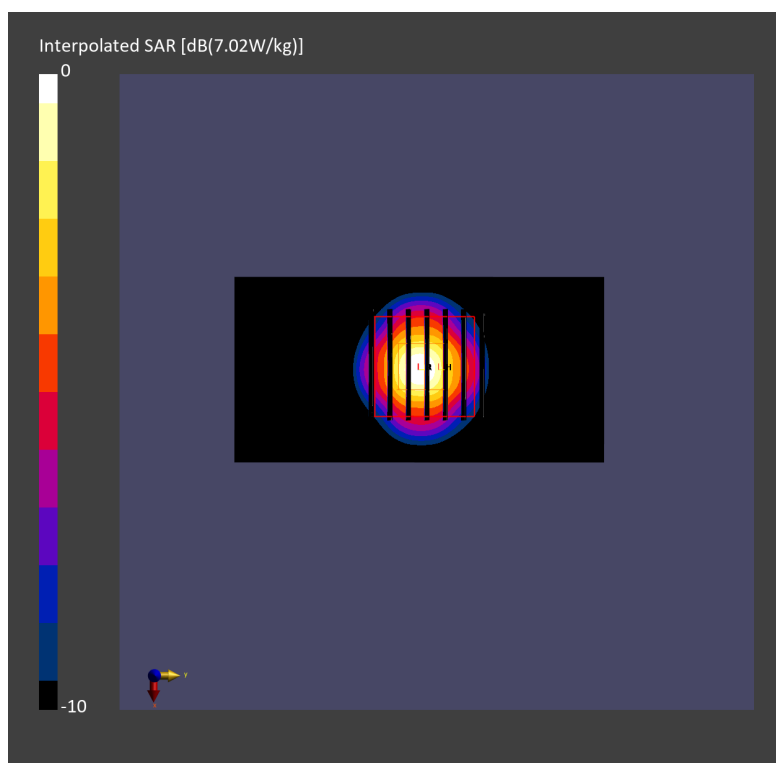

System Check_Head_5750MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5750.000 MHz

Medium: HSL_5750_231109 Medium parameters used: $f=5750.000$ MHz; $\sigma=5.23$ S/m; $\epsilon_r=36.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(4.23, 4.23, 4.23); Calibrated: 2023-04-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2023-08-17
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238-; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.95 W/kg; SAR (10g) = 1.10 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 4.01 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 61.4 %

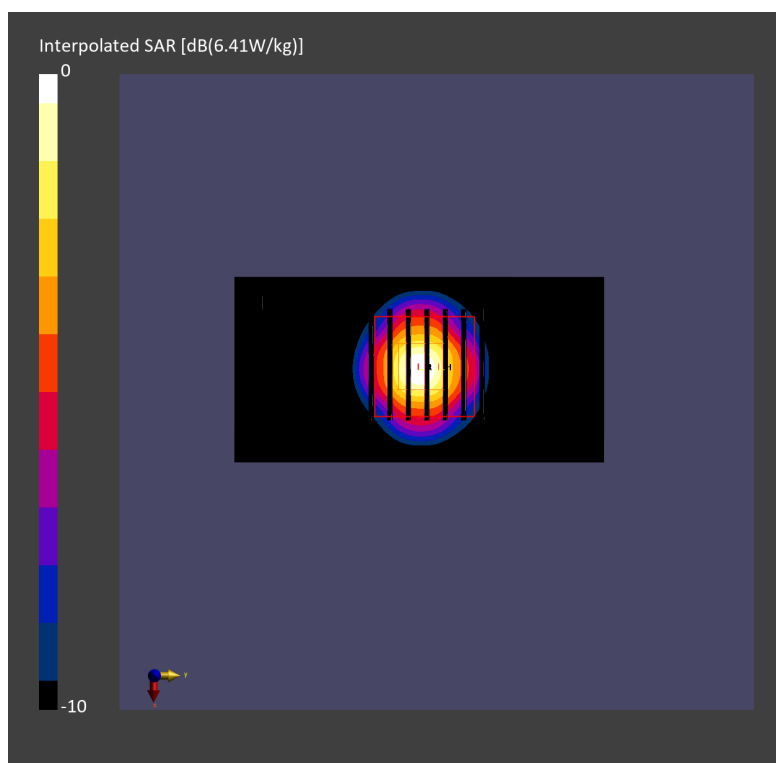

System Check_Head_5850MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5850.000 MHz

Medium: HSL_5850_231109 Medium parameters used: $f = 5850.000$ MHz; $\sigma = 5.33$ S/m; $\epsilon_r = 36.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3642; ConvF(4.06, 4.06, 4.06); Calibrated: 2023-04-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn854; Calibrated: 2023-08-17
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1238-; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 4.04 W/kg; SAR (10g) = 1.12 W/kg;

Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.00 dB

SAR (1g) = 4.09 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 60.9 %

