

System Check_Head_2450MHz

DUT: D2450V2 - SN929

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: HSL_2450_231105 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.77$ S/m; $\epsilon_r = 39.0$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(7.5, 7.5, 7.5); Calibrated: 2023-03-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2023-02-22
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2153; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW


Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.20 W/kg; SAR (10g) = 1.05 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.04 dB

SAR (1g) = 2.43 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.15 W/kg

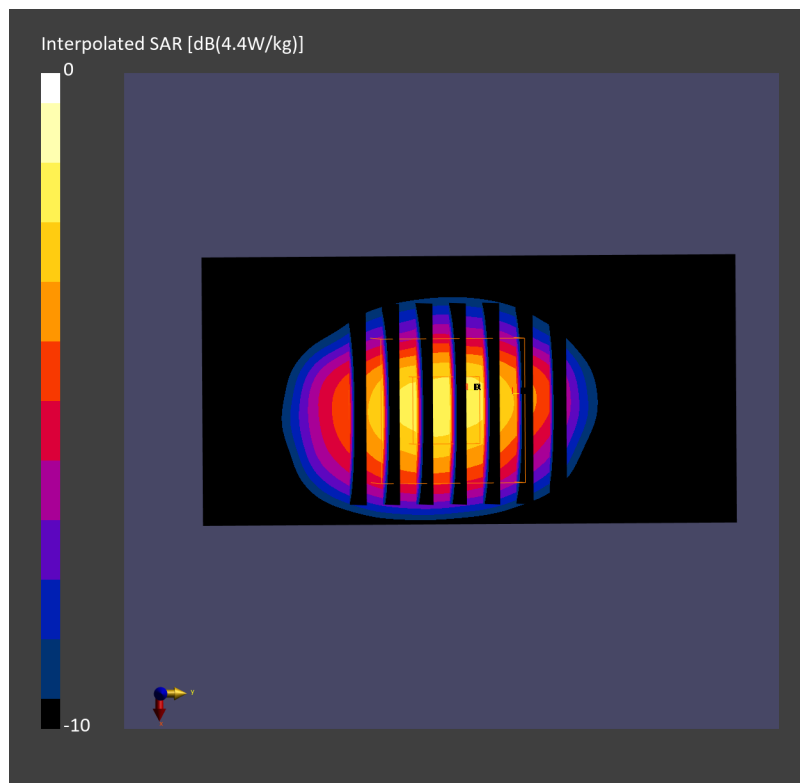

System Check_Head_2450MHz

DUT: D2450V2 - SN929

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: HSL_2450_231106 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.81$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.82, 7.82, 7.82); Calibrated: 2023-02-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2023-01-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW


Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.39 W/kg; SAR (10g) = 1.12 W/kg;

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.04 dB

SAR (1g) = 2.41 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.13 W/kg

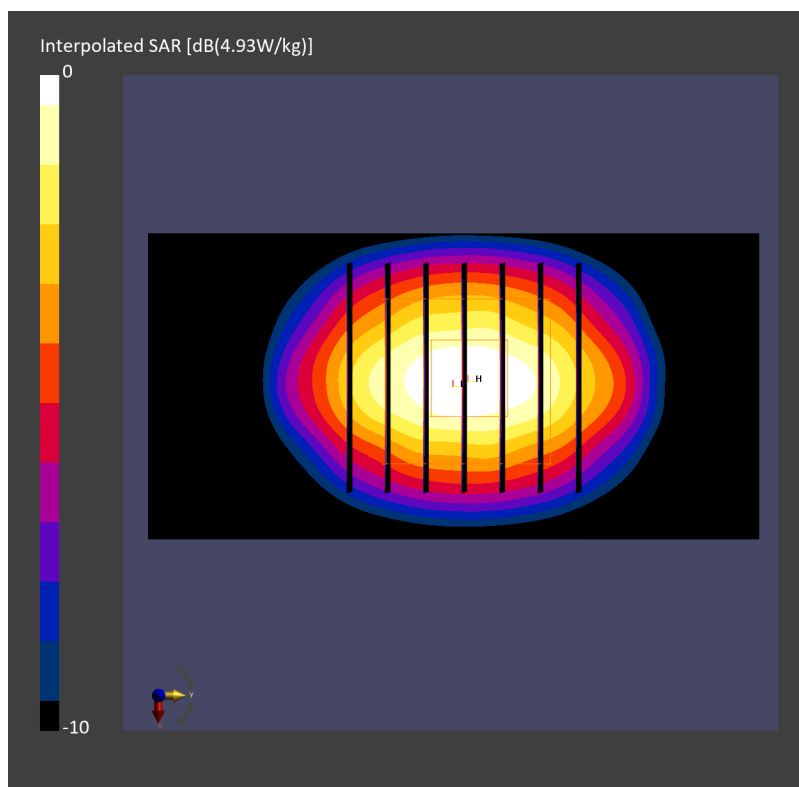

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1128

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: HSL_5G_231106 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.64$ S/m; $\epsilon_r = 35.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(4.93, 5.47, 4.85); Calibrated: 2023-02-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2023-03-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2192_0mm; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW


Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.22 W/kg; SAR (10g) = 1.02 W/kg;

Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.68 W/kg; SAR (8g) = 1.30 W/kg; SAR (10g) = 1.12 W/kg

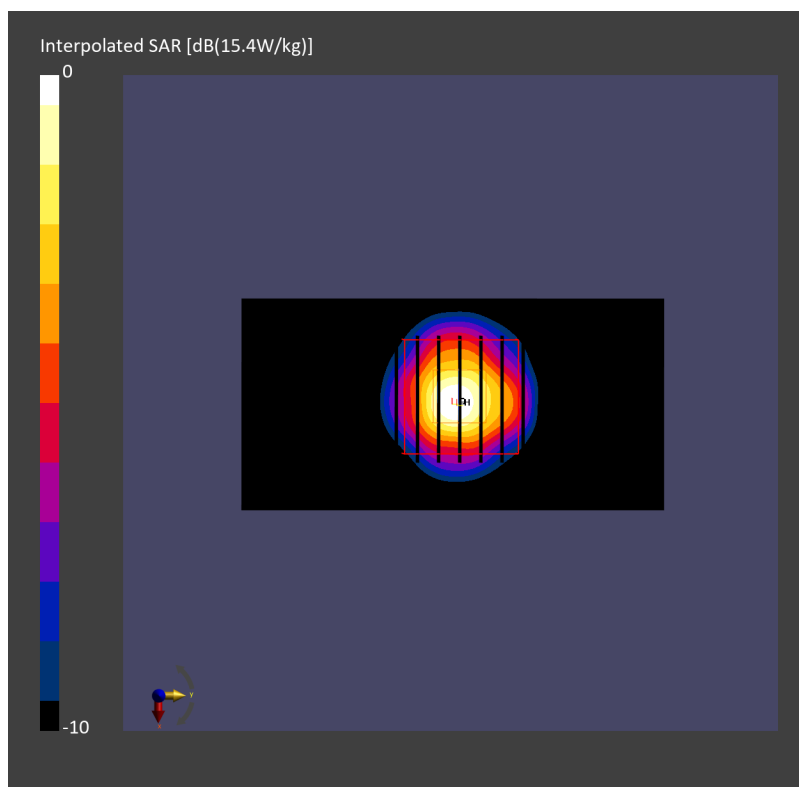

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: HSL_5G_231106 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.65$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(5.46, 5.46, 5.46); Calibrated: 2023-02-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2023-01-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW


Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.51 W/kg; SAR (10g) = 0.994 W/kg;

Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 4.01 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.17 W/kg

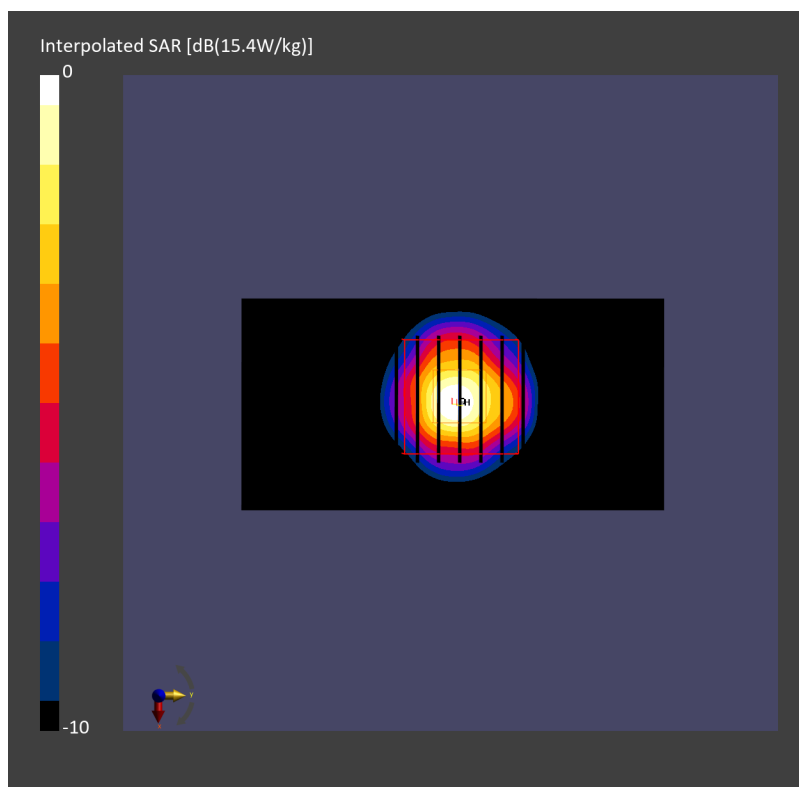

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1128

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: HSL_5G_231116 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.67$ S/m; $\epsilon_r = 37.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7625; ConvF(5.5, 5.5, 5.5); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2023-09-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2196; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.28 W/kg; SAR (10g) = 0.950 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.07 dB

SAR (1g) = 3.53 W/kg; SAR (8g) = 1.25 W/kg; SAR (10g) = 1.08 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 67.2 %

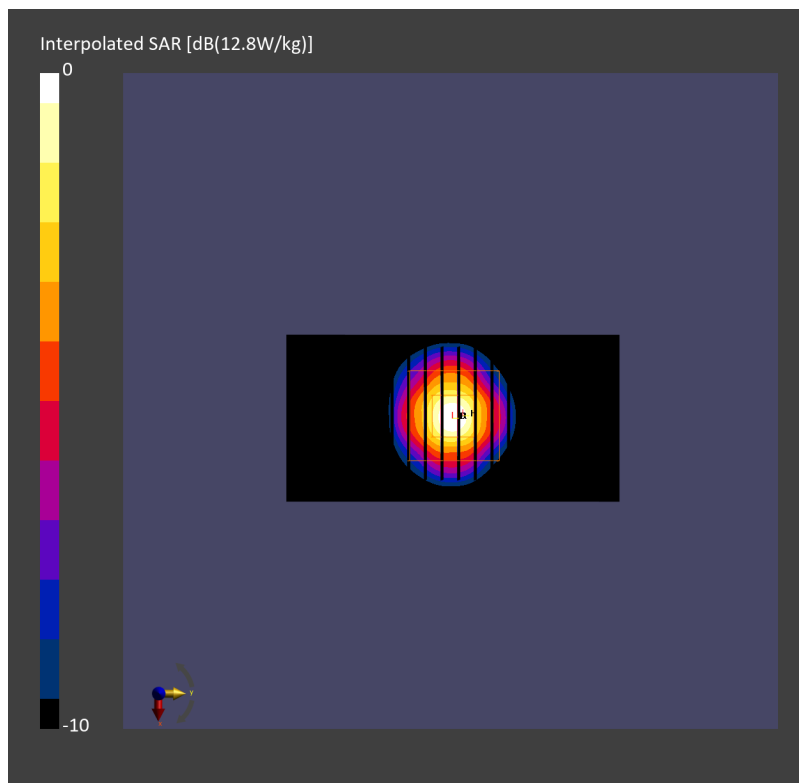

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1128

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: HSL_5G_231106 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.03$ S/m; $\epsilon_r = 34.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(4.35, 4.72, 4.41); Calibrated: 2023-02-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2023-03-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2192_0mm; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW


Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.30 W/kg; SAR (10g) = 1.04 W/kg;

Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.10 dB

SAR (1g) = 3.71 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.15 W/kg

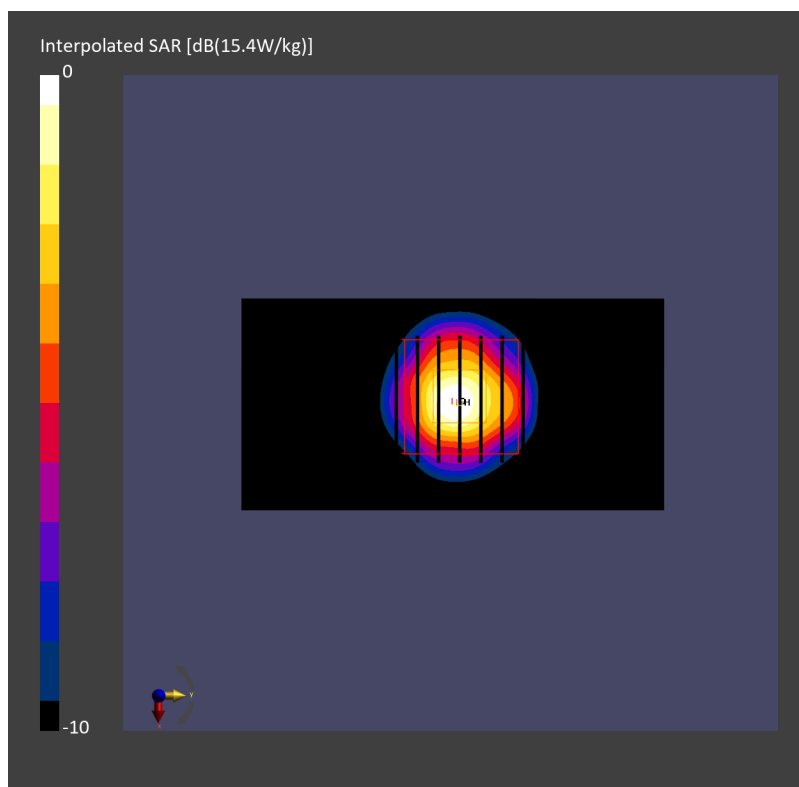

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: HSL_5G_231106 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.05$ S/m; $\epsilon_r = 35.0$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(4.9, 4.9, 4.9); Calibrated: 2023-02-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2023-01-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW


Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.62 W/kg; SAR (10g) = 1.03 W/kg;

Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.95 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.16 W/kg

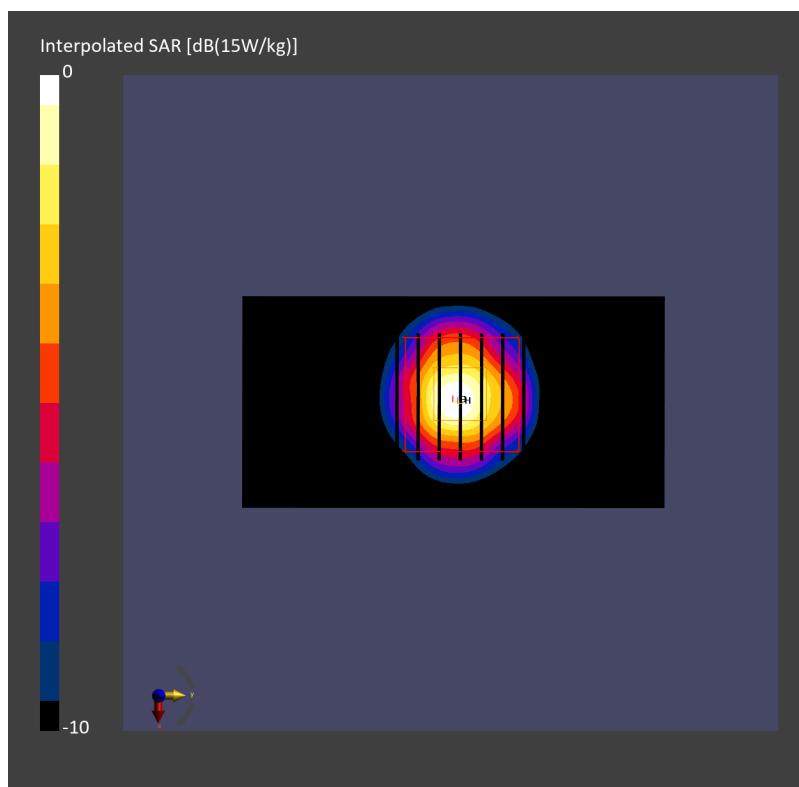

System Check_Head_5750MHz

DUT: D5GHzV2 - SN1128

Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1

Medium: HSL_5G_231105 Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.33$ S/m; $\epsilon_r = 35.9$

Ambient Temperature: 23.9°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7590; ConvF(5.02, 5.02, 5.02); Calibrated: 2023-03-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2023-02-22
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2153; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW


Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.00 W/kg; SAR (10g) = 0.961 W/kg;

Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.04 dB

SAR (1g) = 3.60 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.10 W/kg

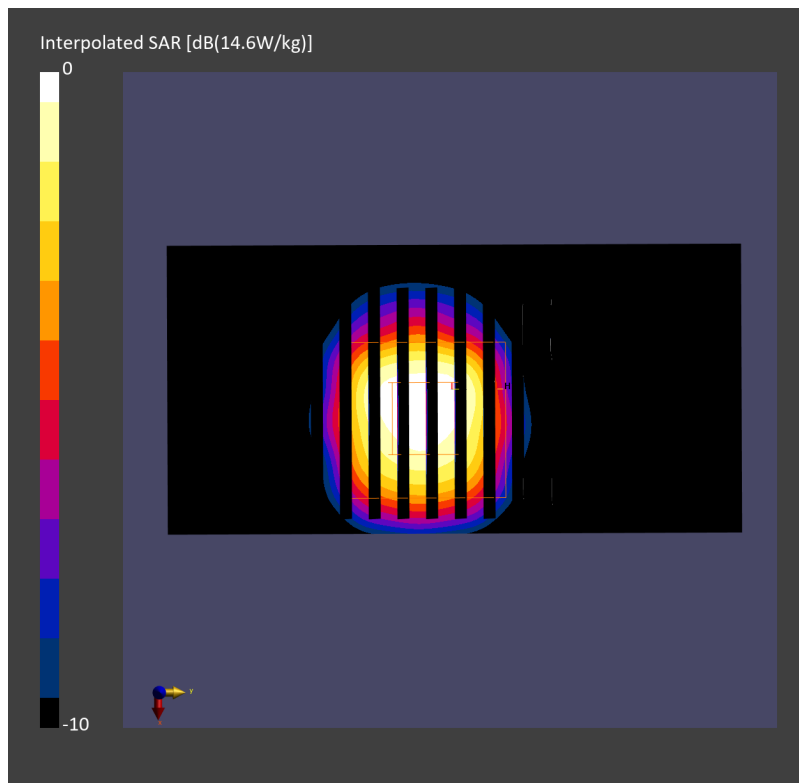

System Check_Head_5750MHz

DUT: D5GHzV2 - SN1128

Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1

Medium: HSL_5G_231106 Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.22$ S/m; $\epsilon_r = 34.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7791; ConvF(4.44, 4.92, 4.4); Calibrated: 2023-02-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1776; Calibrated: 2023-03-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2192_0mm; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW


Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.23 W/kg; SAR (10g) = 1.02 W/kg;

Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.07 dB

SAR (1g) = 3.65 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.12 W/kg

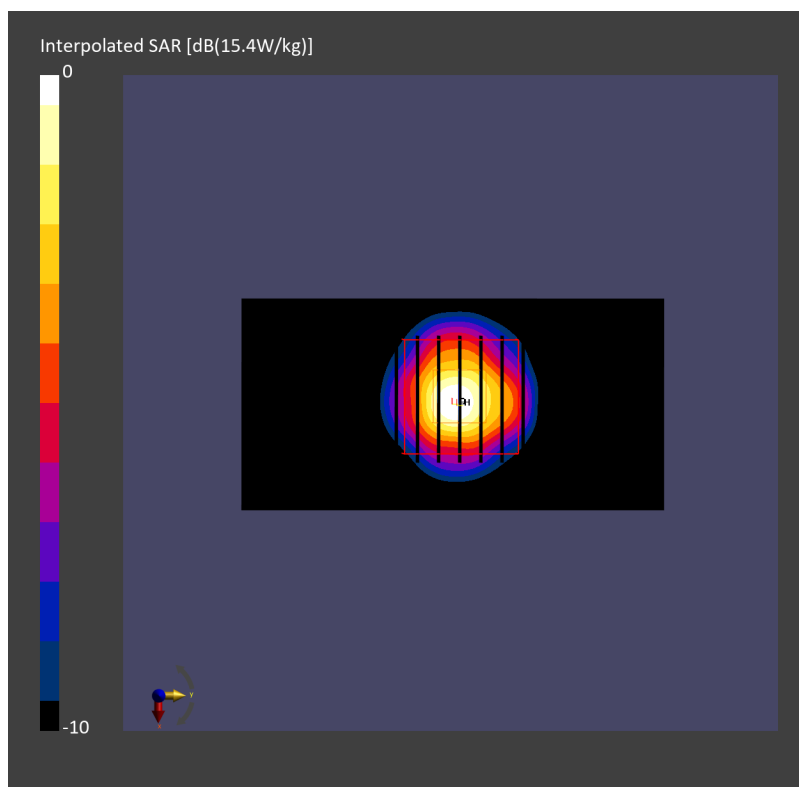

System Check_Head_5750MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1

Medium: HSL_5G_231106 Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.23$ S/m; $\epsilon_r = 34.7$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(4.87, 4.87, 4.87); Calibrated: 2023-02-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2023-01-09
- Phantom: ELI V4.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW


Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.30 W/kg; SAR (10g) = 0.937 W/kg;

Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.86 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.09 W/kg

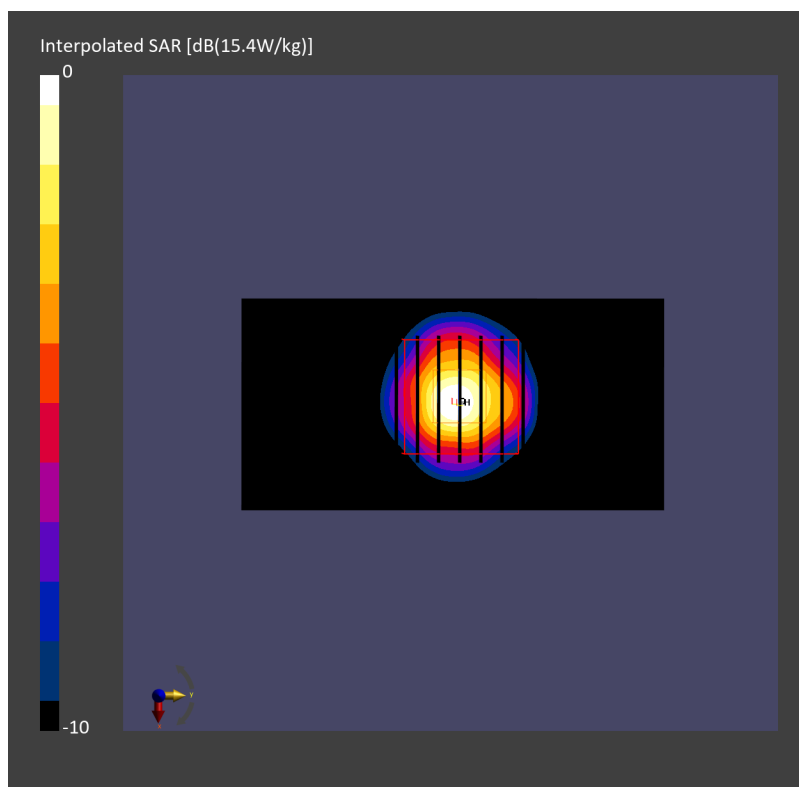

System Check_Head_6500MHz

DUT: D6.5GHzV2 - SN1003

Communication System: CW; Frequency: 6500.000 MHz; Duty Cycle: 1:1

Medium: HSL_6G_231108 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 5.86$ S/m; $\epsilon_r = 35.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7793; ConvF(4.8, 4.6, 4.93); Calibrated: 2023-03-08
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn376; Calibrated: 2023-09-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2196; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 24.4 W/kg; SAR (10g) = 4.86 W/kg;

Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.09 dB

SAR (1g) = 27.2 W/kg; SAR (8g) = 6.36 W/kg; SAR (10g) = 5.23 W/kg

psAPD (1.0cm², sq) = 272 [W/m²]; psAPD (4.0cm², sq) = 127 [W/m²]

