### ANNEX C: DIPOLE CERTIFICATE

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kallbrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

ETC (Auden)

Certificate No: D1900V2-5d054\_Oct06

SE I	D1900V2 - SN: 50	1054	
Object	D1900V2 - 3N. 30		OHIO CONTRACTOR OF THE PROPERTY OF THE PROPERT
Calibration procedure(s)	QA CAL-05.v6 Calibration proces	dure for dipole validation kits	
Calibration date:	October 17, 2006		
Condition of the calibrated item	In Tolerance		
		y facility: environment temperature (22 ± 3)°C and	a numbarry < 70%.
Callbration Equipment used (M&	Vienes.		Cabadulad Callbartina
	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Primary Standards	ID# GB37480704	03-Oct-06 (METAS, No. 217-00608)	Oct-07
Primary Standards Power meter EPM-442A	ID # GB37480704 US37292783	03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608)	Oct-07 Oct-07
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator	ID# GB37480704 US37292783 SN: 5086 (20g)	03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No 217-00591)	Oct-07 Oct-07 Aug-07
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator	ID# GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r)	03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No 217-00591) 10-Aug-06 (METAS, No 217-00591)	Oct-07 Oct-07 Aug-07 Aug-07
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6	ID# GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507	03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No 217-00591) 10-Aug-06 (METAS, No 217-00591) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05)	Oct-07 Oct-07 Aug-07
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 Reference Probe ES3DV3	ID# GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r)	03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No 217-00591) 10-Aug-06 (METAS, No 217-00591)	Oct-07 Oct-07 Aug-07 Aug-07 Oct-06
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 Reference Probe ES3DV3 DAE4	ID# GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507 SN: 3025 SN: 601	03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No 217-00591) 10-Aug-06 (METAS, No 217-00591) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 28-Oct-05 (SPEAG, No. ES3-3025_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05)	Oct-07 Oct-07 Aug-07 Aug-07 Oct-06 Oct-06
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 Reference Probe ES3DV3 DAE4 Secondary Standards	ID#  GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507 SN: 3025 SN: 601  ID#	03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No 217-00591) 10-Aug-06 (METAS, No 217-00591) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 28-Oct-05 (SPEAG, No. ES3-3025_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house)	Oct-07 Oct-07 Aug-07 Aug-07 Oct-06 Oct-06 Dec-06
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A	ID#  GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507 SN: 3025 SN: 601  ID#  MY41092317	03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No 217-00591) 10-Aug-06 (METAS, No 217-00591) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 28-Oct-05 (SPEAG, No. ES3-3025_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05)	Oct-07 Oct-07 Aug-07 Aug-07 Oct-06 Oct-06 Dec-06 Scheduled Check
Primary Standards  Power meter EPM-442A  Power sensor HP 8481A  Reference 20 dB Attenuator  Reference 10 dB Attenuator  Reference Probe ET3DV6  Reference Probe ES3DV3  DAE4  Secondary Standards  Power sensor HP 8481A  RF generator Agilent E4421B	ID#  GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507 SN: 3025 SN: 601  ID#	03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No 217-00591) 10-Aug-06 (METAS, No 217-00591) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 28-Oct-05 (SPEAG, No. ES3-3025_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house)	Oct-07 Oct-07 Aug-07 Aug-07 Oct-06 Oct-06 Dec-06 Scheduled Check In house check: Oct-07
Primary Standards  Power meter EPM-442A  Power sensor HP 8481A  Reference 20 dB Attenuator  Reference 10 dB Attenuator  Reference Probe ET3DV6  Reference Probe ES3DV3  DAE4  Secondary Standards  Power sensor HP 8481A  RF generator Agilent E4421B	ID #  GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507 SN: 3025 SN: 601  ID #  MY41092317 MY41000675 US37390585 S4206	03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No. 217-00591) 10-Aug-06 (METAS, No 217-00591) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 28-Oct-05 (SPEAG, No. ES3-3025_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house)  18-Oct-02 (SPEAG, in house check Nov-05) 11-May-05 (SPEAG, in house check Nov-05)	Oct-07 Oct-07 Aug-07 Aug-07 Oct-06 Oct-06 Dec-06 Scheduled Check In house check: Oct-07 In house check: Nov-07 In house check: Nov-06
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator Agilent E4421B Network Analyzer HP 8753E	ID #  GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507 SN: 3025 SN: 601  ID #  MY41092317 MY41000675 US37390585 S4206  Name	03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No. 217-00591) 10-Aug-06 (METAS, No 217-00591) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 28-Oct-05 (SPEAG, No. ES3-3025_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05)	Oct-07 Oct-07 Aug-07 Aug-07 Oct-06 Oct-06 Dec-06 Scheduled Check In house check: Oct-07 In house check: Nov-07 In house check: Nov-06
Primary Standards  Power meter EPM-442A  Power sensor HP 8481A  Reference 20 dB Attenuator  Reference 10 dB Attenuator  Reference Probe ET3DV6  Reference Probe ES3DV3  DAE4  Secondary Standards  Power sensor HP 8481A  RF generator Agilent E4421B	ID #  GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507 SN: 3025 SN: 601  ID #  MY41092317 MY41000675 US37390585 S4206	03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No. 217-00591) 10-Aug-06 (METAS, No 217-00591) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 28-Oct-05 (SPEAG, No. ES3-3025_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house)  18-Oct-02 (SPEAG, in house check Nov-05) 11-May-05 (SPEAG, in house check Nov-05)	Oct-07 Oct-07 Aug-07 Aug-07 Oct-06 Oct-06 Dec-06 Scheduled Check In house check: Oct-07 In house check: Nov-07 In house check: Nov-06
Calibration Equipment used (M& Primary Standards  Power meter EPM-442A  Power sensor HP 8481A  Reference 20 dB Attenuator  Reference 10 dB Attenuator  Reference Probe ET3DV6  Reference Probe ES3DV3  DAE4  Secondary Standards  Power sensor HP 8481A  RF generator Agilent E4421B  Network Analyzer HP 8753E  Calibrated by:	ID #  GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507 SN: 3025 SN: 601  ID #  MY41092317 MY41000675 US37390585 S4206  Name	03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No. 217-00591) 10-Aug-06 (METAS, No 217-00591) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 28-Oct-05 (SPEAG, No. ES3-3025_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05)	Oct-07 Oct-07 Aug-07 Aug-07 Oct-06 Oct-06 Dec-06 Scheduled Check In house check: Oct-07 In house check: Nov-07 In house check: Nov-06

Certificate No: D1900V2-5d054\_Oct06

Page 1 of 9

### Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z not applicable or not measured

Calibration is Performed According to the Following Standards:

 a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003

b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001

c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

### **Additional Documentation:**

d) DASY4 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D1900V2-5d054\_Oct06

Page 2 of 9

### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

### **Head TSL parameters**

The following parameters and calculations were applied.

ne following parameters and calculations were	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.3 ± 6 %	1.42 mho/m ± 6 %
Head TSL temperature during test	(20.5 ± 0.2) °C		

### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	condition	
SAR measured	250 mW input power	9.56 mW / g
SAR normalized	normalized to 1W	38.2 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	37.6 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.07 mW / g
SAR normalized	normalized to 1W	20.3 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	20.1 mW / g ± 16.5 % (k=2)

Certificate No: D1900V2-5d054\_Oct06

<sup>&</sup>lt;sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

### **Body TSL parameters**

The following parameters and calculations were applied.

ne following parameters and calculations were	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.4 ± 6 %	1.54 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C		( <del></del>

### SAR result with Body TSL

SAR averaged over 1 cm3 (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.60 mW / g
SAR normalized	normalized to 1W	38.4 mW / g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	37.7 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.08 mW / g
SAR normalized	normalized to 1W	20.3 mW / g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	20.1 mW / g ± 16.5 % (k=2)

<sup>&</sup>lt;sup>2</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Report No.: 07-09-MAS-015-03 Page 58 of 71

FCC ID: U23MD6430H

### **Appendix**

# Antenna Parameters with Head TSL

Impedance, transformed to feed point	56.9 Ω + 3.5 jΩ	
Return Loss	- 22.8 dB	
Totalli Edda		

### Antenna Parameters with Body TSL

Impedance, transformed to feed point	51.8 Ω + 5.1 jΩ	
impedance, transformed to feed point		
Return Loss	- 25.5 dB	

### General Antenna Parameters and Design

1.198 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	March 19, 2004

## DASY4 Validation Report for Head TSL

Date/Time: 11.10.2006 15:17:05

Test Laboratory: SPEAG, Zurich, Switzerland

# DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d054

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL U10 BB;

Medium parameters used: f = 1900 MHz;  $\sigma$  = 1.42 mho/m;  $\epsilon_r$  = 39.3;  $\rho$  = 1000 kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

### DASY4 Configuration:

Probe: ET3DV6 - SN1507 (HF); ConvF(4.74, 4.74, 4.74); Calibrated: 28.10.2005

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 15.12.2005

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA

Measurement SW: DASY4, V4.7 Build 44; Postprocessing SW: SEMCAD, V1.8 Build 171

## Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 90.1 V/m; Power Drift = 0.042 dB

Peak SAR (extrapolated) = 16.3 W/kg

SAR(1 g) = 9.56 mW/g; SAR(10 g) = 5.07 mW/g

Maximum value of SAR (measured) = 10.7 mW/g

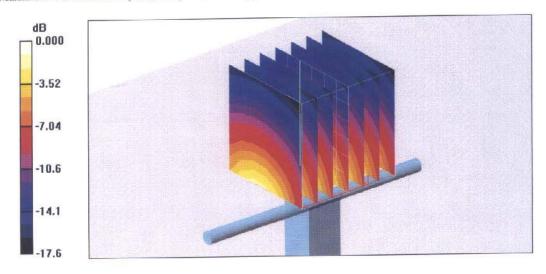


0 dB = 10.7 mW/g

Certificate No: D1900V2-5d054\_Oct06

Page 6 of 9

# Impedance Measurement Plot for Head TSL

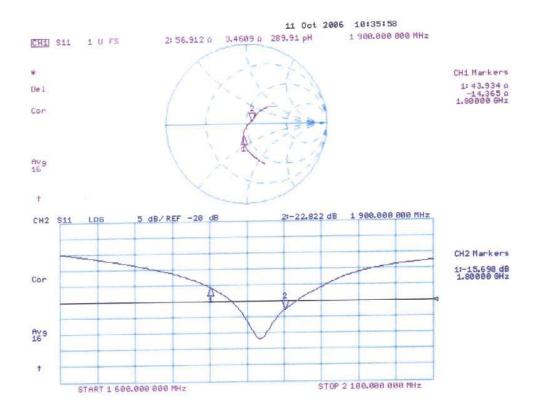

### DASY4 Validation Report for Body TSL

Date/Time: 17.10.2006 15:56:11

Test Laboratory: SPEAG, Zurich, Switzerland

# DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d054

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: MSL U10;

Medium parameters used: f = 1900 MHz;  $\sigma = 1.54$  mho/m;  $\epsilon_r = 52.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

### DASY4 Configuration:

Probe: ET3DV6 - SN1507 (HF); ConvF(4.3, 4.3, 4.3); Calibrated: 28.10.2005

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 15.12.2005

Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA

Measurement SW: DASY4, V4.7 Build 44; Postprocessing SW: SEMCAD, V1.8 Build 171


### Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 90.4 V/m; Power Drift = -0.027 dB

Peak SAR (extrapolated) = 16.8 W/kg

SAR(1 g) = 9.6 mW/g; SAR(10 g) = 5.08 mW/g

Maximum value of SAR (measured) = 10.9 mW/g

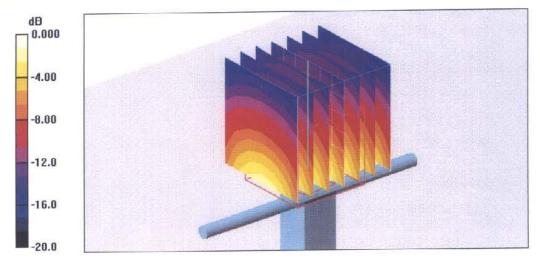


0 dB = 10.9 mW/g

Certificate No: D1900V2-5d054\_Oct06

Page 8 of 9

# Impedance Measurement Plot for Body TSL

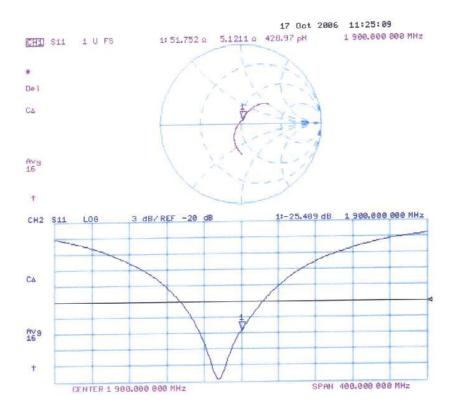

### **ANNEX D: PROBE CERTIFICATE**

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

ETC (Auden)

Accreditation No.: SCS 108

Certificate No: ET3-1791\_Sep06

Object	ET3DV6 - SN:1791				
Calibration procedure(s)	QA CAL-01.v5 Calibration procedure for dosimetric E-field probes				
Calibration date:	September 19,	2006			
Condition of the calibrated item	In Tolerance				
		ntional standards, which realize the physical units of probability are given on the following pages and are			
All authoritors have been condu	ated in the alaced laborat	ory facility: environment temperature (22 ± 3)°C and	d humidity < 70%		
All calibrations have been condu	cted in the closed laborat	ory racinty, environment temperature (22 1 5) G and	d Harriotty - 7076.		
		ory racinity. environment temperature (22 ± 3) © and	o namony × 1076.		
Calibration Equipment used (M&		Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration		
Calibration Equipment used (M&	TE critical for calibration)				
Calibration Equipment used (M& Primary Standards Power meter E4419B	TE critical for calibration)	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration		
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A	TE critical for calibration)  ID #  GB41293874	Cal Date (Calibrated by, Certificate No.)  5-Apr-06 (METAS, No. 251-00557)  5-Apr-06 (METAS, No. 251-00557)  5-Apr-06 (METAS, No. 251-00557)	Scheduled Calibration  Apr-07  Apr-07  Apr-07		
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A	TE critical for calibration)  ID #  GB41293874  MY41495277	Cal Date (Calibrated by, Certificate No.)  5-Apr-06 (METAS, No. 251-00557)  5-Apr-06 (METAS, No. 251-00557)  5-Apr-06 (METAS, No. 251-00557)  10-Aug-06 (METAS, No. 217-00592)	Scheduled Calibration  Apr-07  Apr-07  Apr-07  Aug-07		
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	ID #  GB41293874  MY41495277  MY41498087  SN: S5054 (3c)  SN: S5086 (20b)	Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 251-00558)	Scheduled Calibration  Apr-07  Apr-07  Aug-07  Aug-07  Apr-07		
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator	TE critical for calibration)  ID #  GB41293874  MY41495277  MY41498087  SN: S5054 (3c)  SN: S5086 (20b)  SN: S5129 (30b)	Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 251-00558) 10-Aug-06 (METAS, No. 217-00593)	Scheduled Calibration  Apr-07  Apr-07  Apr-07  Aug-07  Apr-07  Aug-07		
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2	TE critical for calibration)  ID #  GB41293874  MY41495277  MY41498087  SN: S5054 (3c)  SN: S5086 (20b)  SN: S5129 (30b)  SN: 3013	Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 217-00593) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06)	Scheduled Calibration  Apr-07  Apr-07  Apr-07  Aug-07  Apr-07  Aug-07  Jan-07		
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2	TE critical for calibration)  ID #  GB41293874  MY41495277  MY41498087  SN: S5054 (3c)  SN: S5086 (20b)  SN: S5129 (30b)	Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 251-00558) 10-Aug-06 (METAS, No. 217-00593)	Scheduled Calibration  Apr-07  Apr-07  Apr-07  Aug-07  Apr-07  Aug-07		
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	TE critical for calibration)  ID #  GB41293874  MY41495277  MY41498087  SN: S5054 (3c)  SN: S5086 (20b)  SN: S5129 (30b)  SN: 3013	Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 217-00593) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06)	Scheduled Calibration  Apr-07  Apr-07  Apr-07  Aug-07  Apr-07  Aug-07  Jan-07		
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4	TE critical for calibration)  ID #  GB41293874  MY41495277  MY41498087  SN: S5054 (3c)  SN: S5086 (20b)  SN: S5129 (30b)  SN: 3013  SN: 654	Cal Date (Calibrated by, Certificate No.)  5-Apr-06 (METAS, No. 251-00557)  5-Apr-06 (METAS, No. 251-00557)  5-Apr-06 (METAS, No. 251-00557)  10-Aug-06 (METAS, No. 217-00592)  4-Apr-06 (METAS, No. 217-00598)  10-Aug-06 (METAS, No. 217-00593)  2-Jan-06 (SPEAG, No. ES3-3013_Jan06)  21-Jun-06 (SPEAG, No. DAE4-654_Jun06)	Scheduled Calibration Apr-07 Apr-07 Apr-07 Aug-07 Apr-07 Aug-07 Jan-07 Jun-07		
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	TE critical for calibration)  ID #  GB41293874  MY41495277  MY41498087  SN: S5054 (3c)  SN: S5086 (20b)  SN: S5129 (30b)  SN: 3013  SN: 654	Cal Date (Calibrated by, Certificate No.)  5-Apr-06 (METAS, No. 251-00557)  5-Apr-06 (METAS, No. 251-00557)  5-Apr-06 (METAS, No. 251-00557)  10-Aug-06 (METAS, No. 217-00592)  4-Apr-06 (METAS, No. 217-00598)  10-Aug-06 (METAS, No. 217-00593)  2-Jan-06 (SPEAG, No. ES3-3013_Jan06)  21-Jun-06 (SPEAG, No. DAE4-654_Jun06)  Check Date (in house)	Scheduled Calibration  Apr-07  Apr-07  Apr-07  Aug-07  Aug-07  Jan-07  Jun-07  Scheduled Check		
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	TE critical for calibration)  ID #  GB41293874  MY41495277  MY41498087  SN: S5054 (3c)  SN: S5086 (20b)  SN: S5129 (30b)  SN: 3013  SN: 654  ID #  US3642U01700 US37390585  Name	Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 217-00598) 10-Aug-06 (METAS, No. 217-00593) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06) 21-Jun-06 (SPEAG, No. DAE4-654_Jun06) Check Date (in house) 4-Aug-99 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05)	Scheduled Calibration  Apr-07 Apr-07 Apr-07 Aug-07 Apr-07 Aug-07 Jan-07 Jun-07 Scheduled Check In house check: Nov-07		
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ID #  GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 654  ID #  US3642U01700 US37390585	Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557) 10-Aug-06 (METAS, No. 217-00592) 4-Apr-06 (METAS, No. 217-00598) 10-Aug-06 (METAS, No. 217-00593) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06) 21-Jun-06 (SPEAG, No. DAE4-654_Jun06) Check Date (in house) 4-Aug-99 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05)	Scheduled Calibration  Apr-07  Apr-07  Aug-07  Aug-07  Aug-07  Jan-07  Jun-07  Scheduled Check  In house check: Nov-07  In house check: Nov 06		

Certificate No: ET3-1791\_Sep06

Page 1 of 9

### Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL NORMx,y,z tissue simulating liquid sensitivity in free space

ConF

sensitivity in TSL / NORMx,y,z

Polarization φ

diode compression point φ rotation around probe axis

Polarization 9

9 rotation around an axis that is in the plane normal to probe axis (at

measurement center), i.e., 9 = 0 is normal to probe axis

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001

### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This
  linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of
  the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ET3-1791\_Sep06

Page 2 of 9

ET3DV6 SN:1791

September 19, 2006

# Probe ET3DV6

SN:1791

Manufactured:

May 28, 2003

Last calibrated: Recalibrated:

November 26, 2004 September 19, 2006

ocptember 10,

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: ET3-1791\_Sep06

Page 3 of 9

ET3DV6 SN:1791

September 19, 2006

### DASY - Parameters of Probe: ET3DV6 SN:1791

Sensitivity in Free	Diode Compression <sup>B</sup>			
NormX	1.72 ± 10.1%	$\mu V/(V/m)^2$	DCP X	96 mV
NormY	1.67 ± 10.1%	$\mu V/(V/m)^2$	DCP Y	96 mV
NormZ	1.78 ± 10.1%	$\mu V/(V/m)^2$	DCP Z	94 mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

### **Boundary Effect**

TSL 900 MHz Typical SAR gradient: 5 % per mm

Sensor Cente	er to Phantom Surface Distance	3.7 mm	4.7 mm	
SAR <sub>be</sub> [%]	Without Correction Algorithm	8.3	4.4	
SAR <sub>be</sub> [%]	With Correction Algorithm	0.1	0.2	

TSL 1750 MHz Typical SAR gradient: 10 % per mm

Sensor Cente	er to Phantom Surface Distance	3.7 mm	4.7 mm	
SAR <sub>be</sub> [%]	Without Correction Algorithm	11.5	6.5	
SAR <sub>be</sub> [%]	With Correction Algorithm	0.2	0.3	

### Sensor Offset

Probe Tip to Sensor Center 2.7 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: ET3-1791\_Sep06

A The uncertainties of NormX,Y,Z do not affect the E2-field uncertainty inside TSL (see Page 8).


<sup>&</sup>lt;sup>B</sup> Numerical linearization parameter: uncertainty not required.

ET3DV6 SN:1791

September 19, 2006

# Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

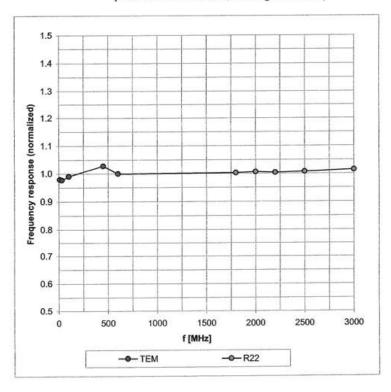

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Certificate No: ET3-1791\_Sep06


Page 5 of 9


### ET3DV6 SN:1791

### September 19, 2006

# Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

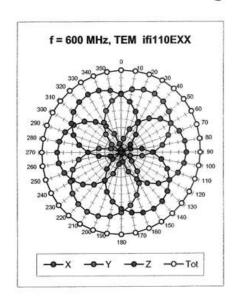



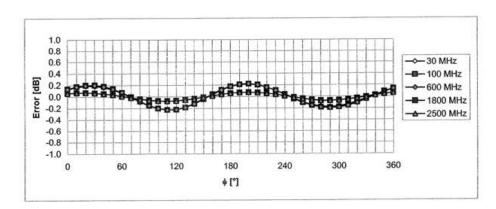

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: ET3-1791\_Sep06


Page 6 of 9

### ET3DV6 SN:1791

### September 19, 2006

# Dynamic Range f(SAR<sub>head</sub>)

(Waveguide R22, f = 1800 MHz)

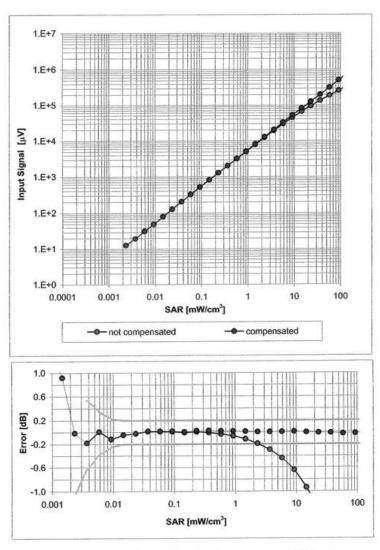

Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: ET3-1791\_Sep06


Page 7 of 9


Report No.: 07-09-MAS-015-03 FCC ID: U23MD6430H

### ET3DV6 SN:1791

### September 19, 2006

### **Conversion Factor Assessment**

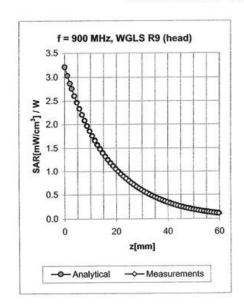



f [MHz]	Validity [MHz] <sup>c</sup>	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.55	1.87	6.60 ± 11.0% (k=2)
1750	± 50 / ± 100	Head	40.1 ± 5%	1.37 ± 5%	0.52	2.54	5.29 ± 11.0% (k=2)
1950	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.50	2.89	5.00 ± 11.0% (k=2)
2450	± 50 / ± 100	Head	39.2 ± 5%	1.80 ± 5%	0.69	1.96	4.62 ± 11.8% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.47	2.15	6.30 ± 11.0% (k=2)
1750	± 50 / ± 100	Body	53.4 ± 5%	1.49 ± 5%	0.59	2.89	4.76 ± 11.0% (k=2)
1950	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.65	2.73	4.50 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.60	1.69	4.16 ± 11.8% (k=2)

Certificate No: ET3-1791\_Sep06

Page 8 of 9


<sup>&</sup>lt;sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

ET3DV6 SN:1791

September 19, 2006

# **Deviation from Isotropy in HSL**

Error (\$\phi\$, \$9), f = 900 MHz

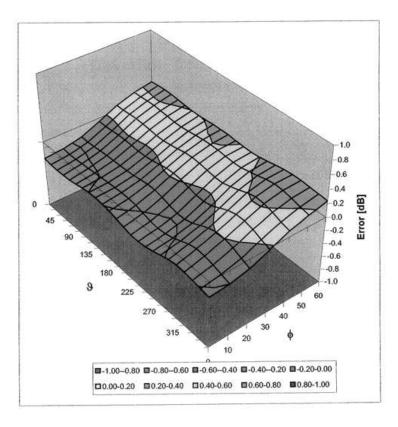

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ET3-1791\_Sep06

Page 9 of 9