

**Test of: Panasonic Mobile Comms Dev of Europe Ltd.  
VS70A**

**To: OET Bulletin 65 Supplement C: (2001-01)**

---

## **Appendix 1. Test Equipment Used**

RFI No.	Instrument	Manufacturer	Type No.	Serial No.	Date Last Calibrated	Cal. Interval
A034	Narda 20W Termination	Narda	374BNM	8706	Calibrated as part of system	-
A1094	Sony MVC FD-81	Sony	MVC - FD81	125805	Not Applicable	-
A1097	SMA Directional Coupler	MiDISCO	MDC6223-30	None	Calibrated as part of system	-
A1137	3dB Attenuator	Narda	779	04690	Calibrated as part of system	-
A1174	Dielectric Probe Kit	Agilent Technologies	85070C	Us99360072	Calibrated before use	-
A1182	Handset Positioner	Schmid & Partners	V3.0	None	Not Applicable	-
A1184	Data Acquisition Electronics	Schmid & Partners	DAE3	394	19 May 2006	12
A1185	E-Field Probe	Schmid & Partners	ET3 DV6	1528	12 July 2006	12
A1237	1900 MHz Validation Dipole	Schmid & Partners	D1900v2	540	14 June 2005	24
A1238	SAM Phantom	Schmid & Partners	001	001	Calibrated before use	-
A1328	Dasy 4 Handset Positioner	Schmid & Partners	Modification	SD 000 H01 DA	Calibrated before use	-
A1497	Mini-Circuits	Mini-Circuits	zhl-42w (sma)	e020105	Calibrated as part of system	-
A1531	Hyper LOG 7025	AARONIA AG	7025	02458	Not Applicable	-
A1566	SAM Phantom	SPEAG	002	002	Not Applicable	-
A215	20 dB Attenuator	Narda	766-20	9402	Calibrated as part of system	-
C1092	Cable	RS	293-334	1087200-3 3402	Calibrated as part of system	-
C1144	Cable	Rosenberger MICRO-COAX	FA147AF001 503030	41842-1	Calibrated as part of system	-
C1145	Cable	Rosenberger MICRO-COAX	FA147AF003 003030	41843-1	Calibrated as part of system	-
C1146	Cable	Rosenberger MICRO-COAX	FA147AF030 003030	41752-1	Calibrated as part of system	-
G051	Signal Generator	Gigatronics	7100/.01-20	749472	01 November 2005	12

**Test of: Panasonic Mobile Comms Dev of Europe Ltd.  
VS70A**

**To: OET Bulletin 65 Supplement C: (2001-01)**

---

**Test Equipment Used (Continued)**

RFI No.	Instrument	Manufacturer	Type No.	Serial No.	Date Last Calibrated	Cal. Interval
G0528	Robot Power Supply	Schmid & Partner	DASY	None	Calibrated before Use	12
G087	PSU	Thurlby Thandar	CPX200	100701	Not Applicable	-
M010	NRV Power Meter	Rohde & Schwarz	NRV	882 317/065	19 June 2006	12
M1015	Network Analyser	Agilent Technologies	8753ES	US39172406	19 September 2006	12
M1047	Robot Arm	Staubli	RX908 L	F00/SD89A1/A/01	Calibrated before use	-
M1069	Diode Power Sensor	Rohde & Schwarz	NRV-Z2	838824/010	05 April 2006	12
M1129	URY-Z2	Rohde & Schwarz	URY-Z2	890242/16	Calibrated as part of system	-
M1150	Compact Data Logger with Interface	Testo	175-T2	37503417 / 301	Not Applicable	-
M136	Temperature/Humidity/Pressure Meter	RS Components	None	None	Internal Calibration	-
M509	Thermometer	Testo	110	4037880043 3	20 March 2006	12 months
S256	SAR Laboratory	RFI	-	-	Calibration before use	-

**NB** In accordance with UKAS requirements, all the measurement equipment is on a calibration schedule.

Test of: **Panasonic Mobile Comms Dev of Europe Ltd.**  
**VS70A**

To: **OET Bulletin 65 Supplement C: (2001-01)**

---

**A.1.1. Calibration Certificates**

This section contains the calibration certificates and data for the Probe(s) and Dipole(s) used, which are not included in the total number of pages for this report.

A1185  
B.Möldli  
19/07/06

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client

RFI

Certificate No: ET3-1528\_Jul06

## CALIBRATION CERTIFICATE

Object ET3DV6 - SN:1528

Calibration procedure(s)  
QA CAL-01.v5 and QA CAL-12.v4  
Calibration procedure for dosimetric E-field probes

Calibration date: July 12, 2006

Condition of the calibrated item In Tolerance

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	5-Apr-06 (METAS, No. 251-00557)	Apr-07
Power sensor E4412A	MY41495277	5-Apr-06 (METAS, No. 251-00557)	Apr-07
Power sensor E4412A	MY41498087	5-Apr-06 (METAS, No. 251-00557)	Apr-07
Reference 3 dB Attenuator	SN: S5054 (3c)	11-Aug-05 (METAS, No. 251-00499)	Aug-06
Reference 20 dB Attenuator	SN: S5086 (20b)	4-Apr-06 (METAS, No. 251-00558)	Apr-07
Reference 30 dB Attenuator	SN: S5129 (30b)	11-Aug-05 (METAS, No. 251-00500)	Aug-06
Reference Probe ES3DV2	SN: 3013	2-Jan-06 (SPEAG, No. ES3-3013_Jan06)	Jan-07
DAE4	SN: 654	21-Jun-06 (SPEAG, No. DAE4-654_Jun06)	Jun-07

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check Nov-05)	In house check: Nov-07
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-05)	In house check: Nov 06

Calibrated by:	Name	Function	Signature
	Katja Pokovic	Technical Manager	

Approved by:	Name	Function	Signature
	Niels Kuster	Quality Manager	

Issued: July 12, 2006

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Federal Office of Metrology and Accreditation  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

### **Glossary:**

TSL	tissue simulating liquid
NORM $x,y,z$	sensitivity in free space
ConF	sensitivity in TSL / NORM $x,y,z$
DCP	diode compression point
Polarization $\phi$	$\phi$ rotation around probe axis
Polarization $\vartheta$	$\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis

### **Calibration is Performed According to the Following Standards:**

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz)", July 2001

### **Methods Applied and Interpretation of Parameters:**

- $NORMx,y,z$ : Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide).  $NORMx,y,z$  are only intermediate values, i.e., the uncertainties of  $NORMx,y,z$  does not effect the  $E^2$ -field uncertainty inside TSL (see below *ConvF*).
- $NORM(f)x,y,z = NORMx,y,z * frequency\_response$  (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- $DCPx,y,z$ : DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters*: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to  $NORMx,y,z * ConvF$  whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)*: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

# Probe ET3DV6

## SN:1528

Manufactured:	March 21, 2000
Last calibrated:	July 13, 2005
Recalibrated:	July 12, 2006

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

## DASY - Parameters of Probe: ET3DV6 SN:1528

Sensitivity in Free Space <sup>A</sup>			Diode Compression <sup>B</sup>	
NormX	<b>1.53</b> $\pm$ 10.1%	$\mu\text{V}/(\text{V}/\text{m})^2$	DCP X	91 mV
NormY	<b>1.83</b> $\pm$ 10.1%	$\mu\text{V}/(\text{V}/\text{m})^2$	DCP Y	94 mV
NormZ	<b>1.57</b> $\pm$ 10.1%	$\mu\text{V}/(\text{V}/\text{m})^2$	DCP Z	101 mV

### Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

### Boundary Effect

TSL                    900 MHz                    Typical SAR gradient: 5 % per mm

Sensor Center to Phantom Surface Distance	3.7 mm	4.7 mm
SAR <sub>be</sub> [%]      Without Correction Algorithm	8.9	4.7
SAR <sub>be</sub> [%]      With Correction Algorithm	0.1	0.2

TSL                    1750 MHz                    Typical SAR gradient: 10 % per mm

Sensor Center to Phantom Surface Distance	3.7 mm	4.7 mm
SAR <sub>be</sub> [%]      Without Correction Algorithm	10.1	5.9
SAR <sub>be</sub> [%]      With Correction Algorithm	0.3	0.6

### Sensor Offset

Probe Tip to Sensor Center                    2.7 mm


The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the  $E^2$ -field uncertainty inside TSL (see Page 8).




<sup>B</sup> Numerical linearization parameter: uncertainty not required.

## Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

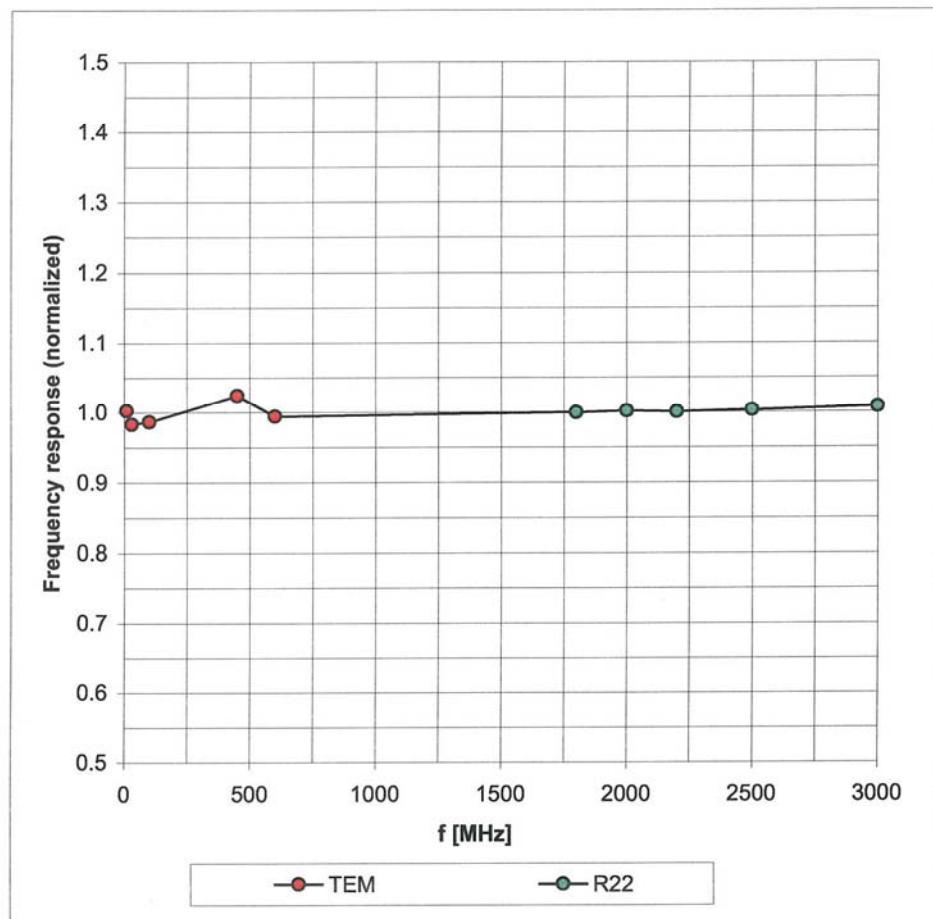


Uncertainty of Frequency Response of E-field:  $\pm 6.3\% (k=2)$

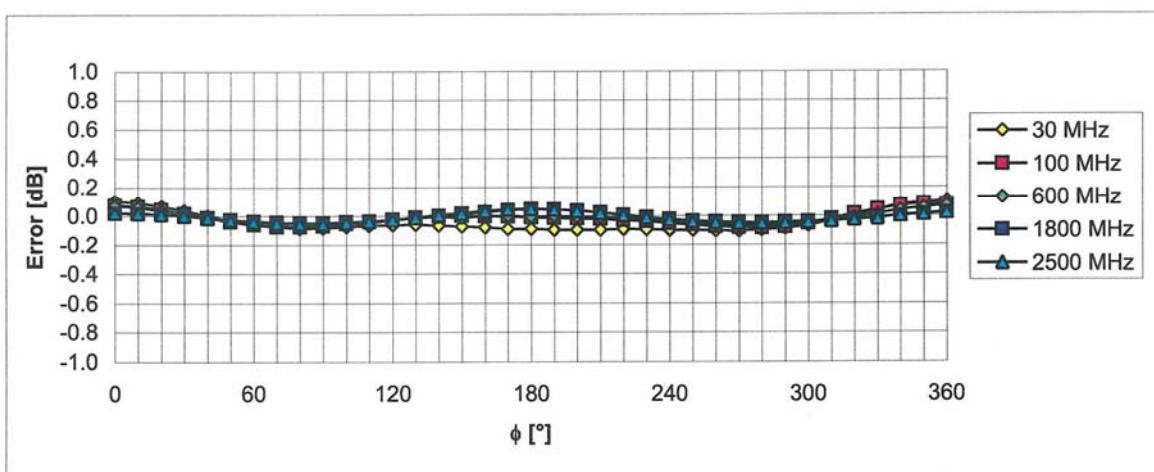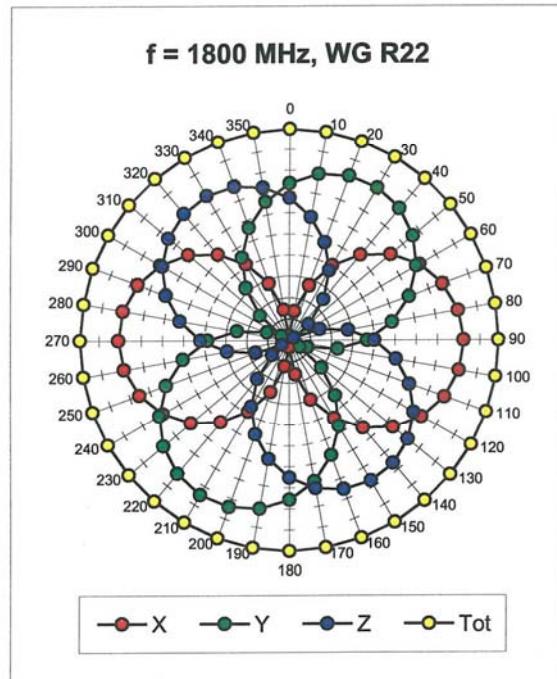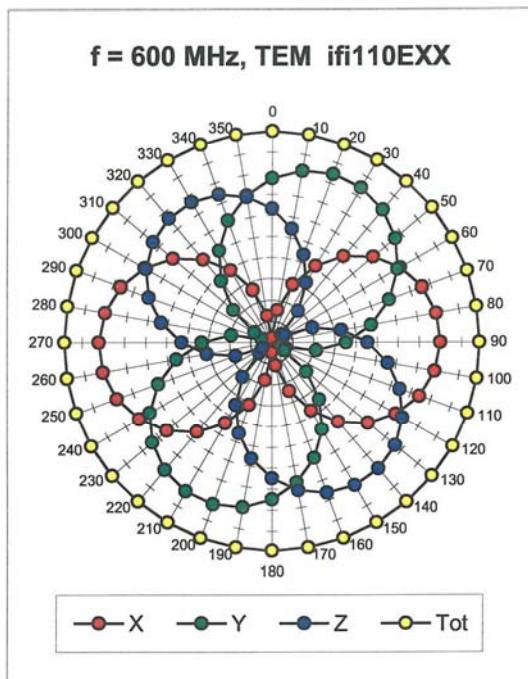Receiving Pattern ( $\phi$ ),  $\vartheta = 0^\circ$ Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  (k=2)


### Dynamic Range f(SAR<sub>head</sub>)

(Waveguide R22, f = 1800 MHz)

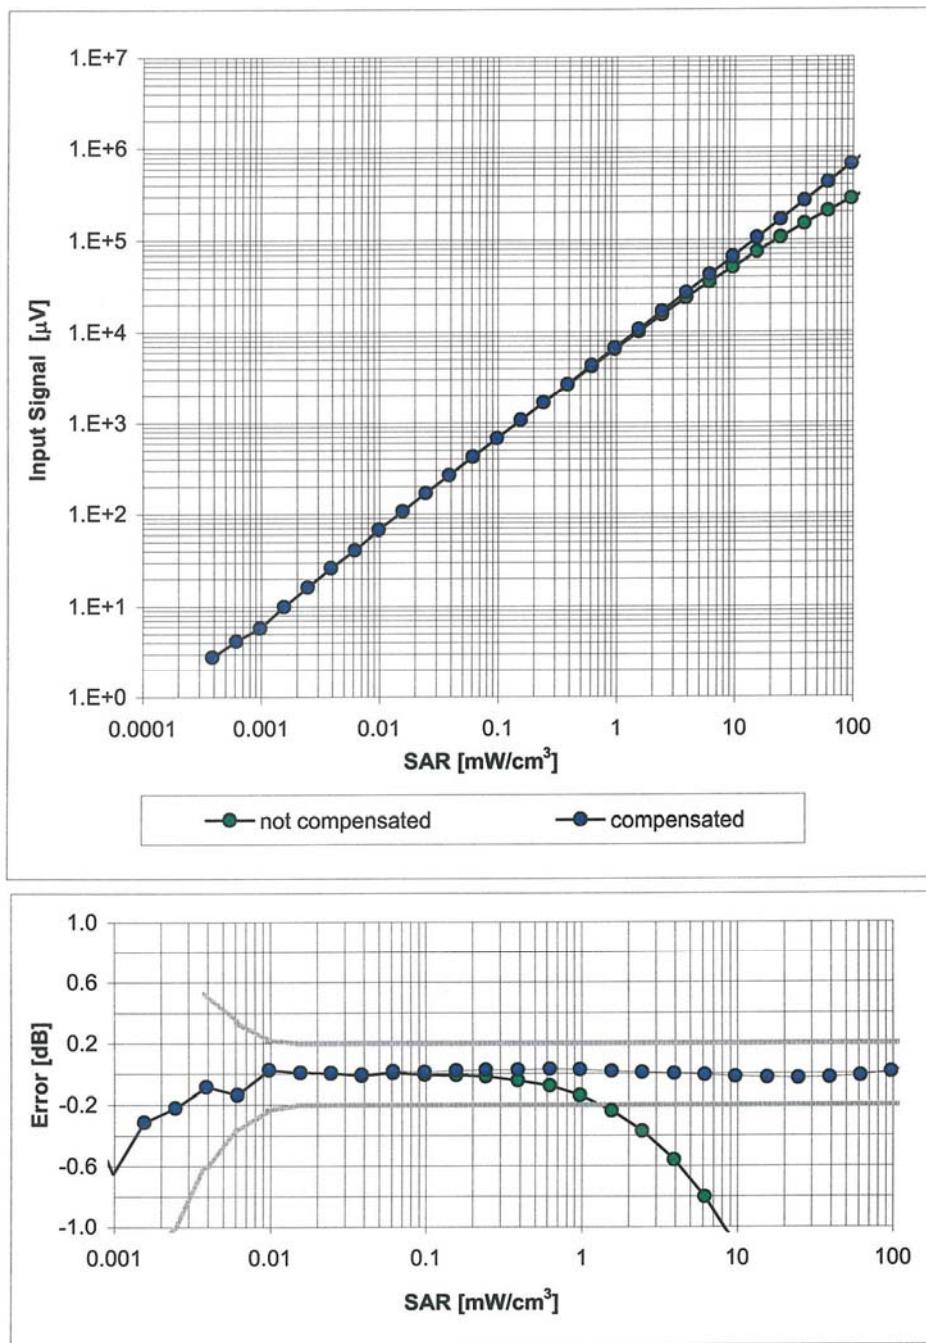

Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )

## Conversion Factor Assessment

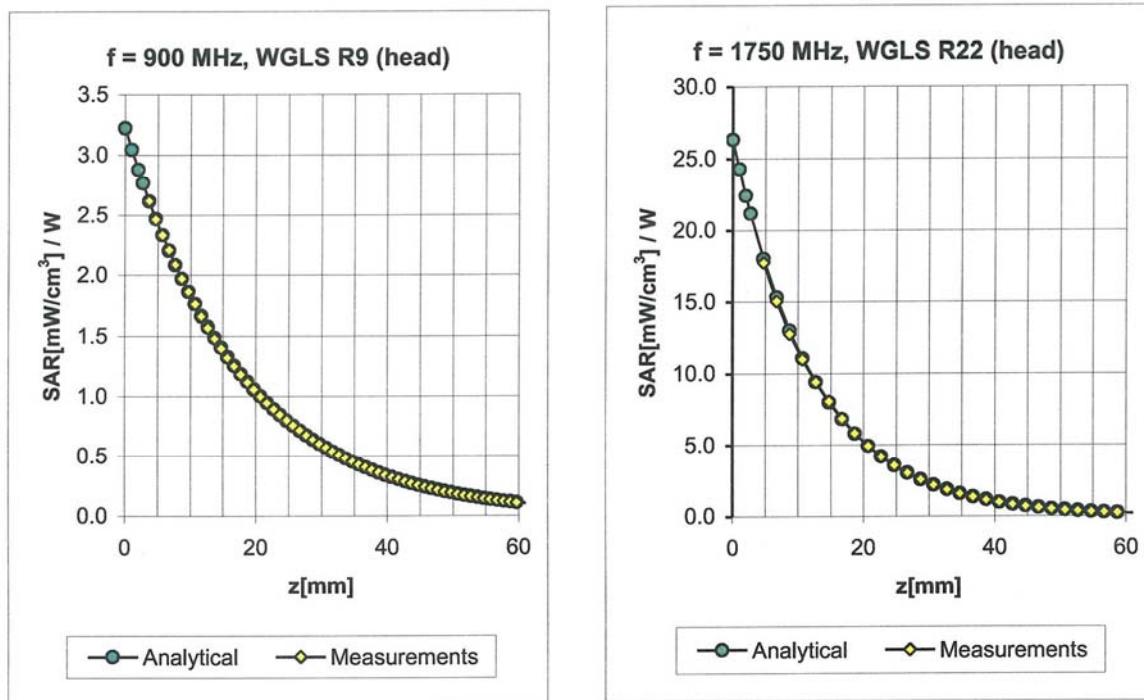


f [MHz]	Validity [MHz] <sup>c</sup>	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF	Uncertainty
450	± 50 / ± 100	Head	43.5 ± 5%	0.87 ± 5%	0.38	1.92	7.16	± 13.3% (k=2)
835	± 50 / ± 100	Head	41.5 ± 5%	0.90 ± 5%	0.64	1.78	6.44	± 11.0% (k=2)
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.63	1.81	6.28	± 11.0% (k=2)
1750	± 50 / ± 100	Head	40.1 ± 5%	1.37 ± 5%	0.60	2.36	5.30	± 11.0% (k=2)
1900	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.60	2.43	5.09	± 11.0% (k=2)
2450	± 50 / ± 100	Head	39.2 ± 5%	1.80 ± 5%	0.98	1.57	4.59	± 11.8% (k=2)
450	± 50 / ± 100	Body	56.7 ± 5%	0.94 ± 5%	0.32	1.96	7.72	± 13.3% (k=2)
835	± 50 / ± 100	Body	55.2 ± 5%	0.97 ± 5%	0.58	1.93	6.29	± 11.0% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.53	2.06	6.08	± 11.0% (k=2)
1750	± 50 / ± 100	Body	53.4 ± 5%	1.49 ± 5%	0.80	2.25	4.65	± 11.0% (k=2)
1900	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.70	2.37	4.55	± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.80	1.90	4.27	± 11.8% (k=2)

<sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

## Deviation from Isotropy in HSL

Error ( $\phi, \theta$ ),  $f = 900$  MHz

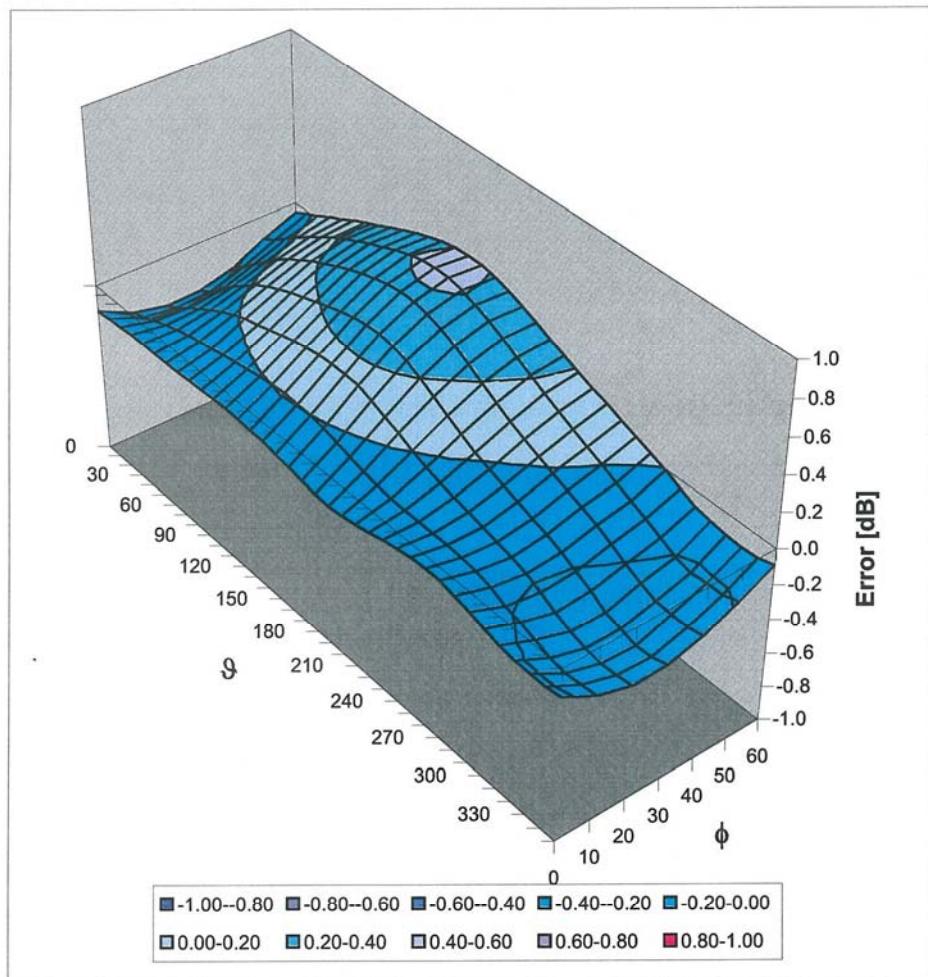

Uncertainty of Spherical Isotropy Assessment:  $\pm 2.6\%$  ( $k=2$ )