#### Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client

Auden

Certificate No: D2450V2-735\_Mar06

Accreditation No.: SCS 108

### **CALIBRATION CERTIFICATE**

Object D2450V2 - SN: 735

Calibration procedure(s) QA CAL-05.v6

Calibration procedure for dipole validation kits

Calibration date: March 6, 2006

Condition of the calibrated item In Tolerance

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	04-Oct-05 (METAS, No. 251-00516)	Oct-06
Power sensor HP 8481A	US37292783	04-Oct-05 (METAS, No. 251-00516)	Oct-06
Reference 20 dB Attenuator	SN: 5086 (20g)	11-Aug-05 (METAS, No 251-00498)	Aug-06
Reference 10 dB Attenuator	SN: 5047.2 (10r)	11-Aug-05 (METAS, No 251-00498)	Aug-06
Reference Probe ES3DV2	SN 3025	28-Oct-05 (SPEAG, No. ES3-3025_Oct05)	Oct-06
DAE4	SN 601	15-Dec-05 (SPEAG, No. DAE4-601_Dec05)	Dec-06
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (SPEAG, in house check Oct-05)	In house check: Oct-07
RF generator Agilent E4421B	MY41000675	11-May-05 (SPEAG, in house check Nov-05)	In house check: Nov-07
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (SPEAG, in house check Nov-05)	In house check: Nov-06
	Name	Function	Signature
Calibrated by:	Marcel Fehr	Laboratory Technician	M. Tiller
Approved by:	Katja Pokovic	Technical Manager	De Kil

Issued: March 7, 2006

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

#### Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### Additional Documentation:

d) DASY4 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Area Scan resolution	dx, dy = 15 mm	
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.5 ± 6 %	1.79 mho/m ± 6 %
Head TSL temperature during test	(21.6 ± 0.2) °C		

#### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	condition	
SAR measured	250 mW input power	13.8 mW / g
SAR normalized	normalized to 1W	55.2 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	54.8 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.39 mW / g
SAR normalized	normalized to 1W	25.6 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	25.4 mW / g ± 16.5 % (k=2)

Certificate No: D2450V2-735\_Mar06

<sup>&</sup>lt;sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.7 ± 6 %	1.97 mho/m ± 6 %
Body TSL temperature during test	(21.8 ± 0.2) °C	*****	

### SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.7 mW / g
SAR normalized	normalized to 1W	54.8 mW / g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	55.1 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	6.32 mW / g
SAR normalized	normalized to 1W	25.3 mW / g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	25.4 mW / g ± 16.5 % (k=2)

Certificate No: D2450V2-735\_Mar06

<sup>&</sup>lt;sup>2</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

#### **Appendix**

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.0 Ω + 2.6 jΩ	
Return Loss	-29.9 dB	

#### **Antenna Parameters with Body TSL**

Impedance, transformed to feed point	$48.6 \Omega + 4.5 j\Omega$
Return Loss	- 26.3 dB

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.154 ns	
----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	May 7, 2003

#### **DASY4 Validation Report for Head TSL**

Date/Time: 06.03.2006 15:48:10

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN735

Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U10 BB;

Medium parameters used: f = 2450 MHz;  $\sigma = 1.79 \text{ mho/m}$ ;  $\epsilon_r = 38.5$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

#### DASY4 Configuration:

Probe: ES3DV2 - SN3025 (HF); ConvF(4.4, 4.4, 4.4); Calibrated: 28.10.2005

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 15.12.2005

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA;;

Measurement SW: DASY4, V4.7 Build 12; Postprocessing SW: SEMCAD, V1.8 Build 165

Pin = 250 mW; d = 10 mm/Area Scan (71x71x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 16.9 mW/g


Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 93.6 V/m; Power Drift = -0.018 dB

Peak SAR (extrapolated) = 28.8 W/kg


SAR(1 g) = 13.8 mW/g; SAR(10 g) = 6.39 mW/g

Maximum value of SAR (measured) = 15.7 mW/g

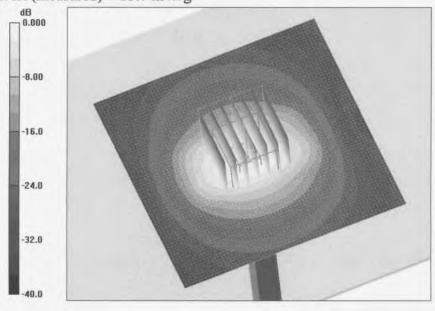

0 dB = 15.7 mW/g

#### Impedance Measurement Plot for Head TSL

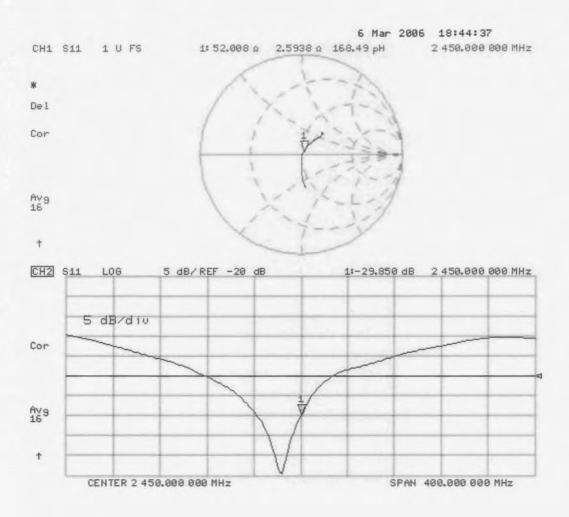

#### **DASY4 Validation Report for Body TSL**

Date/Time: 06.03.2006 12:07:30

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN735

Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL U10;

Medium parameters used: f = 2450 MHz;  $\sigma = 1.97 \text{ mho/m}$ ;  $\epsilon_r = 53.7$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

#### DASY4 Configuration:

Probe: ES3DV2 - SN3025 (HF); ConvF(4.06, 4.06, 4.06); Calibrated: 28.10.2005

Sensor-Surface: 4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 15.12.2005

Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA;;

Measurement SW: DASY4, V4.7 Build 16; Postprocessing SW: SEMCAD, V1.8 Build 165

Pin = 250 mW; d = 10 mm/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 16.2 mW/g


Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 88.4 V/m; Power Drift = -0.120 dB

Peak SAR (extrapolated) = 29.0 W/kg


SAR(1 g) = 13.7 mW/g; SAR(10 g) = 6.32 mW/g

Maximum value of SAR (measured) = 15.4 mW/g

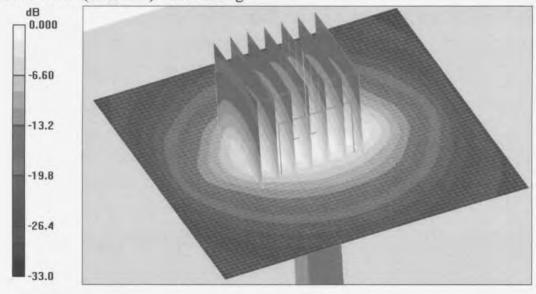

0 dB = 15.4 mW/g

### Impedance Measurement Plot for Body TSL

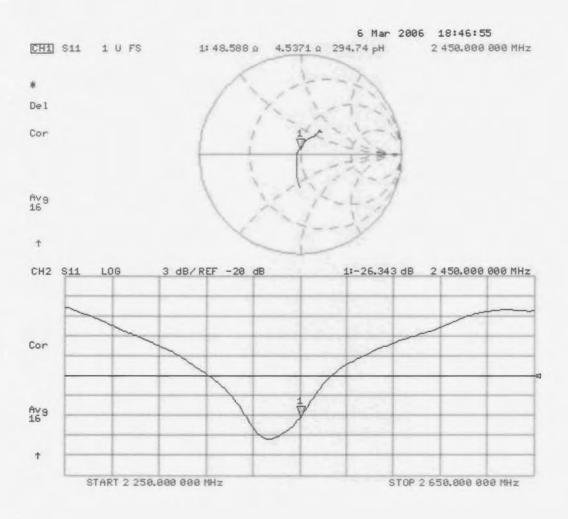

#### Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service sulsse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client

ATL (Auden)

Certificate No: ET3-1531\_Jan06

Object	ET3DV6 - SN:15	31	
Calibration procedure(s)		nd QA CAL-12.v4 edure for dosimetric E-field probes	
Calibration date:	January 21, 200	6	
Condition of the calibrated item	In Tolerance	STATE OF THE PARTY	
All calibrations have been condu			
Calibration Equipment used (M&		Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Calibration Equipment used (M&	TE critical for calibration)	Cal Date (Calibrated by, Certificate No.) 3-May-05 (METAS, No. 251-00466)	Scheduled Calibration May-06
Calibration Equipment used (M& Primary Standards Power meter E4419B	TE critical for calibration)	Cal Date (Calibrated by, Certificate No.)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)	Scheduled Calibration May-06 May-06
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A	TE critical for calibration)  ID #  GB41293874	Cal Date (Calibrated by, Certificate No.)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)	Scheduled Calibration May-06 May-06 May-06
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A	TE critical for calibration)  ID #  GB41293874  MY41495277	Cal Date (Calibrated by, Certificate No.)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00499)	Scheduled Calibration May-06 May-06 May-06 Aug-06
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator	TE critical for calibration)  ID #  GB41293874  MY41495277  MY41498087  SN: S5054 (3c)  SN: S5086 (20b)	Cal Date (Calibrated by, Certificate No.)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)  11-Aug-05 (METAS, No. 251-00499)  3-May-05 (METAS, No. 251-00467)	Scheduled Calibration May-06 May-06 May-06 Aug-06 May-06
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator	TE critical for calibration)  ID #  GB41293874  MY41495277  MY41498087  SN: S5054 (3c)  SN: S5086 (20b)  SN: S5129 (30b)	Cal Date (Calibrated by, Certificate No.)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)  11-Aug-05 (METAS, No. 251-00499)  3-May-05 (METAS, No. 251-00467)  11-Aug-05 (METAS, No. 251-00500)	Scheduled Calibration May-06 May-06 May-06 Aug-06 May-06 Aug-06 Aug-06
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2	TE critical for calibration)  ID #  GB41293874  MY41495277  MY41498087  SN: S5054 (3c)  SN: S5086 (20b)	Cal Date (Calibrated by, Certificate No.)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)  11-Aug-05 (METAS, No. 251-00499)  3-May-05 (METAS, No. 251-00467)	Scheduled Calibration May-06 May-06 May-06 Aug-06 May-06
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	TE critical for calibration)  ID #  GB41293874  MY41495277  MY41498087  SN: S5054 (3c)  SN: S5086 (20b)  SN: S5129 (30b)  SN: 3013	Cal Date (Calibrated by, Certificate No.)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)  11-Aug-05 (METAS, No. 251-00499)  3-May-05 (METAS, No. 251-00497)  11-Aug-05 (METAS, No. 251-00467)  11-Aug-05 (METAS, No. 251-00500)  2-Jan-06 (SPEAG, No. ES3-3013_Jan06)  27-Oct-05 (SPEAG, No. DAE4-654_Oct05)  Check Date (in house)	Scheduled Calibration May-06 May-06 May-06 Aug-06 May-06 Aug-06 Jan-07
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	TE critical for calibration)  ID #  GB41293874  MY41495277  MY41498087  SN: S5054 (3c)  SN: S5054 (20b)  SN: S5129 (30b)  SN: 3013  SN: 654	Cal Date (Calibrated by, Certificate No.)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)  11-Aug-05 (METAS, No. 251-00499)  3-May-05 (METAS, No. 251-00497)  11-Aug-05 (METAS, No. 251-00500)  2-Jan-06 (SPEAG, No. ES3-3013_Jan06)  27-Oct-05 (SPEAG, No. DAE4-654_Oct05)	Scheduled Calibration May-06 May-06 May-06 Aug-06 Aug-06 Jan-07 Oct-06 Scheduled Check In house check: Nov-07
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	TE critical for calibration)  ID #  GB41293874  MY41495277  MY41498087  SN: S5054 (3c)  SN: S5054 (20b)  SN: S5129 (30b)  SN: 3013  SN: 654	Cal Date (Calibrated by, Certificate No.)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)  11-Aug-05 (METAS, No. 251-00499)  3-May-05 (METAS, No. 251-00497)  11-Aug-05 (METAS, No. 251-00467)  11-Aug-05 (METAS, No. 251-00500)  2-Jan-06 (SPEAG, No. ES3-3013_Jan06)  27-Oct-05 (SPEAG, No. DAE4-654_Oct05)  Check Date (in house)	Scheduled Calibration May-06 May-06 May-06 Aug-06 Aug-06 Jan-07 Oct-06 Scheduled Check
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ID #  GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 654  ID #  US3642U01700	Cal Date (Calibrated by, Certificate No.)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)  11-Aug-05 (METAS, No. 251-00499)  3-May-05 (METAS, No. 251-00497)  11-Aug-05 (METAS, No. 251-00500)  2-Jan-06 (SPEAG, No. ES3-3013_Jan06)  27-Oct-05 (SPEAG, No. DAE4-654_Oct05)  Check Date (in house)  4-Aug-99 (SPEAG, in house check Nov-05)  18-Oct-01 (SPEAG, in house check Nov-05)	Scheduled Calibration May-06 May-06 May-06 Aug-06 Aug-06 Jan-07 Oct-06 Scheduled Check In house check: Nov-07 In house check: Nov 06
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37390585	Cal Date (Calibrated by, Certificate No.)  3-May-05 (METAS, No. 251-00466)  3-May-05 (METAS, No. 251-00466)  11-Aug-05 (METAS, No. 251-00499)  3-May-05 (METAS, No. 251-00497)  11-Aug-05 (METAS, No. 251-00500)  2-Jan-06 (SPEAG, No. ES3-3013_Jan06)  27-Oct-05 (SPEAG, No. DAE4-654_Oct05)  Check Date (in house)  4-Aug-99 (SPEAG, in house check Nov-05)  18-Oct-01 (SPEAG, in house check Nov-05)	Scheduled Calibration May-06 May-06 May-06 Aug-06 Aug-06 Jan-07 Oct-06 Scheduled Check In house check: Nov-07 In house check: Nov 06

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

#### Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL NORMx,y,z tissue simulating liquid sensitivity in free space

ConF

sensitivity in TSL / NORMx,y,z

DCP Polarization φ diode compression point o rotation around probe axis

Polarization 9

9 rotation around an axis that is in the plane normal to probe axis (at

measurement center), i.e., 9 = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

 a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003

 b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This
  linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of
  the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

January 21, 2006

# Probe ET3DV6

SN:1531

Manufactured:

July 15, 2000

Last calibrated:

November 19, 2004

Recalibrated:

January 21, 2006

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

ET3DV6 SN:1531

### DASY - Parameters of Probe: ET3DV6 SN:1531

Sensitivity in Free Space <sup>A</sup>	Diode Compression <sup>8</sup>

NormX	1.45 ± 10.1%	$\mu V/(V/m)^2$	DCP X	93 mV
NormY	1.50 ± 10.1%	$\mu V/(V/m)^2$	DCP Y	93 mV
NormZ	1.55 ± 10.1%	$\mu V/(V/m)^2$	DCP Z	93 mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

### **Boundary Effect**

TSL 900 MHz Typical SAR gradient: 5 % per mm

Sensor Center to Phantom Surface Distance		3.7 mm	4.7 mm
SAR <sub>be</sub> [%]	Without Correction Algorithm	9.6	5.2
SAR <sub>be</sub> [%]	With Correction Algorithm	0.0	0.3

TSL 1810 MHz Typical SAR gradient: 10 % per mm

Sensor Center to Phantom Surface Distance		3.7 mm	4.7 mm
SAR <sub>be</sub> [%]	Without Correction Algorithm	7.9	4.5
SAR <sub>be</sub> [%]	With Correction Algorithm	0.1	0.3

#### Sensor Offset

Probe Tip to Sensor Center 2.7 mm


The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>&</sup>lt;sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Page 8).

<sup>&</sup>lt;sup>n</sup> Numerical linearization parameter; uncertainty not required.


# Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

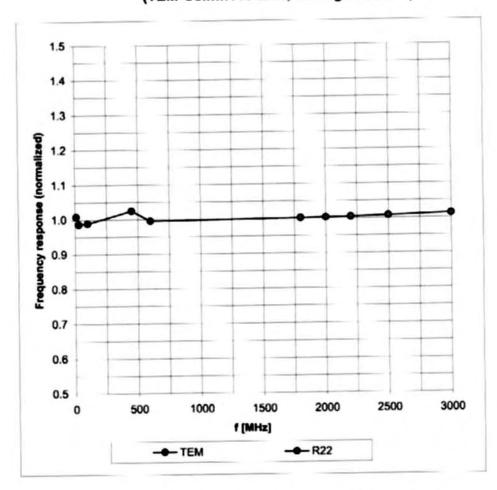


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Receiving Pattern ( $\phi$ ),  $\theta$  = 0°

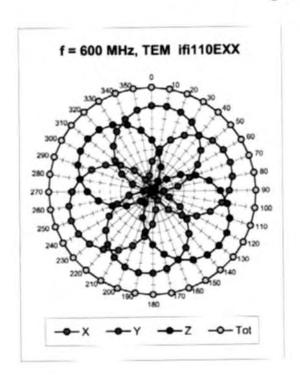

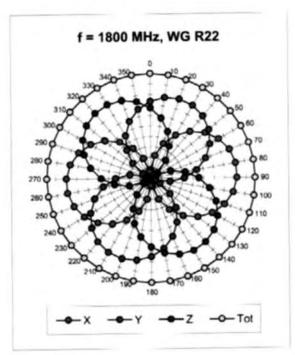


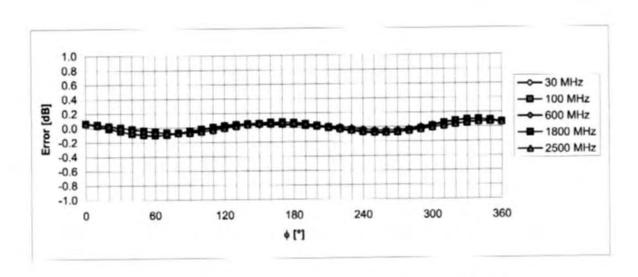

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


## Dynamic Range f(SAR<sub>head</sub>)


(Waveguide R22, f = 1800 MHz)

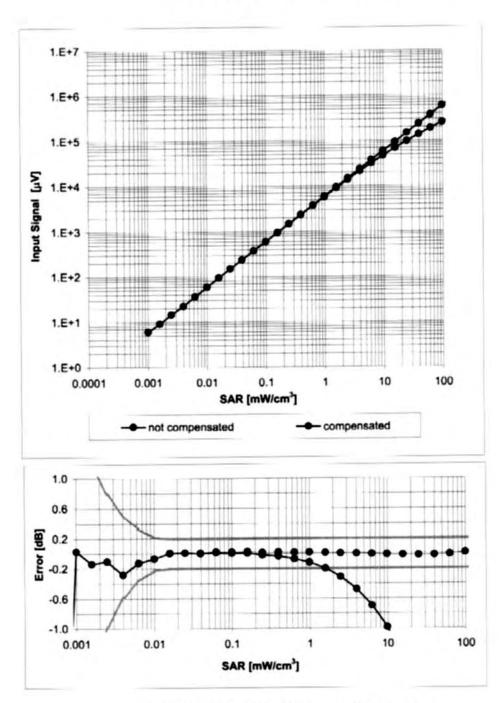

Uncertainty of Linearity Assessment: ± 0.6% (k=2)

### **Conversion Factor Assessment**

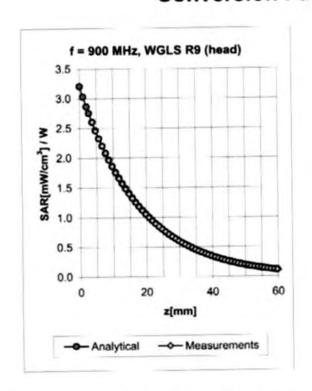

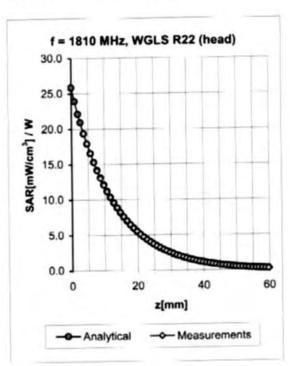


f [MHz]	Validity [MHz] <sup>c</sup>	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
450	±50/±100	Head	43.5 ± 5%	0.87 ± 5%	0.28	3.21	6.96 ± 13.3% (k=2)
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.59	1.93	6.18 ± 11.0% (k=2)
1810	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.62	1.72	5.09 ± 11.0% (k=2)
2000	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.75	1.52	4.87 ± 11.0% (k=2)
2450	± 50 / ± 100	Head	39.2 ± 5%	1.80 ± 5%	1.12	1.07	4.53 ± 11.8% (k=2)
450	±50/±100	Body	56.7 ± 5%	0.94 ± 5%	0.25	4.34	7.37 ± 13.3% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.54	2.08	5.96 ± 11.0% (k=2)
1810	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.66	2.10	4.62 ± 11.0% (k=2)
2000	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.55	2.39	4.36 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.92	1.25	4.24 ± 11.8% (k=2)

 $<sup>^{\</sup>rm C}$  The validity of  $\pm$  100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

### **Deviation from Isotropy in HSL**

Error (φ, θ), f = 900 MHz

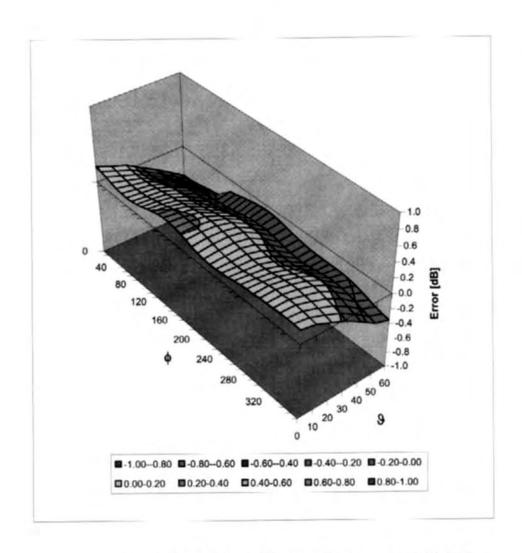

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Page 9 of 9

#### Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst s Service suisse d'étalonnage C Servizio svizzero di taratura **Swiss Calibration Service** 

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

ATL (Auden)

Certificate No: DAE3-541 Oct05

Accreditation No.: SCS 108

#### CALIBRATION CERTIFICATE

DAE3 - SD 000 D03 AA - SN: 541 Object

QA CAL-06.v12 Calibration procedure(s)

Calibration procedure for the data acquisition unit (DAE)

October 19, 2005 Calibration date:

In Tolerance Condition of the calibrated item

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Fluke Process Calibrator Type 5101B	SN: 5015004	29-Jun-05 (ELCAL AG, No. 366856)	Jun-06
	•		
Secondary Standards	ID#	Check Date (in house)	Scheduled Check

Signature Function Name Calibrated by:

Eric Hainfeld Technician

Fin Bomholt **R&D Director** Approved by:

Issued: October 19, 2005

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: DAE3-541\_Oct05

Page 1 of 5

#### Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

#### Glossary

DAE digital acquisition electronics

Connector angle information used in DASY system to align probe sensor X to the robot

coordinate system.

#### Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters contain technical information as a result from the performance test and require no uncertainty.
- DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
- Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
- Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
- AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
- Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
- Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
- Input resistance: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
- Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
- Power consumption: Typical value for information. Supply currents in various operating modes.

Certificate No: DAE3-541\_Oct05

#### **DC Voltage Measurement**

A/D - Converter Resolution nominal

High Range:  $1LSB = 6.1\mu V$ , full range = -100...+300 mVLow Range: 1LSB = 61nV, full range = -1......+3mVDASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	x	Y	Z
High Range	404.642 ± 0.1% (k=2)	404.495 ± 0.1% (k=2)	404.261 ± 0.1% (k=2)
Low Range	3.94353 ± 0.7% (k=2)	3.92284 ± 0.7% (k=2)	3.97962 ± 0.7% (k=2)

#### **Connector Angle**

Connector Angle to be used in DASY system	296°±1°

Certificate No: DAE3-541\_Oct05 Page 3 of 5

#### **Appendix**

1. DC Voltage Linearity

High Range	Input (μV)	Reading (μV)	Error (%)
Channel X + Input	200000	200000.1	0.00
Channel X + Input	20000	19997.48	-0.01
Channel X - Input	20000	-19993.89	-0.03
Channel Y + Input	200000	199999.8	0.00
Channel Y + Input	20000	19997.74	-0.01
Channel Y - Input	20000	-19999.40	0.00
Channel Z + Input	200000	199999.8	0.00
Channel Z + Input	20000	19998.41	-0.01
Channel Z - Input	20000	-19995.29	-0.02

Low Range	Input (μV)	Reading (μV)	Error (%)
Channel X + Input	2000	2000.1	0.00
Channel X + Input	200	200.04	0.02
Channel X - Input	200	-200.61	0.31
Channel Y + Input	2000	1999.9	0.00
Channel Y + Input	200	199.54	-0.23
Channel Y - Input	200	-200.69	0.34
Channel Z + Input	2000	2000.1	0.00
Channel Z + Input	200	199.37	-0.31
Channel Z - Input	200	-201.15	0.58

#### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	9.34	9.40
	- 200	-7.67	-9.88
Channel Y	200	1.02	0.66
	- 200	-1.89	-2.08
Channel Z	200	-0.11	-0.17
	- 200	-1.33	-1.65

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200		2.26	0.18
Channel Y	200	1.20		4.48
Channel Z	200	-1.38	0.92	-

Certificate No: DAE3-541\_Oct05 Page 4 of 5

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15928	16316
Channel Y	15735	16280
Channel Z	15946	16327

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MΩ

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	0.04	-2.40	1.47	0.36
Channel Y	-0.51	-1.88	1.37	0.39
Channel Z	-0.58	-1.37	0.18	0.25

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance

	Zeroing (MOhm)	Measuring (MOhm)
Channel X	0.2000	199.3
Channel Y	0.2001	202.6
Channel Z	0.2001	202.8

8. Low Battery Alarm Voltage (verified during pre test)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

9. Power Consumption (verified during pre test)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.0	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE3-541\_Oct05 Page 5 of 5