


Test Set Up Photos

| | |
|---|--|
|  A photograph showing a white foot pedal with two踏板 on a light-colored wooden table. The background is a dark, textured anechoic chamber wall. |  A photograph of an iTero dental scanner cart. The monitor displays the CADENT iTero logo. The cart is connected to a white computer system with a keyboard and mouse. |
| Foot pedal. Radiated emissions test setup at 1m distance. | iTero cart with USB dongle. Radiated emissions test setup at 1m distance. |
|  A photograph of the same white foot pedal setup on a light-colored wooden table, but in an outdoor field with dry grass and trees in the background. A green tripod-mounted antenna is positioned above the table. |  A photograph of the iTero cart setup on the same outdoor OATS. The monitor is visible, and the green antenna is mounted on a tall white pole above the cart. |
| Foot pedal. Radiated emissions test setup on OATS. | iTero cart with USB dongle. Radiated emissions test setup on OATS. |

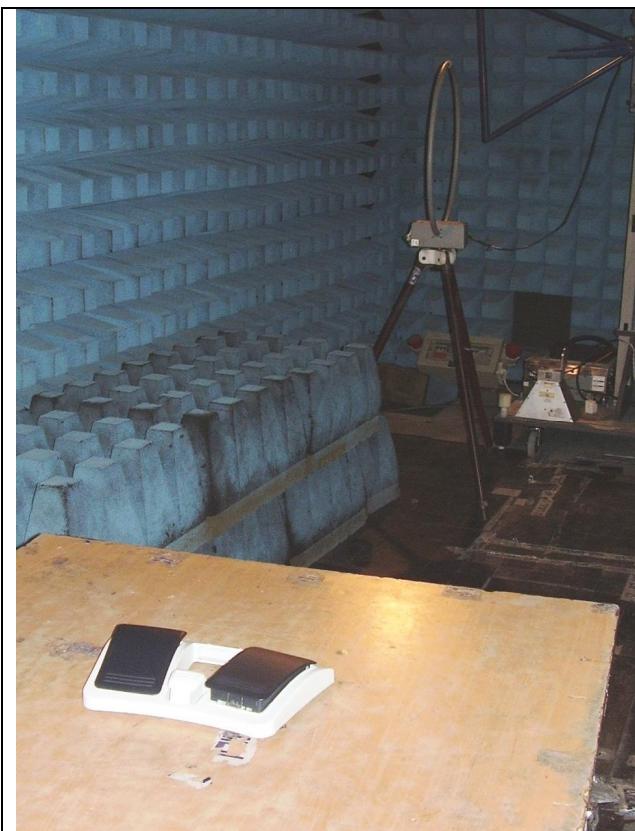

Investigation radiated emissions test of foot pedal transmitter with loop antenna.

iTero cart with USB dongle. Radiated emissions test setup at 1m distance.