

System Cheek_750MHz

D750V2-SN:1099

Communication System: CW; Frequency: 750.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 750.0$ MHz; $\sigma = 0.885$ S/m; $\epsilon_r = 43.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(10.48, 10.36, 10.24); Calibrated: 2024/6/3
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2024/3/14
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.0.0.116
- UID: CW, 0--

Area Scan (40.0 mm x 210.0 mm): Measurement Grid: 5.0 mm x 15.0 mm

SAR (1g) = 2.33 W/kg; SAR (10g) = 1.56 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.26 W/kg; SAR (10g) = 1.48 W/kg

Smallest distance from peaks to all points 3 dB below = 21.2 mm

Ratio of SAR at M2 to SAR at M1 = 88.7 %

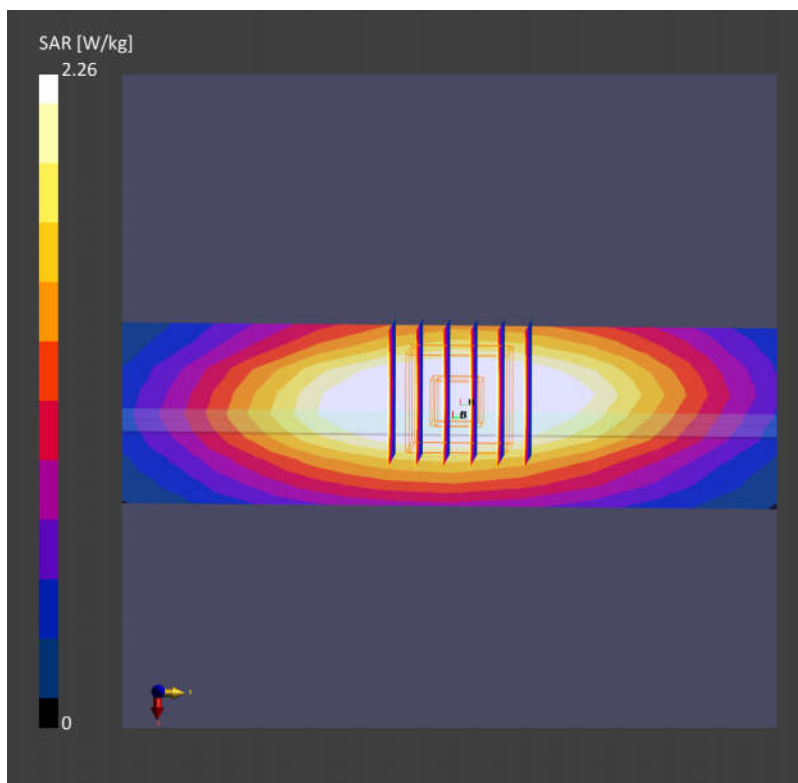

Date: 2024/7/29

System Cheek_835MHz

D835V2-SN:4d162

Communication System: CW; Frequency: 835.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.919$ S/m; $\epsilon_r = 43.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(10.19, 10.07, 9.95); Calibrated: 2024/6/3
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2024/3/14
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.0.0.116
- UID: CW, 0--

Area Scan (36.0 mm x 210.0 mm): Measurement Grid: 3.0 mm x 15.0 mm

SAR (1g) = 2.63 W/kg; SAR (10g) = 1.73 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 2.52 W/kg; SAR (10g) = 1.63 W/kg

Smallest distance from peaks to all points 3 dB below = 17.7 mm

Ratio of SAR at M2 to SAR at M1 = 88.6 %

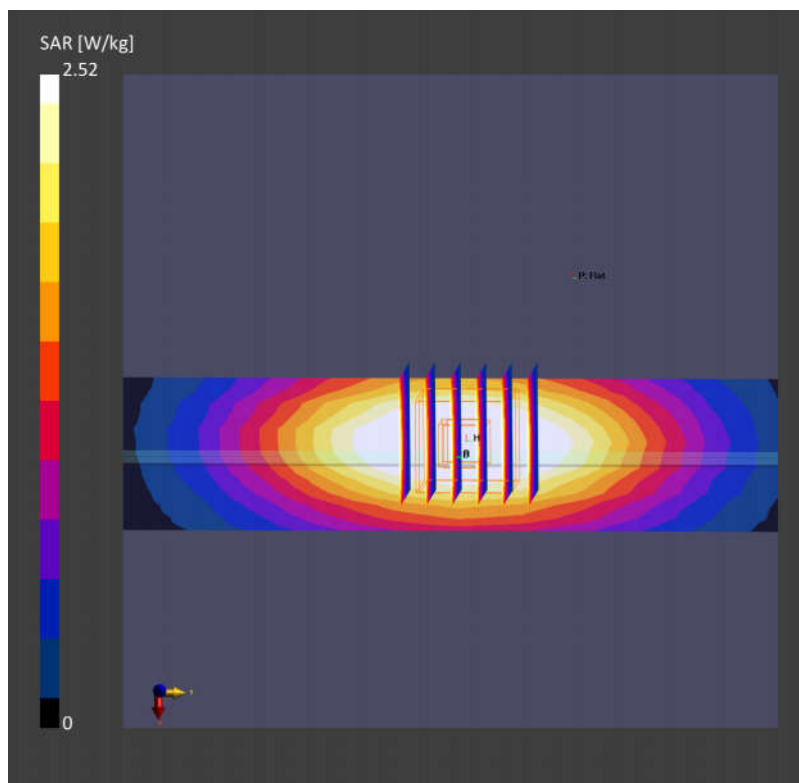

Date: 2024/7/29

System Cheek_1750MHz

D1750V2-SN:1137

Communication System: CW; Frequency: 1750.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.34$ S/m; $\epsilon_r = 41.9$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8.74, 8.64, 8.54); Calibrated: 2024/6/3
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2024/3/14
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.0.0.116
- UID: CW, 0--

Area Scan (36.0 mm x 120.0 mm): Measurement Grid: 3.0 mm x 15.0 mm
SAR (1g) = 9.34 W/kg; SAR (10g) = 5.01 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 9.11 W/kg; SAR (10g) = 4.87 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 85.3 %

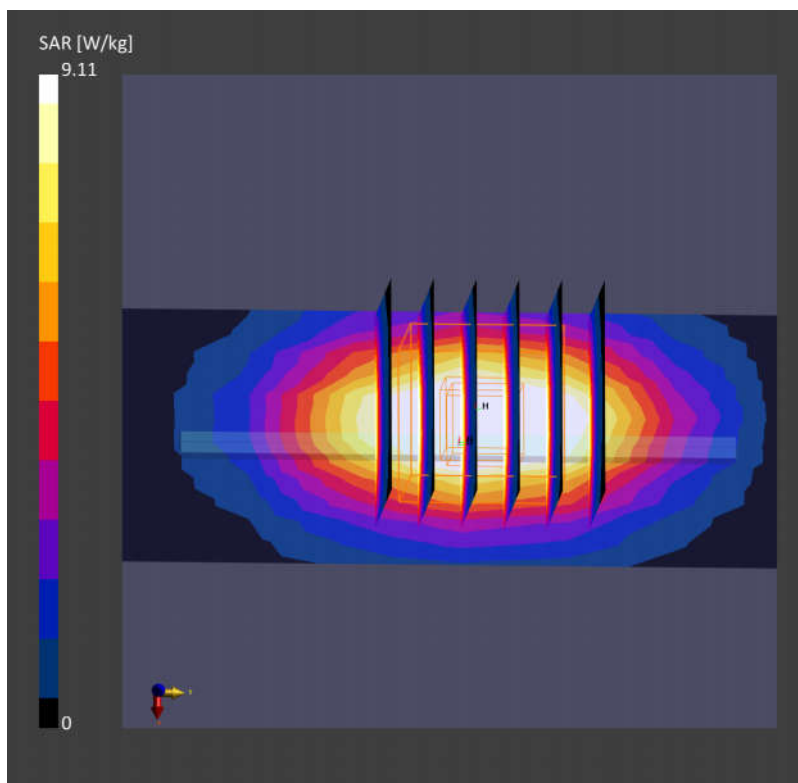

System Check_3500MHz

D3500V2-SN:1076

Communication System: CW; Frequency: 3500.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 3500.0$ MHz; $\sigma = 2.78$ S/m; $\epsilon_r = 39.2$
Ambient Temperature: 23.4°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.99, 6.9, 6.82); Calibrated: 2024/6/3
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2024/3/14
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: cDASY6 V16.0.0.116
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 6.25 W/kg; SAR (10g) = 2.44 W/kg;

Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 6.33 W/kg; SAR (10g) = 2.47 W/kg

Smallest distance from peaks to all points 3 dB below = 8.2 mm

Ratio of SAR at M2 to SAR at M1 = 77.7 %

