

Date: 2024-07-16

System Check_Head_2450MHz**DUT: D2450V2 - SN929**

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_2450_240716 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.83$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(7.39, 7.39, 7.39); Calibrated: 2024-03-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.34 W/kg; SAR (10g) = 1.12 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.05 dB

SAR (1g) = 2.40 W/kg; SAR (8g) = 1.26 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.7 %

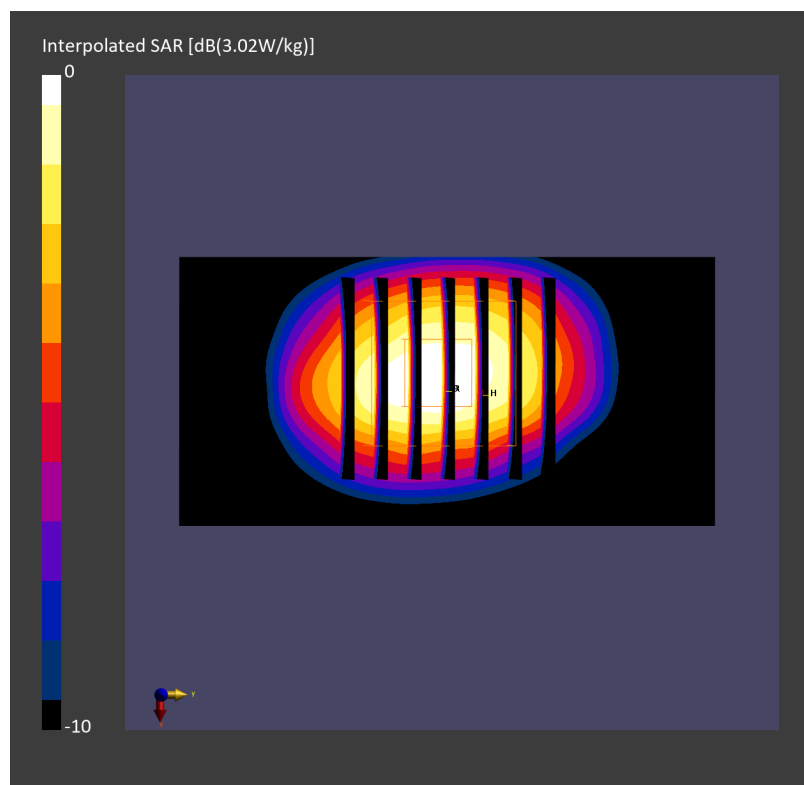

Date: 2024-07-16

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5G_240716 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.64$ S/m; $\epsilon_r = 36.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(5.1, 5.1, 5.1); Calibrated: 2024-03-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.31 W/kg; SAR (10g) = 0.940 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.08 dB

SAR (1g) = 3.82 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.09 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 65.9 %

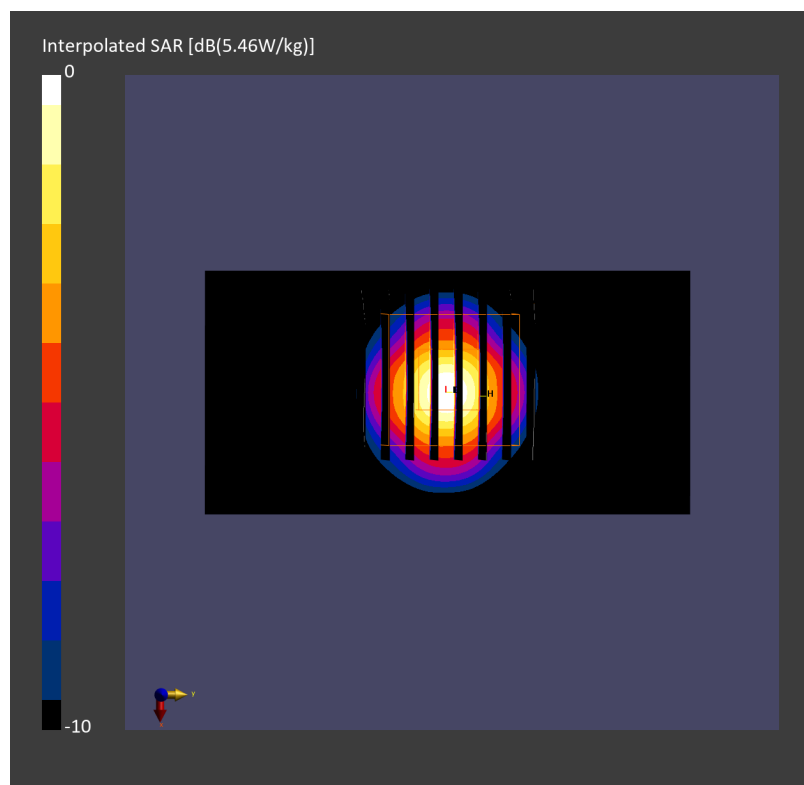

Date: 2024-07-16

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1006**

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_5G_240716 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.97$ S/m; $\epsilon_r = 35.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(4.3, 4.3, 4.3); Calibrated: 2024-03-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.85 W/kg; SAR (10g) = 1.12 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.12 dB

SAR (1g) = 4.24 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 64.2 %

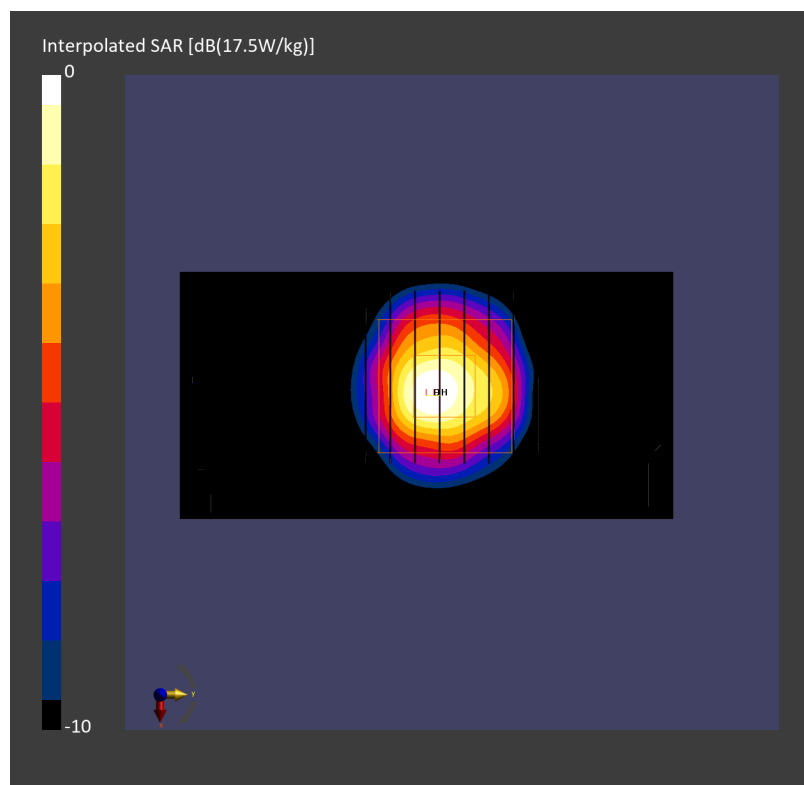

Date: 2024-07-16

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1128**

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_5G_240716 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.30$ S/m; $\epsilon_r = 35.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(4.46, 4.46, 4.46); Calibrated: 2024-03-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.08 W/kg; SAR (10g) = 2.05 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.07 dB

SAR (1g) = 7.71 W/kg; SAR (8g) = 2.55 W/kg; SAR (10g) = 2.19 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 61.3 %

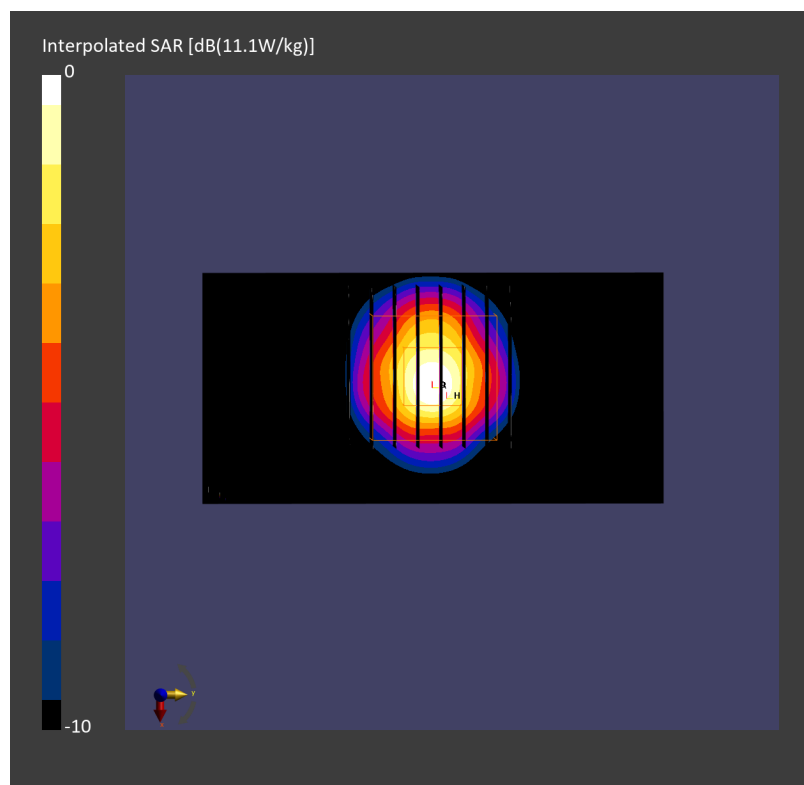

Date: 2024-07-16

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1083**

Communication System: CW; Frequency: 6500.000 MHz

Medium: HSL_6G_240716 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.00$ S/m; $\epsilon_r = 34.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(4.85, 4.85, 4.85); Calibrated: 2024-03-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn656; Calibrated: 2024-01-18
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1227; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 24.9 W/kg; SAR (10g) = 4.69 W/kg;

Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = 0.07 dB

SAR (1g) = 28.3 W/kg; SAR (8g) = 6.31 W/kg; SAR (10g) = 5.18 W/kg

Smallest distance from peaks to all points 3 dB below = 4.6 mm

Ratio of SAR at M2 to SAR at M1 = 51.4 %

psAPD (1.0cm², sq) = 283 [W/m²]; psAPD (4.0cm², sq) = 126 [W/m²]