

System Check_Head_3500MHz

Communication System: ; Frequency: 3500.0

Medium: HSL_3500_211206 Medium parameters used: $f = 3500.0$ MHz; $\sigma = 2.98$ S/m; $\epsilon_r = 37.3$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(7.14, 7.14, 7.14); Calibrated: 2021-10-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2021-01-19
- Phantom: Twin-SAM V4.0 (30deg probe tilt); Serial: 1488; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926
- UID: CW, 0--
- MAIA: Area Scan: N/A; Zoom Scan: N/A


Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.61 W/kg; SAR (10g) = 2.59 W/kg;

Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.11 dB

SAR (1g) = 6.84 W/kg; SAR (10g) = 2.75 W/kg;

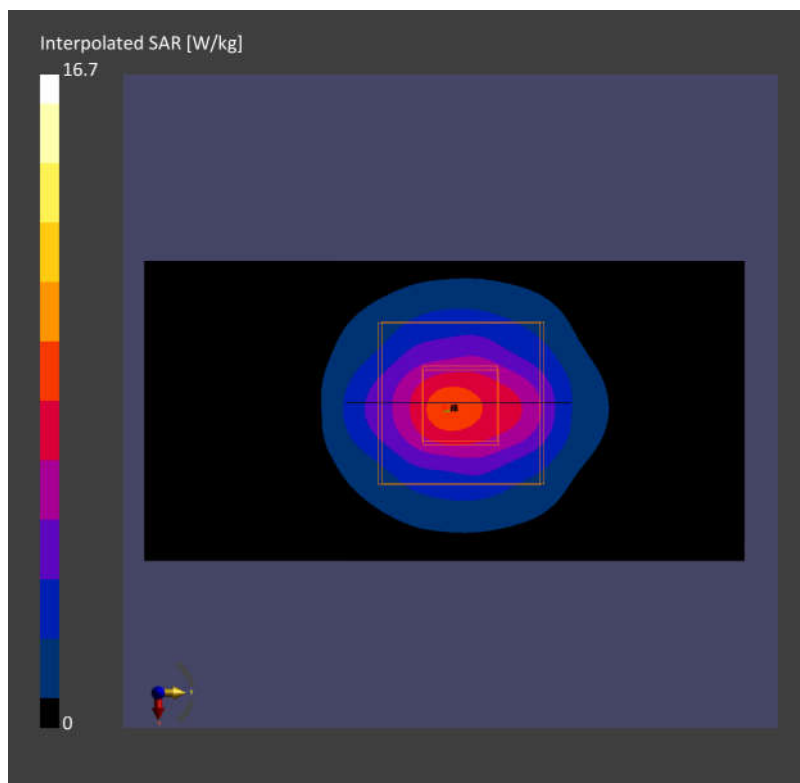

System Check_Head_3900MHz

Communication System: ; Frequency: 3900.0

Medium: HSL_3900_211206 Medium parameters used: $f = 3900.0$ MHz; $\sigma = 3.33$ S/m; $\epsilon_r = 36.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(6.55, 6.55, 6.55); Calibrated: 2021-10-21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1424; Calibrated: 2021-01-19
- Phantom: Twin-SAM V4.0 (30deg probe tilt); Serial: 1488; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926
- UID: CW, 0--
- MAIA: Area Scan: N/A; Zoom Scan: N/A

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.12 W/kg; SAR (10g) = 2.64 W/kg;

Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.06 dB

SAR (1g) = 7.35 W/kg; SAR (10g) = 2.54 W/kg;

