


4. BLOCK DIAGRAM

MiroCam Receiver Block Diagram

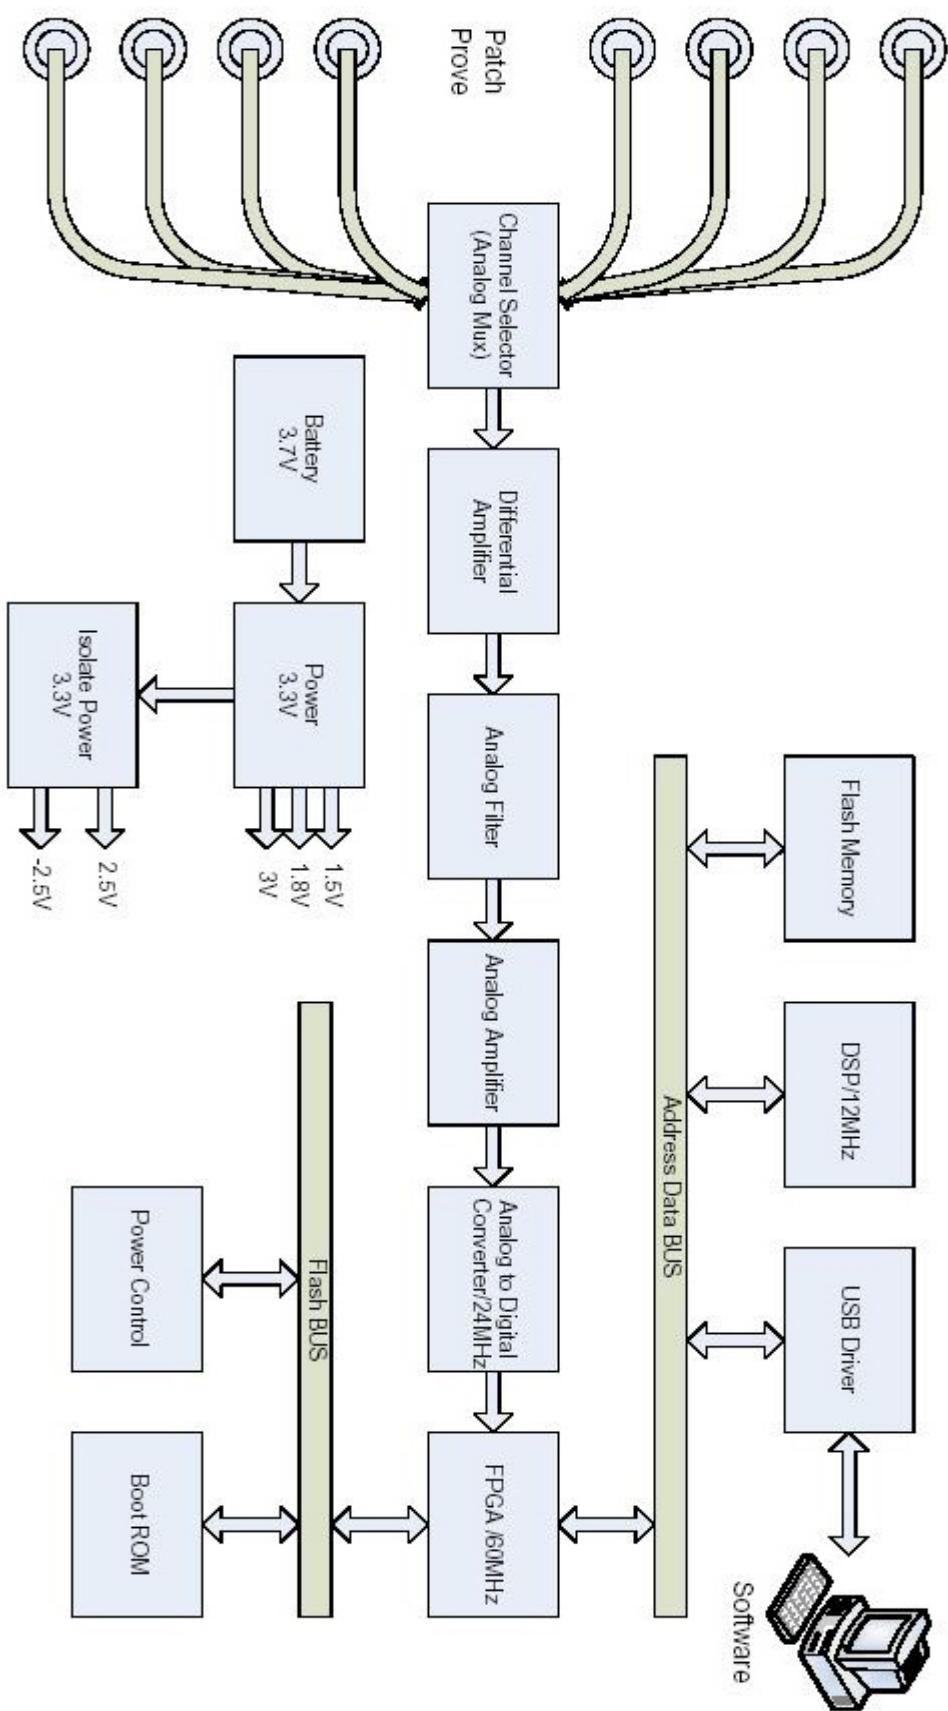

EUT Type: Capsule Endoscope & Receiver

FCC ID: VAXINTROMADIC