CGM System: Monitor Features

Home screen

Power/back button
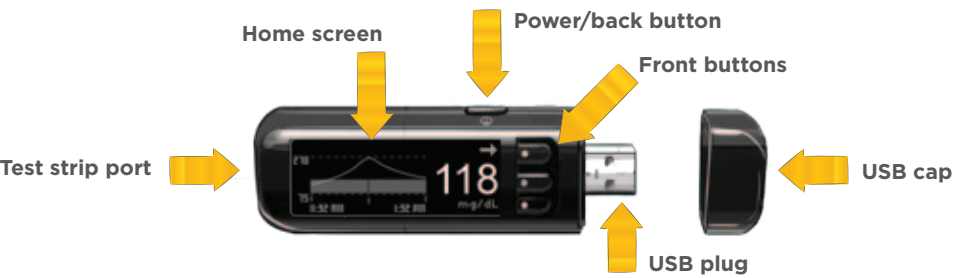
Front buttons

Test strip port

118 mg/dL

USB cap

USB plug

CGM System: Monitor Charging
Charge your monitor every day.

1. Remove the protective cap from the USB plug on the monitor.

2. Insert the monitor's USB plug into the wall adapter.

3. Plug the wall adapter into an outlet.

 - The orange light on the test strip port will blink while it is charging.

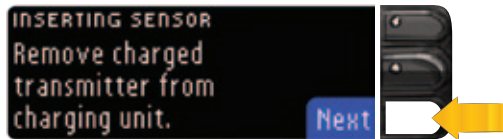 - The light will turn off after it has a full charge.

CGM System: Pairing the Monitor and Transmitter

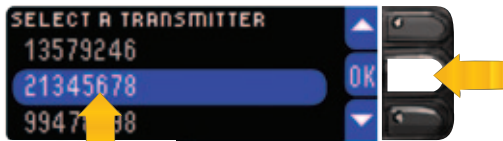1. Press and hold the power/back button for 2 seconds to turn on the monitor.

2. Lift to remove the fully charged transmitter from its charging unit.

   INSERTING SENSOR
   Remove charged transmitter from charging unit.
   Next

3. Wait for the monitor to find the transmitter (it may take as long as one minute).

   LOOKING FOR TRANSMITTER

4. Use the UP and DOWN buttons to find the number on the monitor screen that matches the number on the top of the charged transmitter, and press OK.
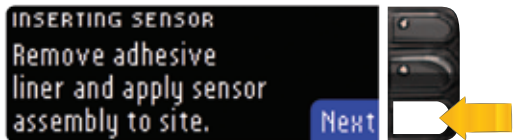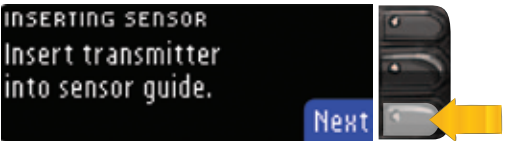
   SELECT A TRANSMITTER
   13579246
   21345678
   9947 98
   OK

5. Wait for the monitor to connect to the transmitter.

   CONNECTING TO TRANSMITTER

CGM System: Wearing a Sensor
Use the monitor screens to help guide you.

1. Remove the sensor guide from its sterile packaging and insert the transmitter into its slot in the sensor guide.

INSERTING SENSOR
Insert transmitter into sensor guide.
Next

2. Turn the sensor assembly over and remove the adhesive liner before putting the sensor assembly on your skin.

INSERTING SENSOR
Remove adhesive liner and apply sensor assembly to site.
Next

3. Insert the sensor (a CLICK sound means the sensor was inserted).

INSERTING SENSOR
Insert sensor then detach insertion tool.
Next

Once you have inserted a new sensor, you must wait 1 hour for the sensor to stabilize before you can calibrate it.

CGM System: Calibrating a Sensor
In order for the monitor to properly display your glucose levels, it must be calibrated with fingertip testing at least every 12 hours.

1. Choose to calibrate now or later.
    - If you are ready to calibrate, press YES and insert a test trip.

CALIBRATION
Stable levels.
Calibrate now?
Yes
No

2. After performing a prick of the tip of your finger, touch the tip of the test strip to the drop of blood and hold it there until the monitor beeps and shows "Accepted"

APPLY BLOOD

3. Read your fingertip test result.
    - If you want to use this result to calibrate your monitor, press YES. If you do not wish to use it to calibrate, press NO.

USE FOR CALIBRATION?
FINGERTIP RESULT
120
mg/dL
Yes
No

4. Your continuous glucose reading will appear on the Home screen within 5 minutes of calibrating.

270
118
75
11:32 AM   1:32 PM   mg/dL