


Impedance Plot for

CLA150-SN:4008; 150Head

Calibrated impedance: $44.7\Omega + 6.6j\Omega$; Measurement impedance: $44.5\Omega - 7.2j\Omega$ (within 5Ω)

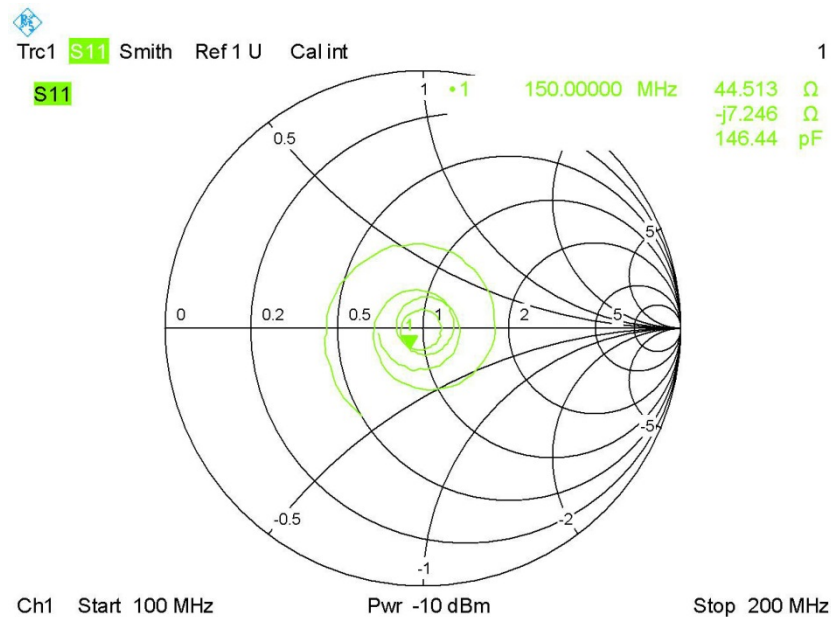

Calibrated return loss: -21.0dB; Measurement return loss: -21.76 dB (within 20%)

