


---

## APPENDIX C EUT TEST POSITION PHOTOS


---

### Liquid depth $\geq 15\text{cm}$

Phantom: SAM (30deg probe tilt) with CRP v5.0\_20150321; Type: QD000P40CD; Serial: TP:1874

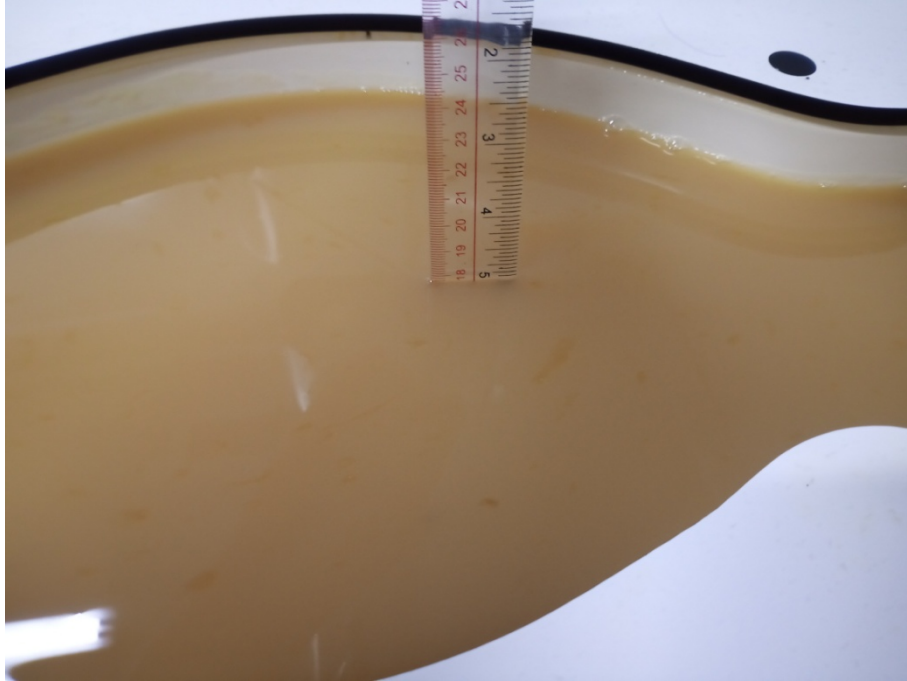

**Body Back Setup Photo(5mm)**

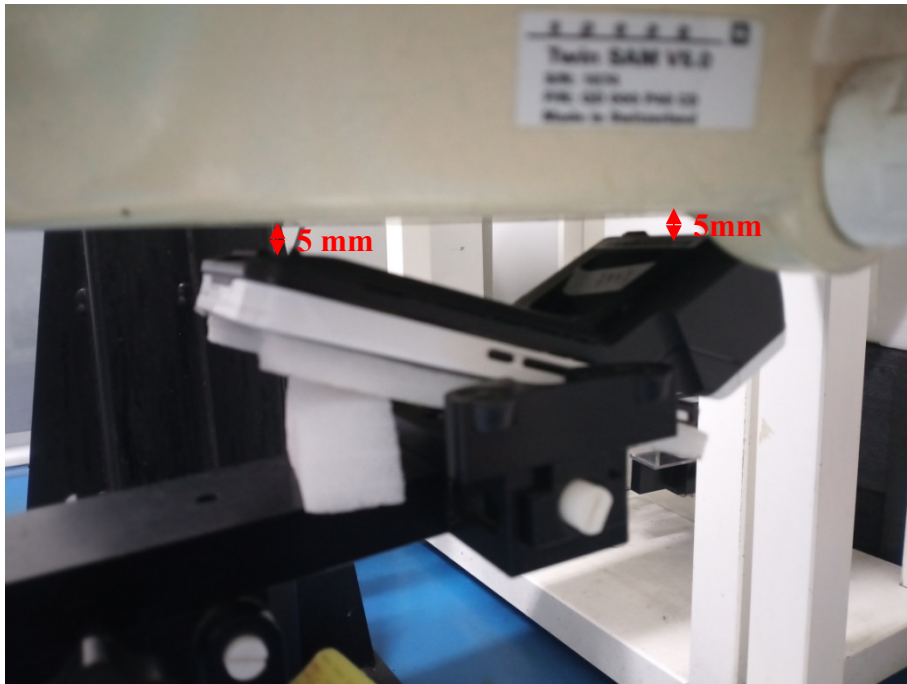

**Handheld Back Setup Photo(0mm)**



Handheld Left Setup Photo(0mm)



Handheld Right Setup Photo(0mm)



**Handheld Top Setup Photo(0mm)**

