

NeuroPace Neurostimulator  
Model RNS-300M

FCC ID:  
WBWRF300

Label Artwork and  
Location Photographs

Implantable Medical Device – Not Desirable or Feasible for FCC ID Label




NeuroPace Neurostimulator  
Model RNS-300M

FCC ID:  
WBWRF300

Label Artwork and  
Location Photographs

Label Locations - Packaging Tray and RNS-300M Kit Box  
(Note that the RNS-300M is placed inside Packaging Tray which is placed inside of RNS-300M Kit Box. )

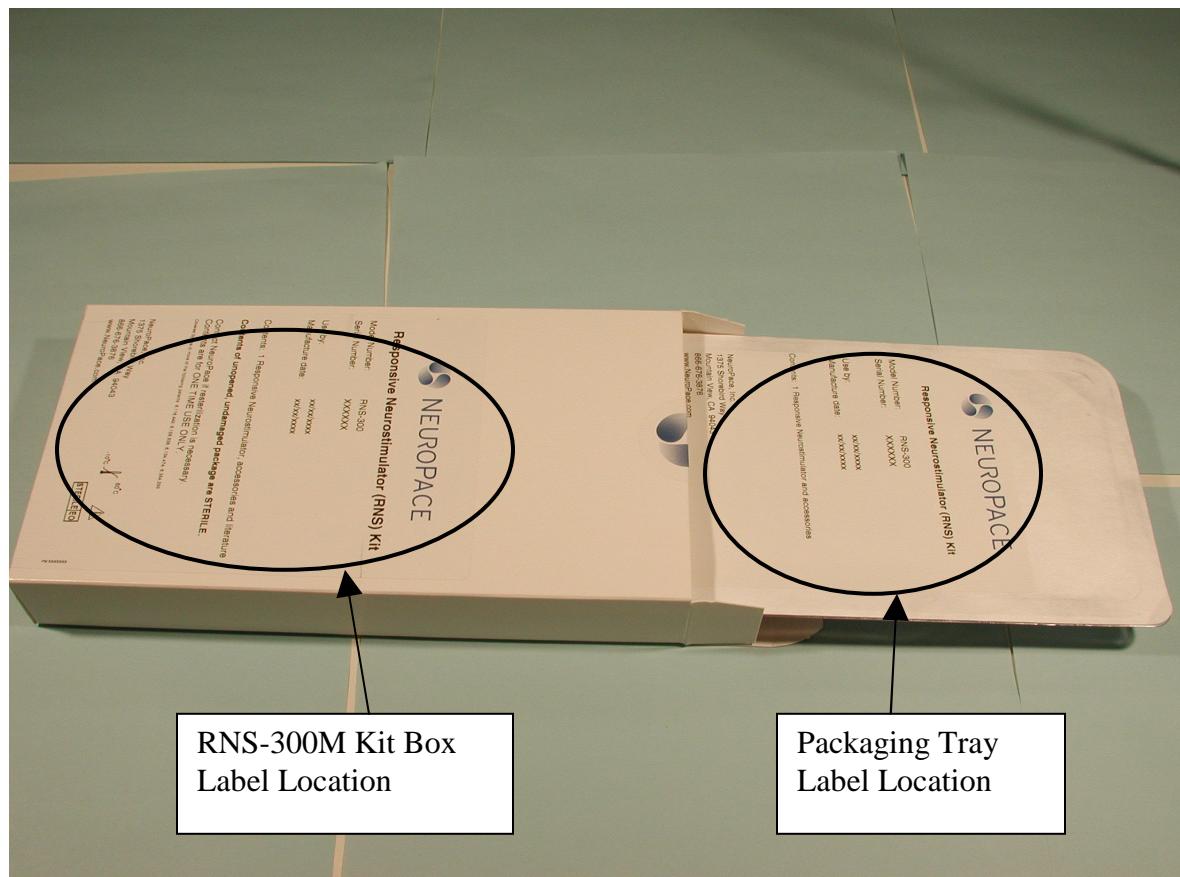


Label Artwork (Top of Packaging Tray) View Showing FCC ID



Caution: Consult the RNS® System User Manual before using package contents. The RNS® System User Manual is also available online at [www.neuropace.com](http://www.neuropace.com). For a hardcopy, contact NeuroPace.

Caution: Federal law restricts this device to sale by or on the order of a physician.

Location of  
FCC ID on  
inner  
packaging.

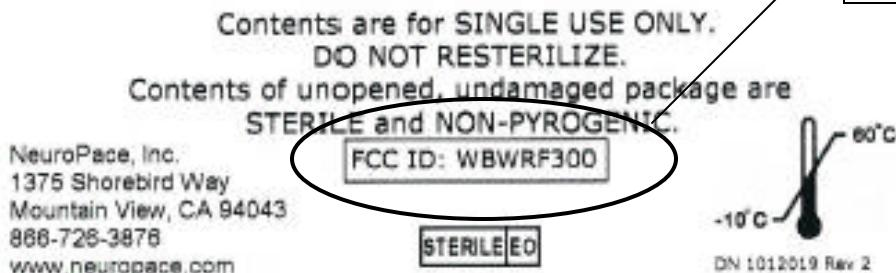

NeuroPace Neurostimulator  
Model RNS-300M

FCC ID:  
WBWRF300

Label Artwork and  
Location Photographs

Label Artwork (Top of RNS-300M Kit Box) View Showing FCC ID



Package Contents:

| Qty | Description            | Model    |
|-----|------------------------|----------|
| (1) | RNS® Neurostimulator   | RNS-300M |
| (1) | Connector Cover        | CC-01    |
| (1) | Craniectomy Template   | CT-01    |
| (1) | Ferrule                | F-01     |
| (1) | Ferrule Clamp          | FC-01    |
| (1) | Lead Strain Relief     | LSR-01   |
| (1) | Torque Driver          | TD-01    |
| (1) | CD with manuals        |          |
|     | Registration Materials |          |

Caution: Consult the RNS® System User Manual before using package contents. The RNS® System User Manual is also available online at [www.neuropace.com](http://www.neuropace.com). For a hardcopy, contact NeuroPace.

Caution: Federal law restricts this device to sale by or on the order of a physician.

Contents may be covered by one or more of the following U.S. Patents: 5,938,689; 6,016,449; 6,128,538; 6,134,474; 6,230,049; 6,427,086; 6,466,822; 6,473,639; 6,480,743; 6,591,138; 6,597,954; 6,647,296; 6,662,035; 6,690,974; 6,810,285; 6,944,501; 7,136,695; 7,158,833.

Location of  
FCC ID on  
packaging  
box

Contents are for SINGLE USE ONLY.  
DO NOT RESTERILIZE.

Contents of unopened, undamaged package are  
STERILE and NON-PYROGENIC.

FCC ID: WBWRF300

STERILE EO



NeuroPace, Inc.  
1375 Shorebird Way  
Mountain View, CA 94043  
866-726-3876  
[www.neuropace.com](http://www.neuropace.com)



RNS® Neurostimulator Kit  
Model Number: RNS-300M-K      Use by Date: DD-MON-YYYY  
Serial Number: 123456  
DN 1012019 Rev 2

Part 15.19 (Labeling Requirement) and Part 15.21 (Information to User) in Manual found in two parts

1) immediately following the title page

© Copyright 2011, NeuroPace, Inc. All rights reserved.

#### **FCC Information**

The following is communications regulation information on the Model RNS-300M Neurostimulator and Model W-02 Wand.

Neurostimulator FCC ID: WBWRF300  
Wand FCC ID: WBW902

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

**IMPORTANT:** Changes or modifications to this product not expressly approved by NeuroPace Inc. could void the FCC Certification and negate your authority to operate this product.

This equipment complies with FCC radiation exposure limits set forth for an uncontrolled environment. This transmitter must not be co-located or operating in conjunction with any other antenna or transmitter.

2) on page 91 of the Manual

*Troubleshooting*

**91**

---

#### **ELECTROMAGNETIC EMISSIONS AND IMMUNITY AND WIRELESS TECHNOLOGY**

Medical Electrical Equipment needs special precautions regarding EMI and the following precautions should be taken before use:

This equipment/system may cause radio interference or may disrupt the operation of nearby equipment. The RNS System may be interfered with by other equipment, even if that other equipment complies with CISPR emission requirements. It may be necessary to take mitigation measures, such as re-orienting or relocating the RNS System or shielding its location.

The NeuroPace Programmer should not be used adjacent to or stacked with other equipment. If adjacent or stacked use is necessary, the RNS System should be observed to verify normal operation in the configuration in which it will be used.

The NeuroPace® RNS™ Neurostimulator, NeuroPace® Cortical Strip Lead, and NeuroPace® Depth Lead are not compatible with non-NeuroPace leads and/or pulse generators. Incompatible configurations may cause increased electromagnetic emissions or decreased immunity of the RNS System.

Portable and mobile RF communications equipment can affect the RNS System.