



7. PHOTOGRAPHS OF MEASUREMENT


Test Position: Right Cheek

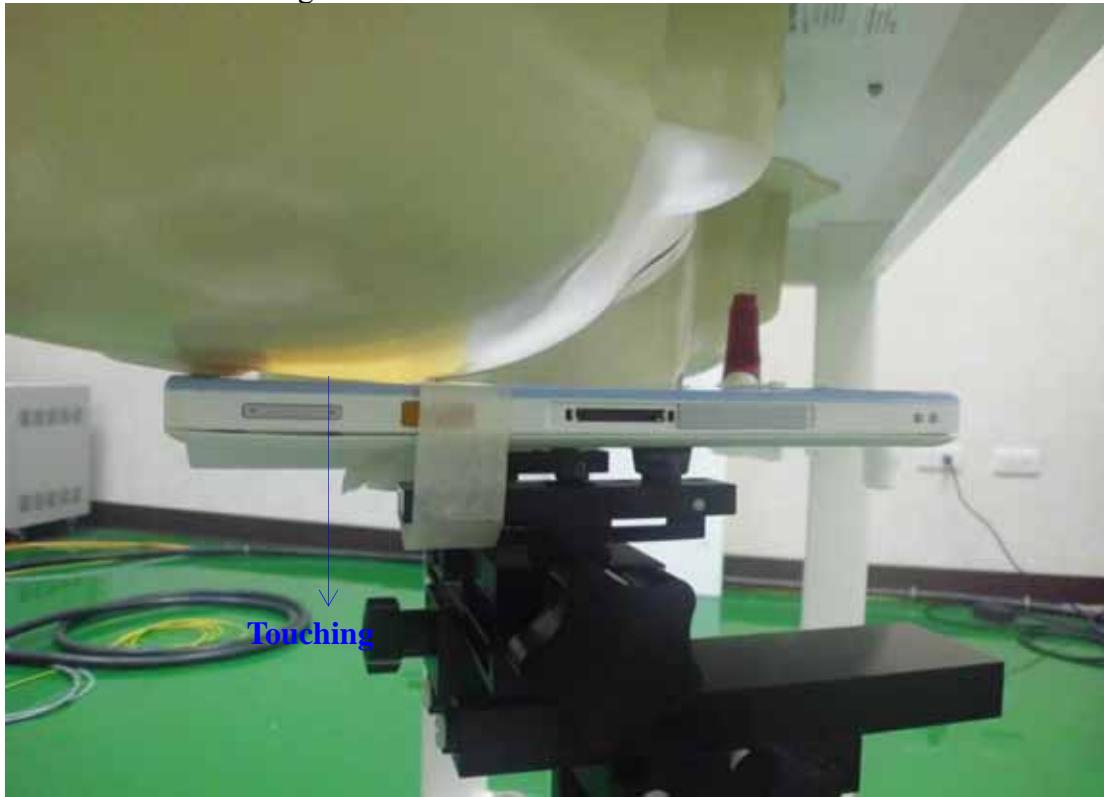


Test Position: Right Tilted

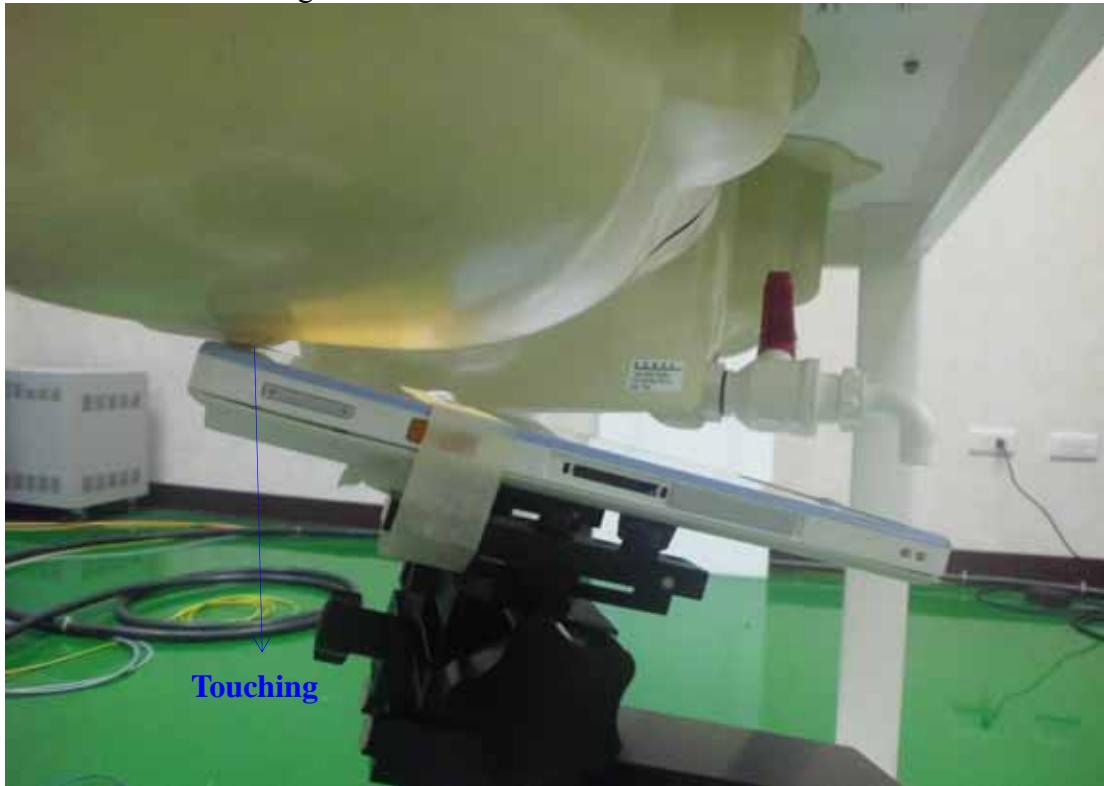

Test Position: Left Cheek

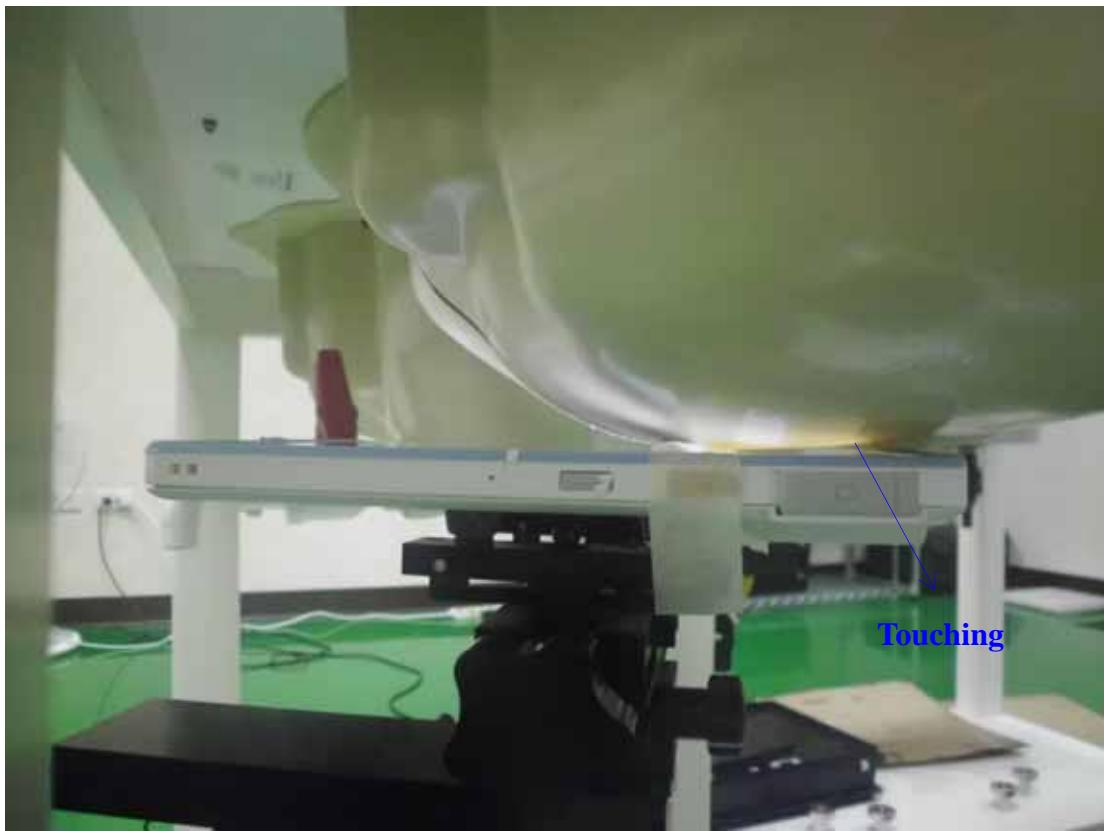

Test Position: Left Tilted

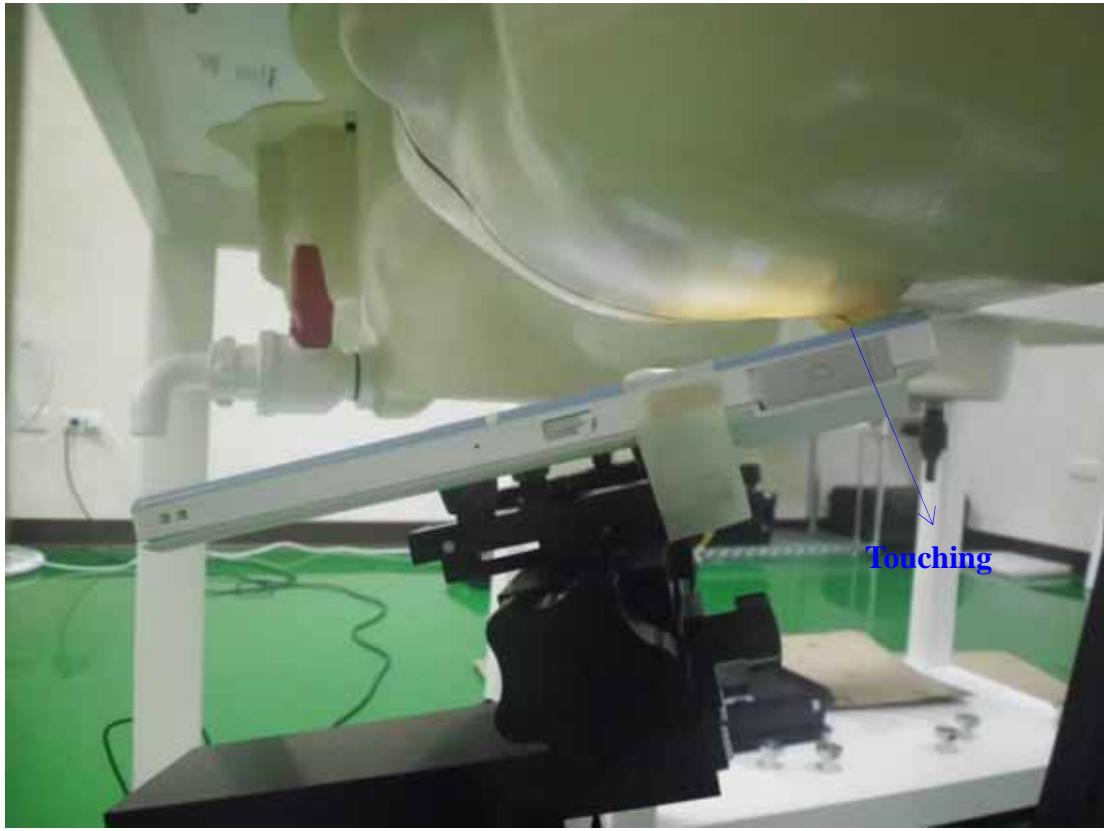

Test Position: Top Side of Panel



Test Position: Back of Panel



Test Position: Right Side of Panel



Test Position: Left Side of Panel



Depth of the Liquid in the Phantom-Zoom In

