



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

FCC Rules and Regulations / Intentional Radiators

Operational in the 902-928 MHz, 2400-2483.5 MHz, and 5725-5850 MHz, Bands

Part 15, Subpart C, Section 15.247

FHSS

**THE FOLLOWING MEETS THE ABOVE TEST SPECIFICATION**

Formal Name: Accu-Chek Aviva Combo  
Kind of Equipment: Blood Glucose Meter  
Frequency Range: 30 MHz - 26 GHz  
Test Configuration: Bluetooth (Tested at 4.5 vdc)  
Model Number(s): Aviva: 670  
Model(s) Tested: Aviva: 670  
Serial Number(s): N/A  
Date of Tests: August 6, 7, 10 & 28, 2009  
Test Conducted For: Roche Diagnostics  
9115 Hague Road  
Indianapolis, Indiana 46250

**NOTICE:** "This report must not be used by the client to claim product endorsement by NVLAP or any agency of the U.S. Government". Please see the "Additional Description of Equipment Under Test" page listed inside of this report.

© Copyright 1983-2009 D.L.S. Electronic Systems, Inc

**COPYRIGHT NOTICE**

This report must not be reproduced (except in full), without the approval of D.L.S. Electronic Systems, Inc.



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

#### SIGNATURE PAGE

Report By:

A handwritten signature in black ink that reads "Aron C. Rowe".

Aron C. Rowe  
Test Engineer  
EMC-001375-NE

Reviewed By:

A handwritten signature in black ink that reads "William Stumpf".

William Stumpf  
OATS Manager

Approved By:

A handwritten signature in black ink that reads "Brian J. Mattson".

Brian Mattson  
General Manager



1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

## TABLE OF CONTENTS

i.	Cover Page .....	1
ii.	Signature Page .....	2
iii.	Table of Contents .....	3
iv.	NVLAP Certificate of Accreditation .....	5
1.0	Summary of Test Report .....	6
2.0	Introduction .....	6
3.0	Object .....	6
4.0	Test Set-Up .....	7
5.0	Test Equipment .....	8
6.0	Ambient Measurements .....	9
7.0	Description of Test Sample .....	10
8.0	Additional Description of Test Sample .....	11
9.0	Photo Information and Test Set-Up .....	11
10.0	Radiated Photos Taken During Testing .....	12
10.0	Conducted Photos Taken During Testing .....	16
11.0	Results of Tests .....	17
12.0	Conclusion .....	17
	TABLE 1 – EQUIPMENT LIST .....	18
	Appendix A – AC Power Line Conducted Emissions Test .....	19
1.0	AC Power Line Conducted Emission Measurements .....	20



1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

## TABLE OF CONTENTS

Appendix B – Electric Field FHSS Radiated Emissions Tests.....	21
1.0 Spurious Emissions at the Antenna Terminals/Antenna Connector.....	22
1.0 RF Conducted Emission Data and Charts made at the Antenna Terminals .....	23
2.0 RF Conducted Emissions Photos Taken During Testing.....	36
3.0 Restricted Bands .....	37
4.0 Restricted Band and Band Edge Compliance .....	37
4.0 Data and Graph(s) taken showing the Restricted Band Compliance.....	38
4.0 Data and Graph(s) taken showing the 20 dB Bandwidth.....	42
4.0 Data and Graph(s) taken showing the Band Edge Conducted Compliance.....	52
4.0 Data and Graph(s) taken of the Upper Band Edge with Restricted Band.....	55
5.0 Field Strength of Fundamental and Spurious Emission Measurements .....	58
5.0 Radiated Data and Graph(s) taken for Fundamental and Spurious Emission.....	60
6.0 Transmitter Duty Cycle Graphs Taken During testing .....	64
6.0 Carrier Frequency Separation Graph(s) taken during testing .....	69
6.0 Number of Hopping Channels Graph(s) taken during testing .....	72
6.0 Time of Occupancy Graphs taken during testing .....	74
6.0 Conducted Peak Output Power Graphs Taken During testing.....	76



1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

United States Department of Commerce  
National Institute of Standards and Technology



## Certificate of Accreditation to ISO/IEC 17025:2005

NVLAP LAB CODE: 100276-0

D.L.S. Electronic Systems, Inc.  
Wheeling, IL

is accredited by the National Voluntary Laboratory Accreditation Program for specific services,  
listed on the Scope of Accreditation, for:

### ELECTROMAGNETIC COMPATIBILITY AND TELECOMMUNICATIONS

This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2005.  
This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory quality  
management system (refer to joint ISO/ILAC/JAF Communiqué dated 18 June 2005).



2008-10-01 through 2009-09-30

Effective dates

Dally S. Bruce  
For the National Institute of Standards and Technology

NVLAP-01C (REV. 2006-09-13)



1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

## 1.0 SUMMARY OF TEST REPORT

It was found that the Accu-Chek Aviva Combo, Model Number(s) Aviva: 670 **meets** the radio interference radiated emission requirements of the FCC "Rules and Regulations", Part 15, Subpart C, Section 15.247 for operational in the 2400-2483.5 MHz Band. The AC Power Line conducted emissions test was not required because the Accu-Chek Aviva Combo is powered from a D.C. power source. It does not have a line cord to plug into the A.C. power line.

## 2.0 INTRODUCTION

On August 6, 7, 10 & 28, 2009, a series of radio frequency interference measurements was performed on Accu-Chek Aviva Combo, Model Number(s) Aviva: 670, Serial Number: N/A. The tests were performed according to the procedures of the FCC as stated in the "Methods of Measurement of Radio-Noise Emissions for Low-Voltage Electrical and Electronic Equipment in the Range of 9 kHz to 40 GHz" found in the American National Standards Institute, ANSI C63.4-2003 & the FCC guidance document "Measurement of Digital Transmission Systems Operating under Section 15.247 - March 23, 2005". Tests were performed by personnel of D.L.S. Electronic Systems, Inc. who are responsible to Donald L. Sweeney, Senior EMC Engineer.

D.L.S. Electronic Systems, Inc. is a full service EMC/Safety Testing Laboratory accredited to ISO 17025. NVLAP Certificate and Scope can be viewed at <http://www.dlsemc.com/certificate>. Our facilities are registered with the FCC, Industry Canada, and VCCI.

### **Main Test Facility:**

D.L.S. Electronic Systems, Inc.  
1250 Peterson Drive  
Wheeling, Illinois 60090

### **O.A.T.S. Test Facility:**

D.L.S. Electronic Systems, Inc.  
166 S. Carter Street  
Genoa City, Wisconsin 53128  
FCC Registration Number: 334127

## 3.0 OBJECT

The purpose of this series of tests was to determine if the test sample could meet the radio frequency interference emission requirements of the FCC "Rules and Regulations", Part 15, Subpart C, Sections 15.205, 15.209 & 15.247 for Intentional Radiators operating in the Bands 902-928 MHz, 2400-2483.5 MHz, and 5725-5850 MHz.



1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

#### 4.0 TEST SET-UP

All emission tests were performed at D.L.S. Electronic Systems, Inc. and set up according to the ANSI C63.4-2003, Annex H or following the guidelines in the FCC's "Measurement of Digital Transmission Systems Operating under Section 15.247 - March 23, 2005". The conducted tests were performed with the test item placed on a non-conductive table (table top equipment), located in the test room. Equipment normally operated on the floor was tested by placing it on the metal ground plane. The ground plane has an electrical isolation layer over its surface approximately 7mm thick. The power line supplied was connected to a dual line impedance stabilization network electrically bonded to the ground plane, located on the floor. The networks were constructed per the requirements of the ANSI C63.4-2003, Annex H.

All radiated emissions tests were performed with the test item placed on a 80 cm high rotating non-conductive table, located in the test room. Equipment normally operated on the floor was placed on a metal covered turntable which is flush with the surrounding conducting ground plane. The ground plane has an electrical isolation layer over its surface approximately 7 mm thick. The EUT is separated from the turntable ground plane by a non-conductive layer. The equipment under test was set up according to ANSI C63.4-2003, Sections 6 and 8 or following the guidelines in the FCC's "Measurement of Digital Transmission Systems Operating under Section 15.247 - March 23, 2005", as indicated in the test data section of this test report..



1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

## 5.0 TEST EQUIPMENT (Bandwidths and Detector Function)

All preliminary data below 1000 MHz was automatically plotted using the ESI 26/40 Fixed Tuned Receiver. The data was taken using Peak, Quasi-Peak or the Average Detector Functions as required. This information was then used to determine the frequencies of maximum emissions. Above 1000 MHz, final data was taken using the Average Detector.

Below 1000 MHz, final data was taken using the ESI 26/40 Fixed Tuned Receiver. These plots were made using the Peak or Quasi-Peak Detector functions, with manual measurements performed on the questionable frequencies using the Quasi-Peak or the Average Detector Function of the ESI 26/40 Fixed Tuned Receiver as required. Above 1000 MHz, final data was taken using the Average Detector on the Spectrum Analyzer.

The bandwidths shown below are specified by ANSI C63.4-2003, Section 4.2.

Frequency Range	Bandwidth (-6 dB)
10 to 150 kHz	200 Hz
150 kHz to 30 MHz	9 kHz
30 MHz to 1 GHz	120 kHz
Above 1 GHz	1 MHz

A list of the equipment used can be found in Table 1. All primary equipment was calibrated against known reference standards with a verified traceable path to NIST.



1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

## 6.0 AMBIENT MEASUREMENTS

For emissions measurements, broadband antennas and an EMI Test Receiver with a panoramic spectrum display are used. First the frequency range is scanned and displayed on the test receiver display. Next the scanned frequency range is divided into smaller ranges, and then it is manually tuned through to determine the emissions from the EUT. A headset or loudspeaker is connected to the test receiver's AM/FM demodulated output as an aid in detecting ambient signals and finding frequencies of significant emission from the EUT. If there is any doubt as to the source of the emission, it is further investigated by rotating the EUT, or by disconnecting the power from the EUT.

The EUT is set up in its typical configuration and operated in its various modes. For tabletop systems, cables are manipulated within the range of likely configurations. For floor-standing equipment, the cables are located in the same manner as the user would install them and no further manipulation is made. If the manner of cable installation is not known, or if it changes with each installation, cables or wires for floor-standing equipment shall be manipulated to the extent possible to produce the maximum level of emissions. For each mode of operation, the frequency spectrum is monitored. Variations in antenna height, antenna polarization, EUT azimuth, and cable or wire placement (each variable within bounds specified elsewhere) are explored to produce the emissions that have the highest amplitude relative to the limit. These methods are performed to the specifications in ANSI C63.4-2003.



1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

## 7.0 DESCRIPTION OF TEST SAMPLE: (See also Paragraph 8.0)

### 7.1 Description:

This device is a blood glucose meter that is capable of communicating with an insulin pump.

### 7.2 PHYSICAL DIMENSIONS OF EQUIPMENT UNDER TEST

Length: 3.7" x Width: 2.2" x Height: 0.9

### 7.3 LINE FILTER USED:

N/A

### 7.4 INTERNAL CLOCK FREQUENCIES:

Switching Power Supply Frequencies:

1.5 MHz

Clock Frequencies:

16 MHz Oscillator, 4.5 MHz clock

### 7.5 DESCRIPTION OF ALL CIRCUIT BOARDS:

1. PWB Satellite DM PN: 7004829 rev D
2. PWA Satellite DM CSII PN: 7003381 rev B
3. PWB Main DM PN: 7002695 rev D



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

8.0 ADDITIONAL DESCRIPTION OF TEST SAMPLE:  
(See also Paragraph 7.0)

1: There were no additional descriptions noted at the time of test.

NOTE:

Battery operated digital device that incorporates a Bluetooth transceiver. A test fixture was used prior to testing to control the Bluetooth module transmit frequency and modulation settings.

9.0 PHOTO INFORMATION AND TEST SET-UP


Item 0 Accu-Chek Aviva Combo  
Model Number: Aviva: 670; Serial Number: N/A



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

#### 10.0 RADIATED PHOTOS TAKEN DURING TESTING

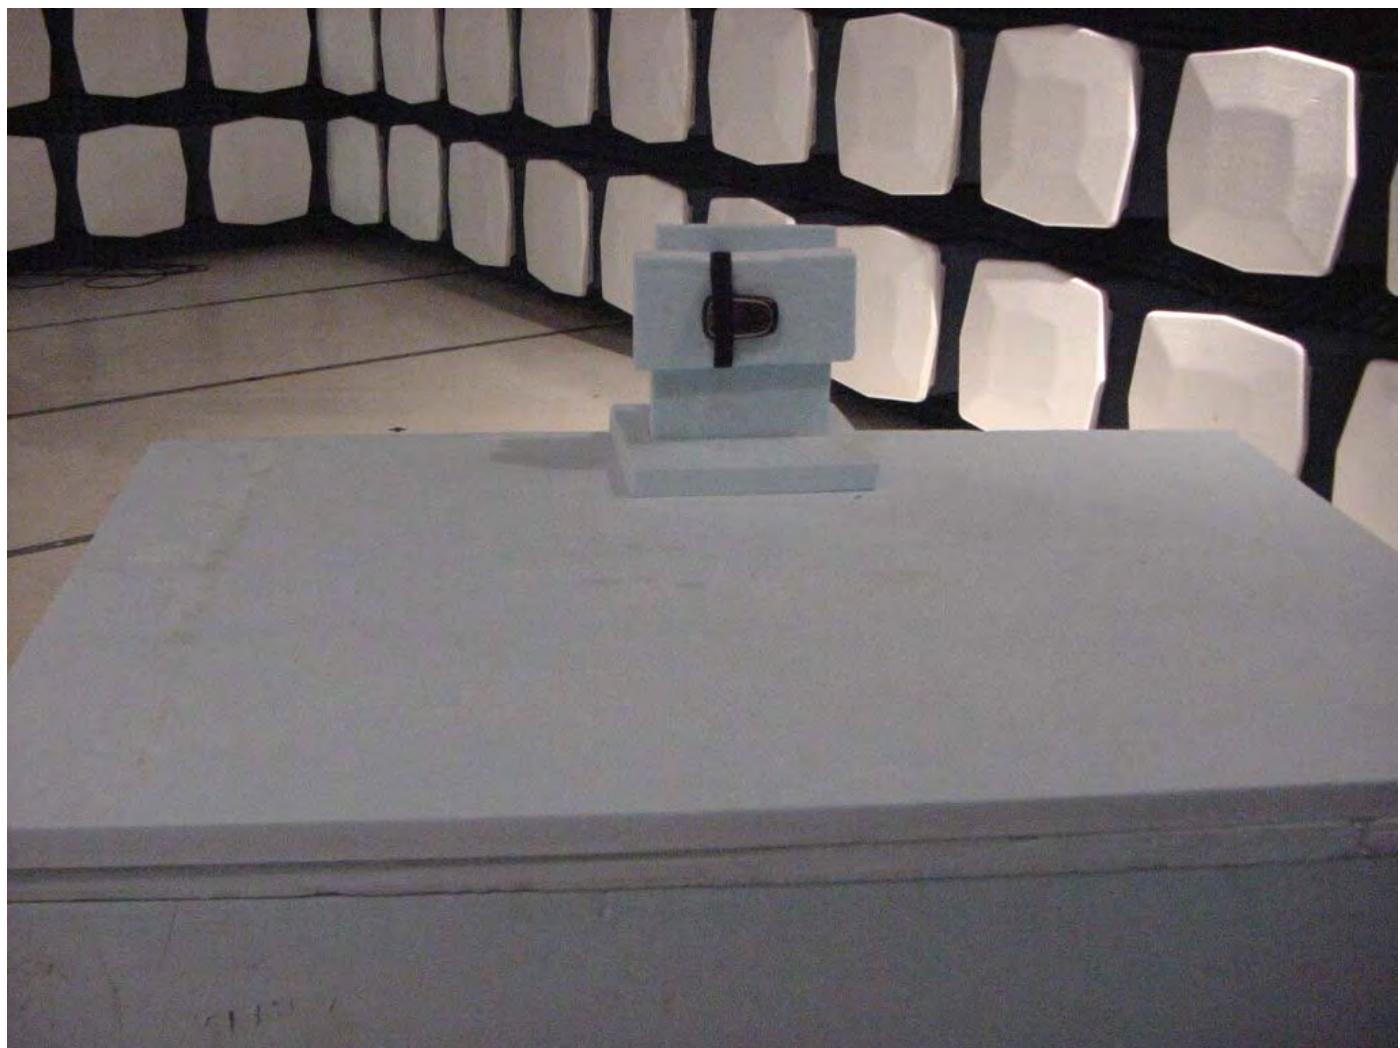


RADIATED X AXIS



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

#### 10.0 RADIATED PHOTOS TAKEN DURING TESTING (CON'T)

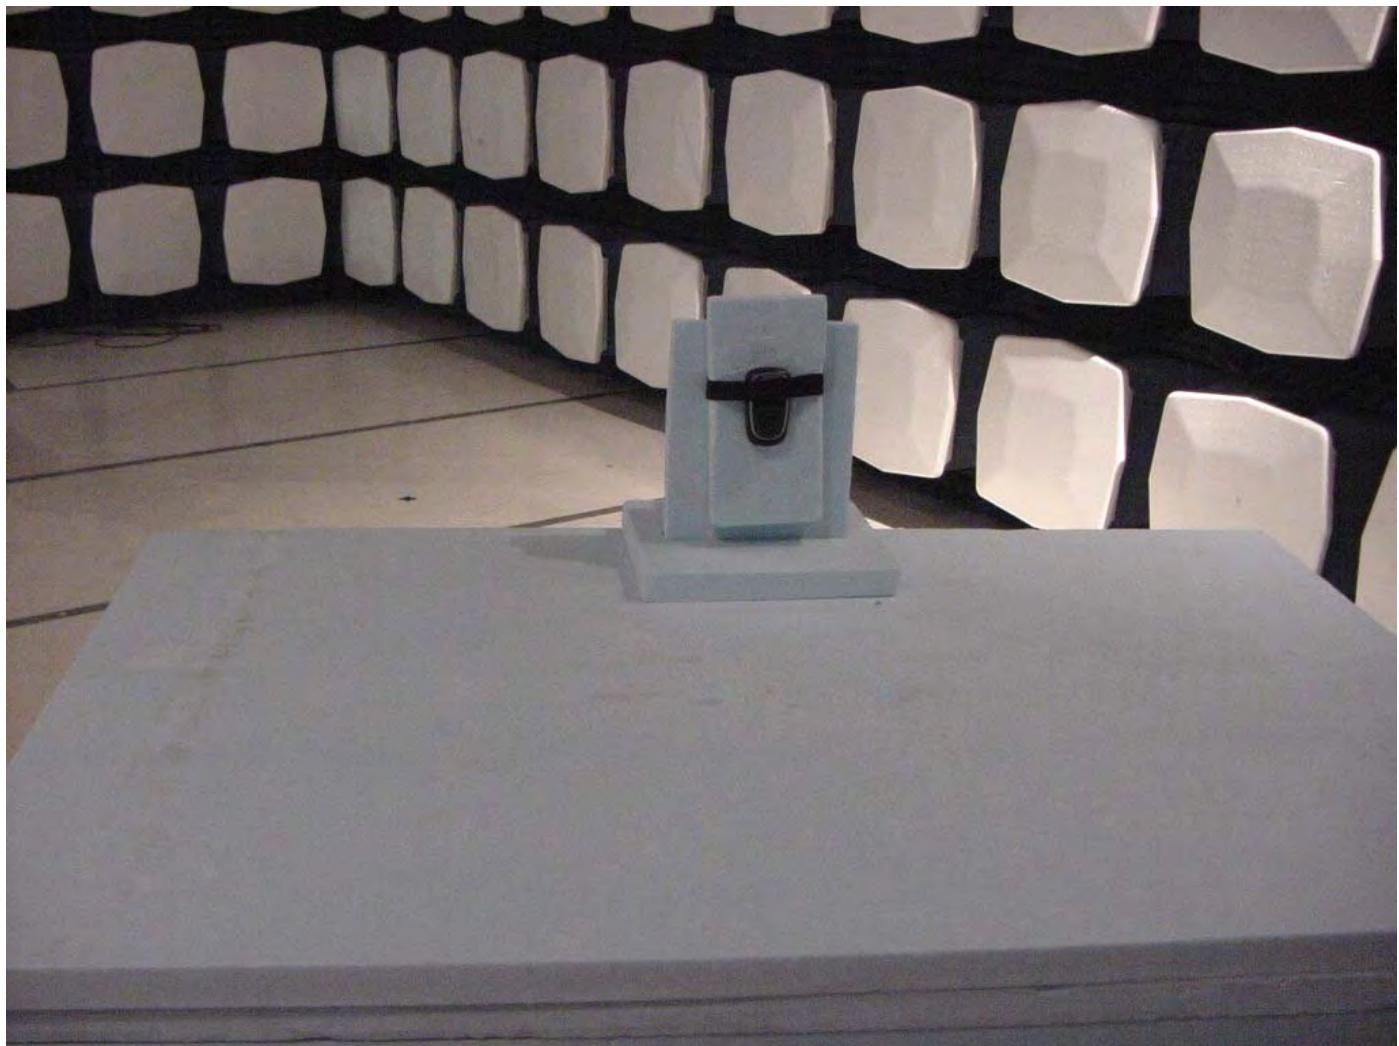


RADIATED Y AXIS



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

#### 10.0 RADIATED PHOTOS TAKEN DURING TESTING (CON'T)

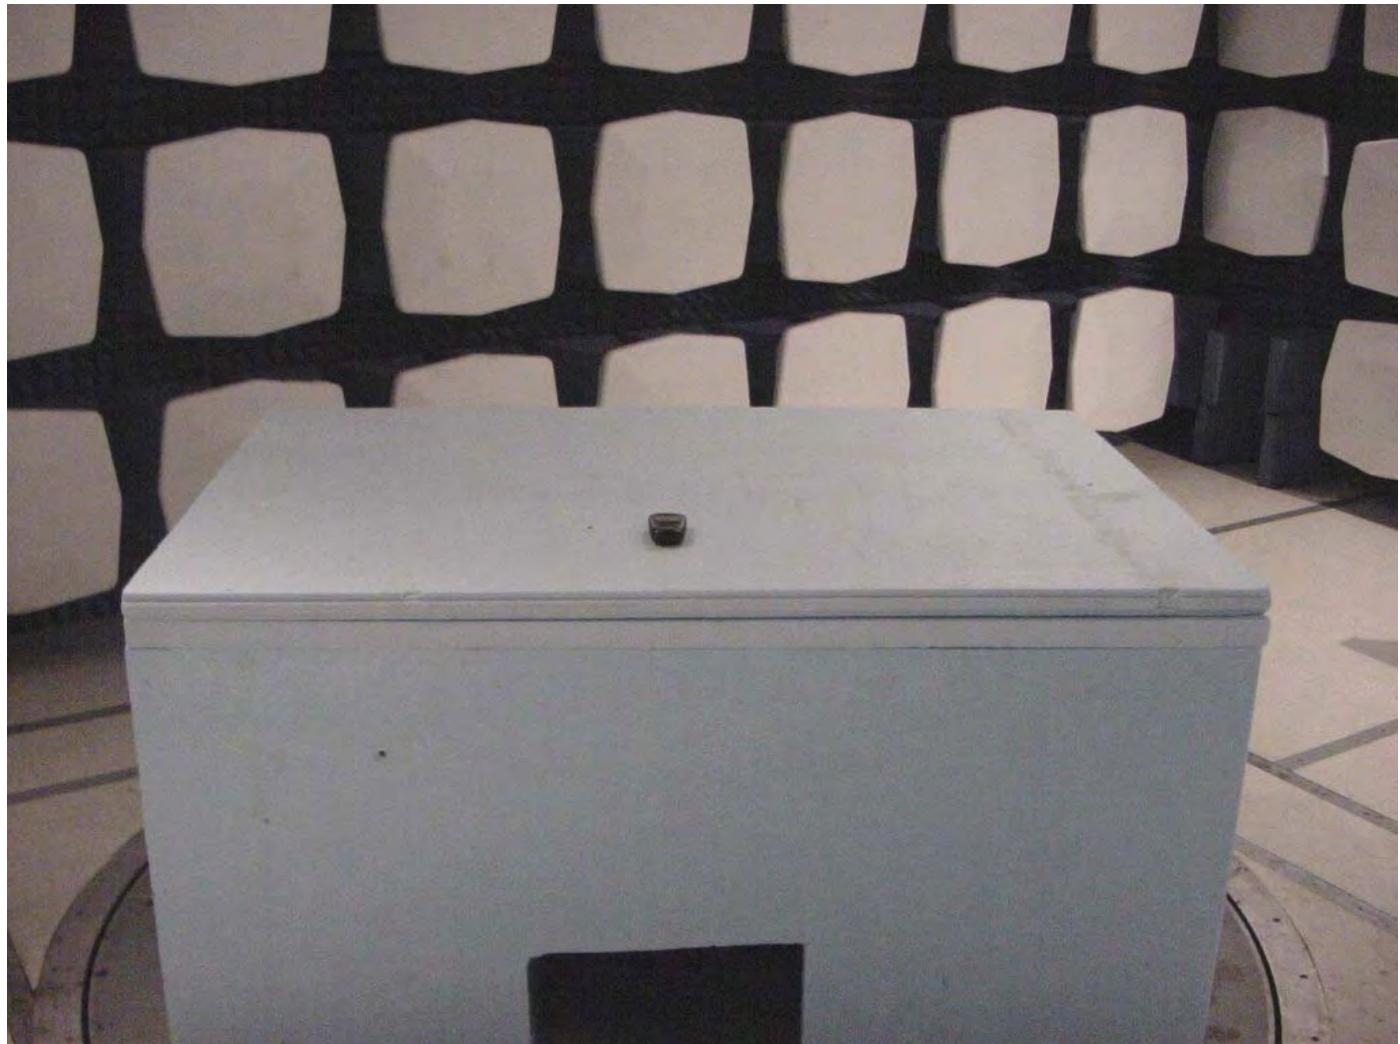

RADIATED Z AXIS



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

#### 10.0 RADIATED PHOTOS TAKEN DURING TESTING (CON'T)



RADIATED BACK



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

**1250 Peterson Dr., Wheeling, IL 60090**

## 10.0 CONDUCTED PHOTOS TAKEN DURING TESTING

### NOTE:

The conducted emissions test was not required because the Accu-Chek Aviva Combo is powered from a D.C. power source. It does not have a line cord to plug into the A.C. power line.



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## 11.0 RESULTS OF TESTS

The radio interference emission charts can be seen on the pages at the end of this report. Data sheets indicating the test measurements taken during testing can also be found at the end of this report.

## 12.0 CONCLUSION

It was found that the Accu-Chek Aviva Combo, Model Number(s) Aviva: 670 **meets** the radio interference radiated emission requirements of the FCC "Rules and Regulations", Part 15, Subpart C, Section 15.247 for operational in the 2400-2483.5 MHz Band. The conducted emissions test was not required because the Accu-Chek Aviva Combo is powered from a D.C. power source. It does not have a line cord to plug into the A.C. power line.



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

TABLE 1 – EQUIPMENT LIST

Description	Manufacturer	Model Number	Serial Number	Frequency Range	Cal Due Dates
Receiver	Rohde & Schwarz	ESI 40	837808/006	20 Hz – 40 GHz	3/10
Preamplifier	Rohde & Schwarz	TS-PR10	032001/004	9 kHz – 1 GHz	1/10
Antenna	EMCO	3104C	00054892	20 MHz – 200 MHz	4/10
Antenna	EMCO	3146	1205	200 MHz – 1 GHz	4/10
Preamp	Ciao	CA118-4010	101	1GHz-18GHz	1/10
Horn Antenna	EMCO	3115	9502-4451	1-18GHz	4/11
Filter- High-Pass	Q-Microwave	100462	2	4.2GHz-18GHz	5/10
Horn Antenna	EMCO	3115	6204	1-18GHz	5/11
Signal Generator	Rhode & Schwarz	SMR40	100092	1-40 GHz	12/09
Receiver	Rohde & Schwarz	ESI 40	837808/005	20 Hz – 40 GHz	7/10
Preamp	Miteq	AMF-8B-180265-40-10P-H/S	438727	18GHz-26GHz	9/09
Horn Antenna	ETS Lindgren	3116	00062917	18 – 40GHz	11/09
High Pass Filter	Planar	CL22500-9000-CD-SS	PF1229/0728	15-40 GHz	7/10

All primary equipment is calibrated against known reference standards with a verified traceable path to NIST.



1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

## APPENDIX A

### TEST PROCEDURE

Part 15, Subpart C, Section 15.207

ANSI C63.4-2003



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX A

### 1.0 AC POWER LINE CONDUCTED EMISSION MEASUREMENTS

If applicable, the conducted emissions were measured over the frequency range from 150 kHz to 30 MHz in accordance with the power line measurements as specified in the American National Standards Institute, ANSI C63.4-2003, Section 12. Since the device is operated from the public utility lines, the 115 Vac 60 Hz power leads, high and low sides, were to be measured by connecting the measuring equipment to the appropriate meter terminal of the LISN. All signals were then recorded. The allowed levels for Intentional Radiators cannot exceed the following:

Frequency of Emissions (MHz)	Conducted Limits (dBuV)	
	Quasi Peak	Average
.15 to .5	66 to 56	56 to 46
.5 to 5	56	46
5 to 30	60	50

#### NOTE:

The conducted emissions test was not required because the Accu-Chek Aviva Combo is powered from a D.C. power source. It does not have a line cord to plug into the A.C. power line.



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

### TEST PROCEDURE

Part 15, Subpart C, Section 15.247 (a-h)

OPERATION WITHIN THE BAND 902-928 MHz,

2400-2483.5 MHz AND 5725-5857 MHz

FCC Public Notice DA 00-705, March 30, 2000 (FHSS)

**NOTE:**

Per the FCC's Public Notice "Filing and Measurement Guidelines for Frequency Hopping Spread Spectrum Systems under DA 00-705 - March 30, 2000", as indicated in the test data section of this test report.



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

### 1.0 SPURIOUS EMISSIONS AT ANTENNA TERMINALS – PART 15.247(d), 15.203 & Per the FCC's Public Notice "Filing and Measurement Guidelines for Frequency Hopping Spread Spectrum Systems under DA 00-705 - March 30, 2000", as indicated in the test data section of this test report.

Spurious conducted emissions were measured at the antenna terminals. Plots were made showing the amplitude of each harmonic emission with the equipment operated. As shown by the radiated charts there was no reason to believe that there were any spurious emissions other than the harmonics that were than individually investigated when doing the conducted test at the antenna terminals. Measurements were made up to the 10<sup>th</sup> harmonic of the fundamental.

As stated in 15.203 the Accu-Chek Aviva Combo was designed to ensure that no antenna other than that furnished by Roche Diagnostics Operations Inc will be used with the EUT. The use of a permanently attached antenna or antenna that uses an unique coupling to the intentional radiator was considered to comply with section 15.203.

The allowed emissions for transmitters operating in the 2400 MHz - 2483.5 MHz bands for Accu-Chek Aviva Combo equipment are found under Part 15, Section 15.247(d). This paragraph states that in any 100 kHz bandwidth outside the frequency band which the spread spectrum intentional radiator is operating, the radio frequency power produced by the intentional radiator shall be at least 20 dB below that in the 100 kHz bandwidth within the band that contains the highest level of the desired power.

**NOTE: See the following pages for the data and graphs of the actual measurements made:**



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

# RF CONDUCTED EMISSION DATA AND GRAPH(S)

TAKEN FOR

SPURIOUS EMISSION MEASUREMENTS MADE

AT THE ANTENNA TERMINALS

PART 15.247(d)



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090


## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Conducted Spurious Emissions  
Operator: Adam A  
Comment: **Low Channel:** Frequency – 2.402 GHz

Frequency Range: 30 to 1000 MHz

Limit = -15.69 dBm

All Spurious Emissions at Least 20 dB below Peak Level of In Band Frequency

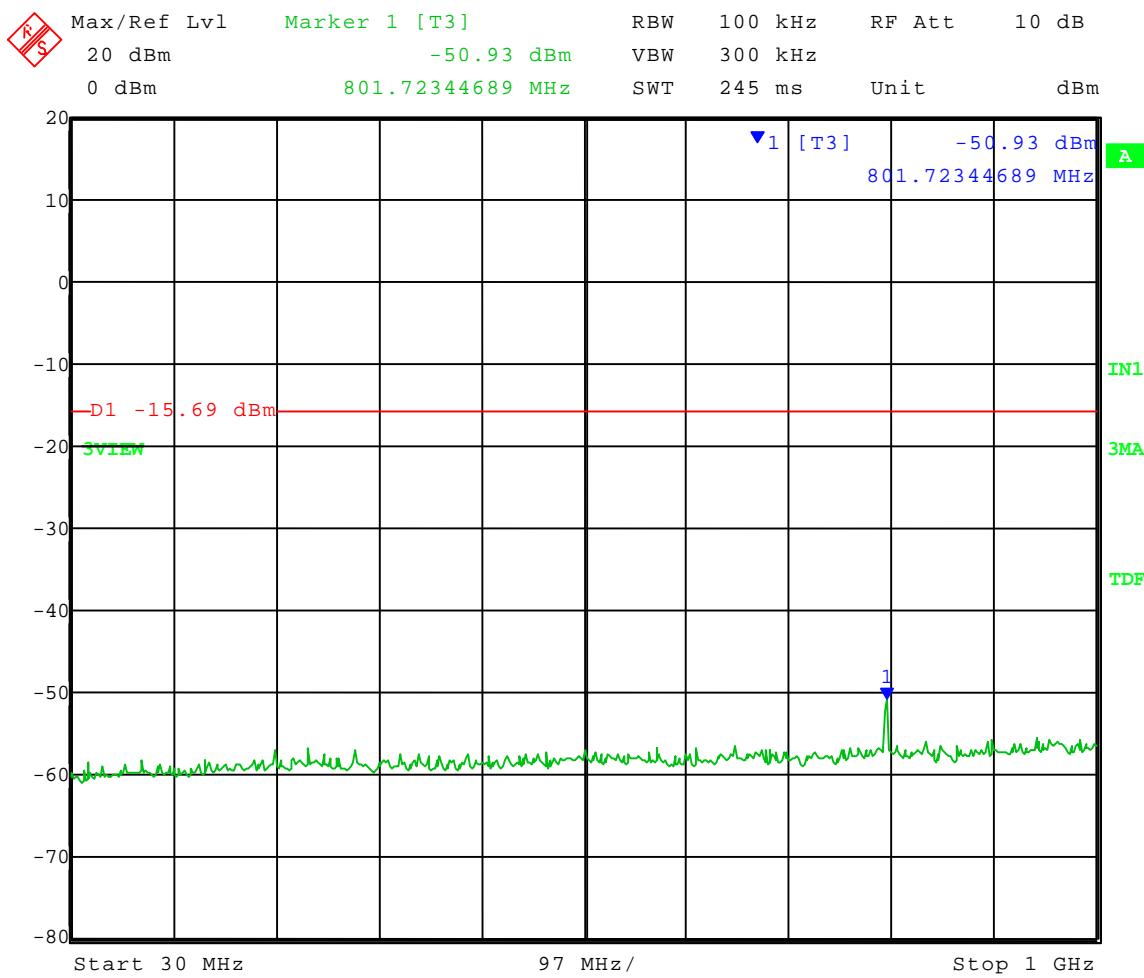

Date: 10.AUG.2009 11:10:42



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090


## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Conducted Spurious Emissions  
Operator: Adam A  
Comment: **Low Channel:** Frequency – 2.402 GHz

Frequency Range: 1 to 10 GHz

Limit = -15.69 dBm

All Spurious Emissions at Least 20 dB below Peak Level of In Band Frequency

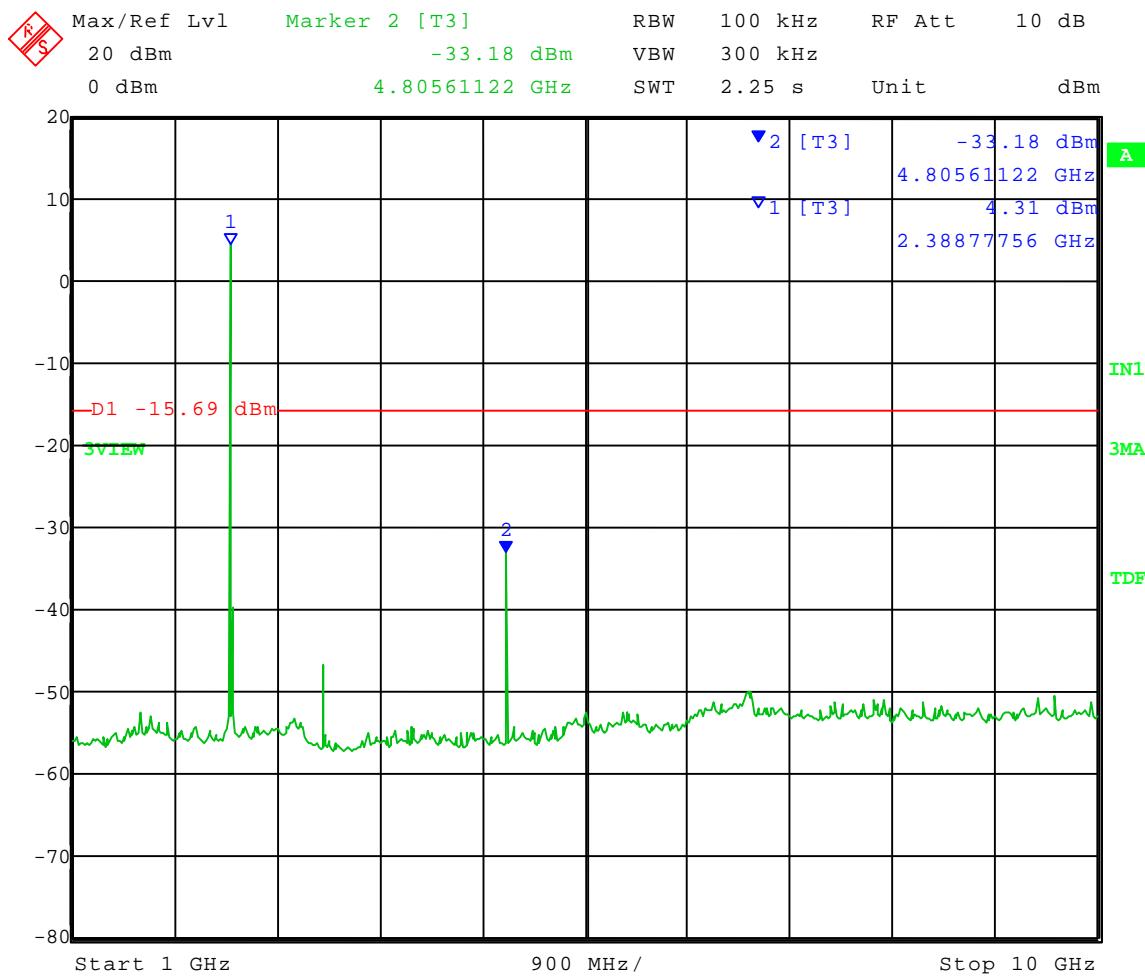



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090


## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Conducted Spurious Emissions  
Operator: Adam A  
Comment: **Low Channel:** Frequency – 2.402 GHz

Frequency Range: 10 to 18 GHz

Limit = -15.69 dBm

All Spurious Emissions at Least 20 dB below Peak Level of In Band Frequency

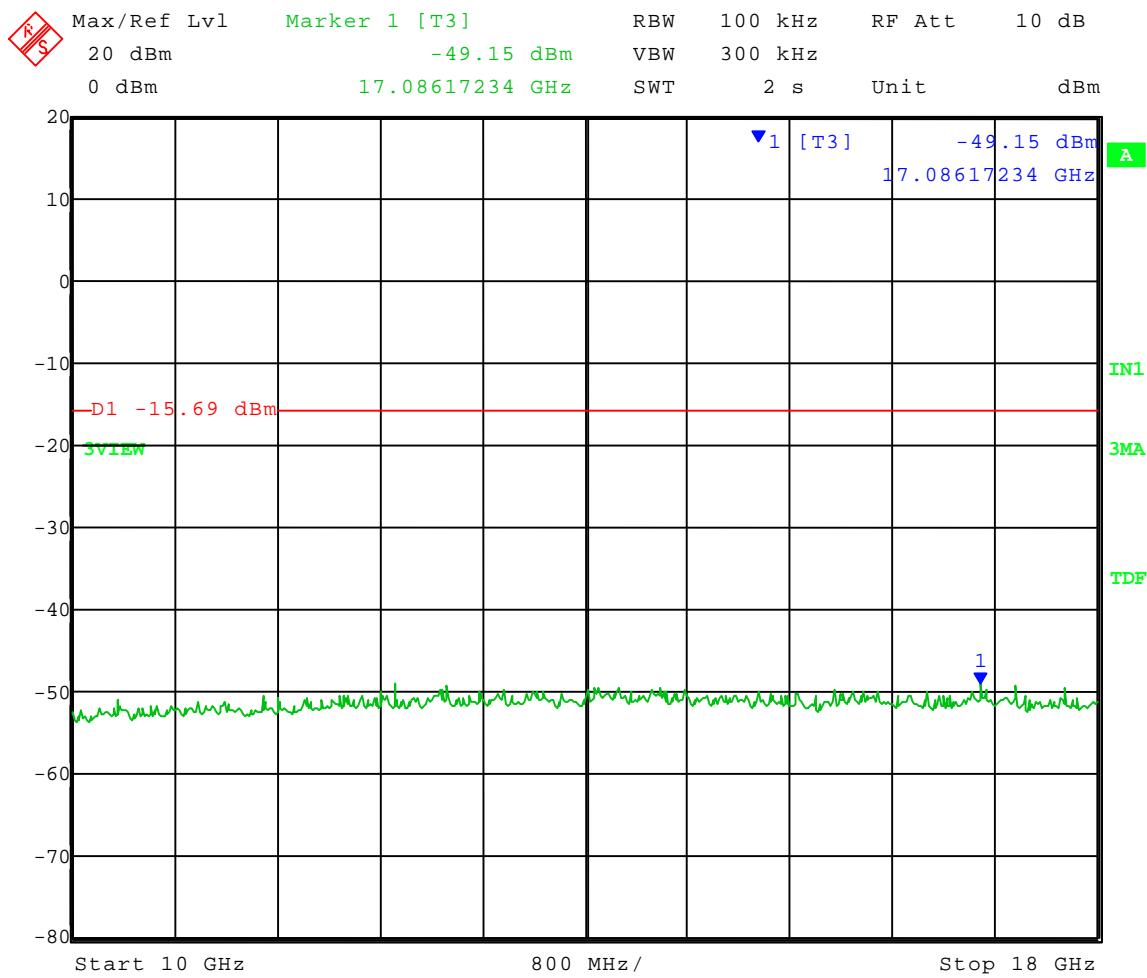

Date: 10.AUG.2009 11:07:26



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090


## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Conducted Spurious Emissions  
Operator: Adam A  
Comment: **Low Channel:** Frequency – 2.402 GHz

Frequency Range: 18 to 26 GHz

Limit = -15.69 dBm

All Spurious Emissions at Least 20 dB below Peak Level of In Band Frequency

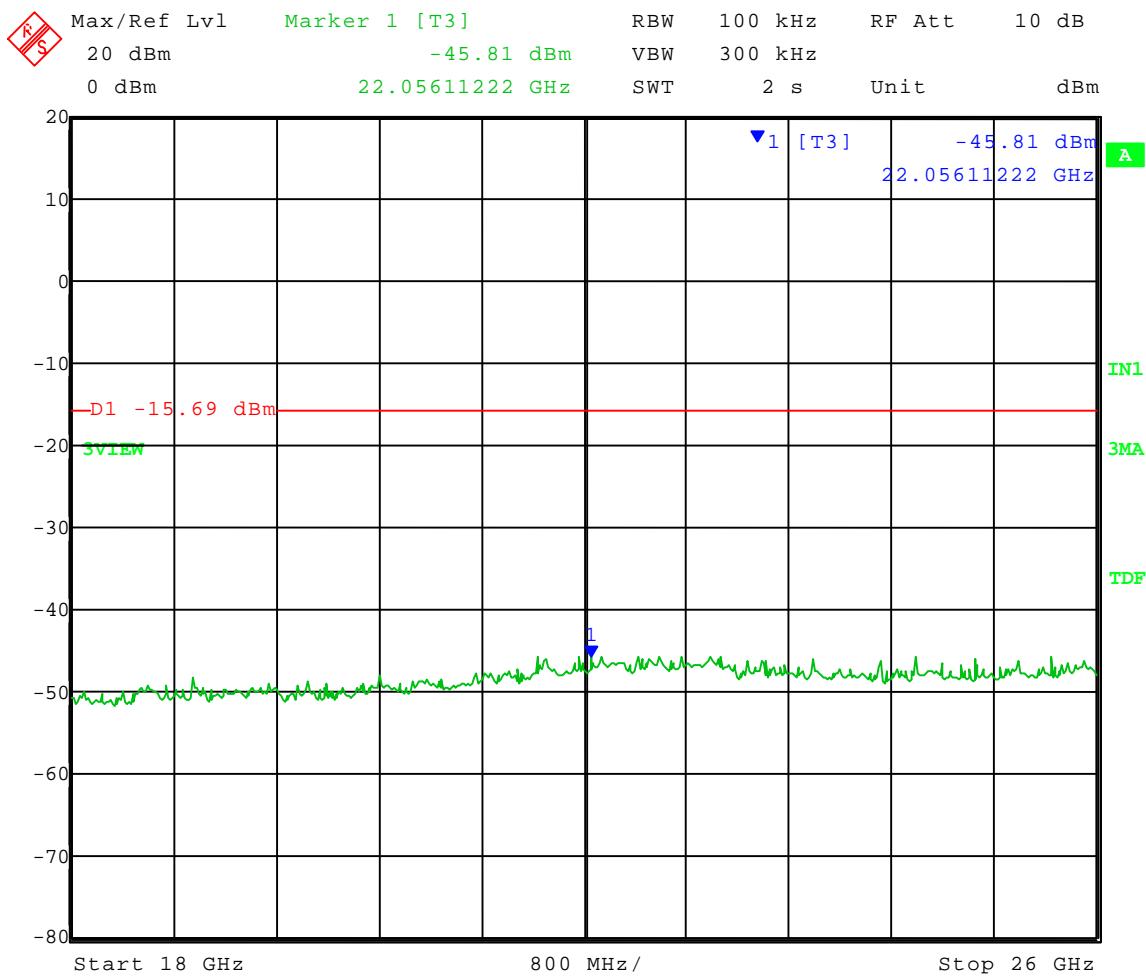



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090


## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Conducted Spurious Emissions  
Operator: Adam A  
Comment: **Mid Channel: Frequency – 2.441 GHz**

Frequency Range: 30 to 1000 MHz

Limit = -15.67 dBm

All Spurious Emissions at Least 20 dB below Peak Level of In Band Frequency

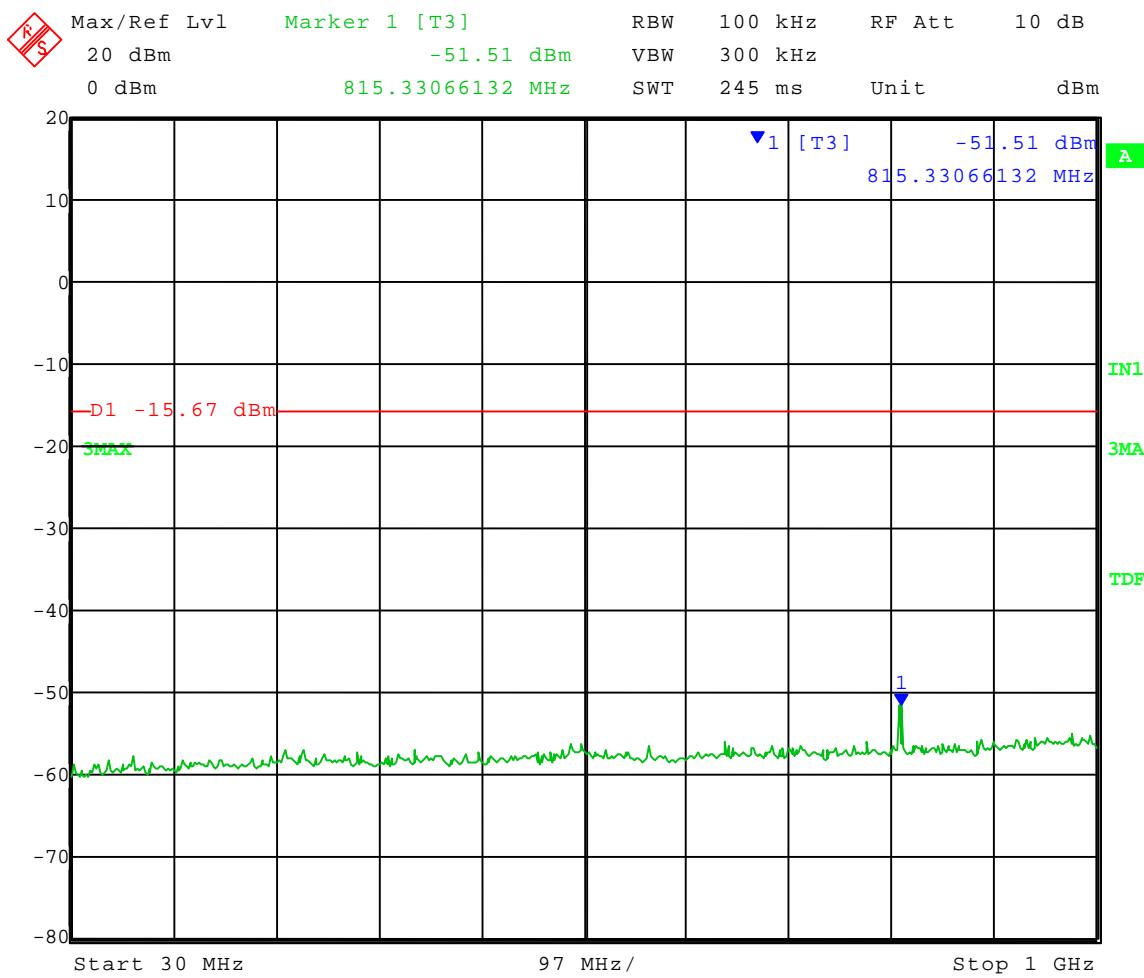

Date: 10.AUG.2009 10:54:45



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090


## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Conducted Spurious Emissions  
Operator: Adam A  
Comment: **Mid Channel:** Frequency – 2.441 GHz

Frequency Range: 1 to 10 GHz

Limit = -15.67 dBm

All Spurious Emissions at Least 20 dB below Peak Level of In Band Frequency

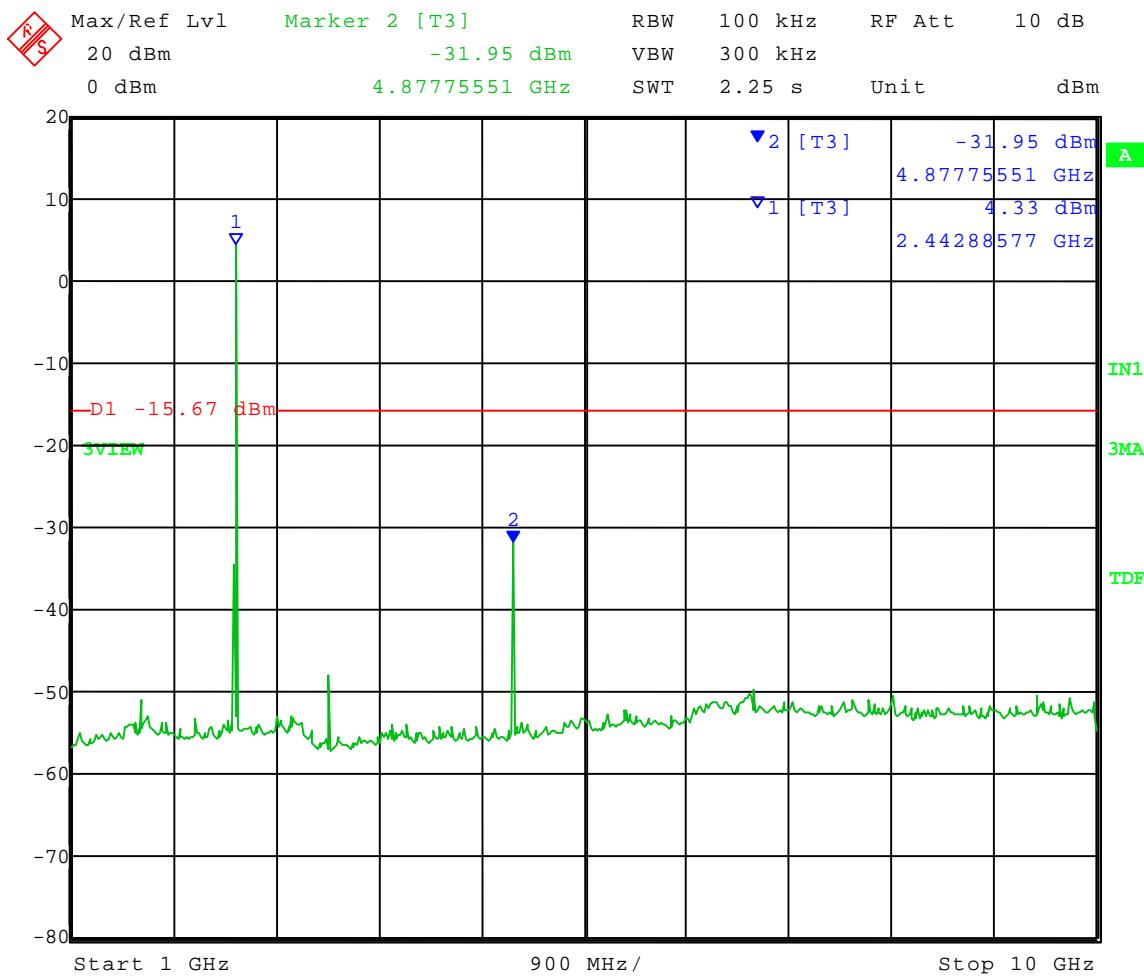

Date: 10.AUG.2009 10:51:17



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090


## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Conducted Spurious Emissions  
Operator: Adam A  
Comment: **Mid Channel:** Frequency – 2.441 GHz

Frequency Range: 10 to 18 GHz

Limit = -15.67 dBm

All Spurious Emissions at Least 20 dB below Peak Level of In Band Frequency

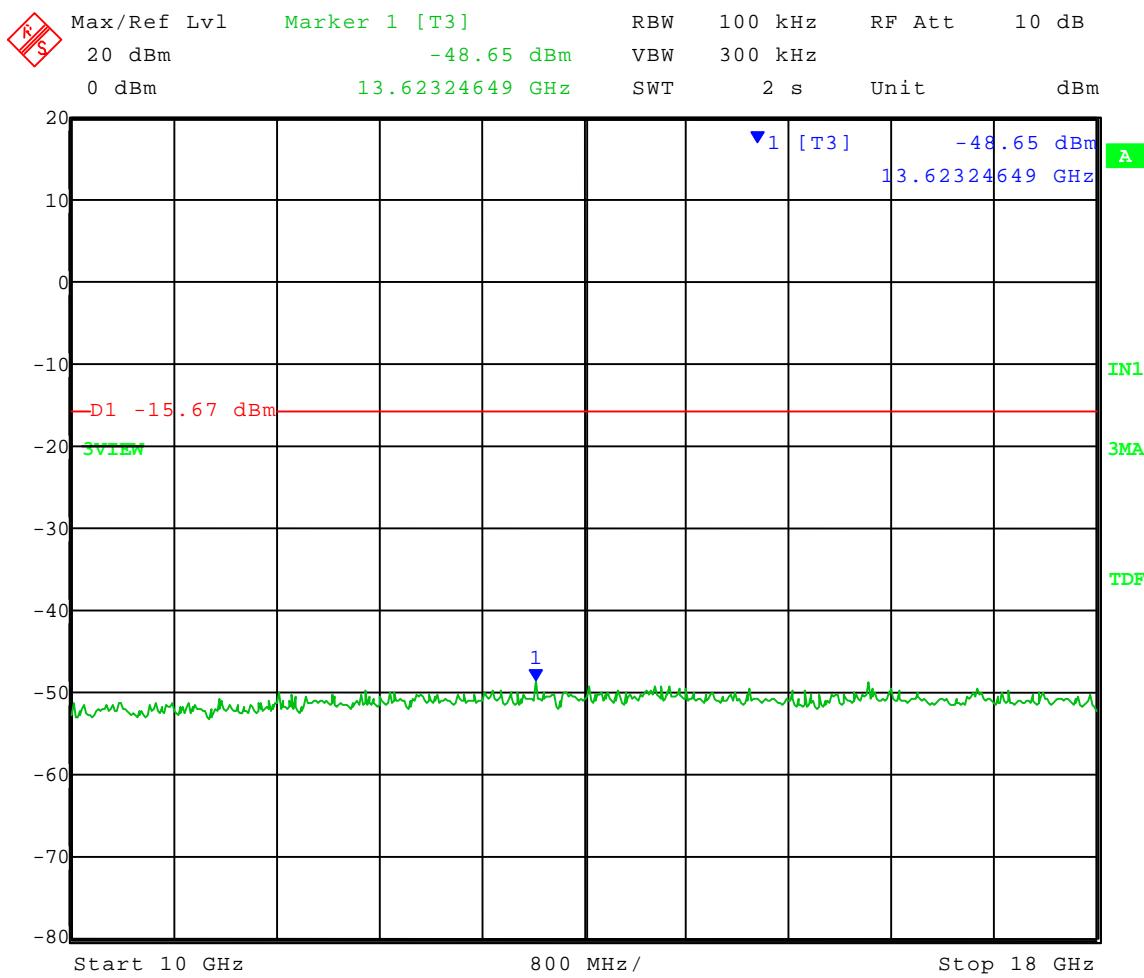

Date: 10.AUG.2009 10:52:26



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090


## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Conducted Spurious Emissions  
Operator: Adam A  
Comment: **Mid Channel:** Frequency – 2.441 GHz

Frequency Range: 18 to 26 GHz

Limit = -15.67 dBm

All Spurious Emissions at Least 20 dB below Peak Level of In Band Frequency

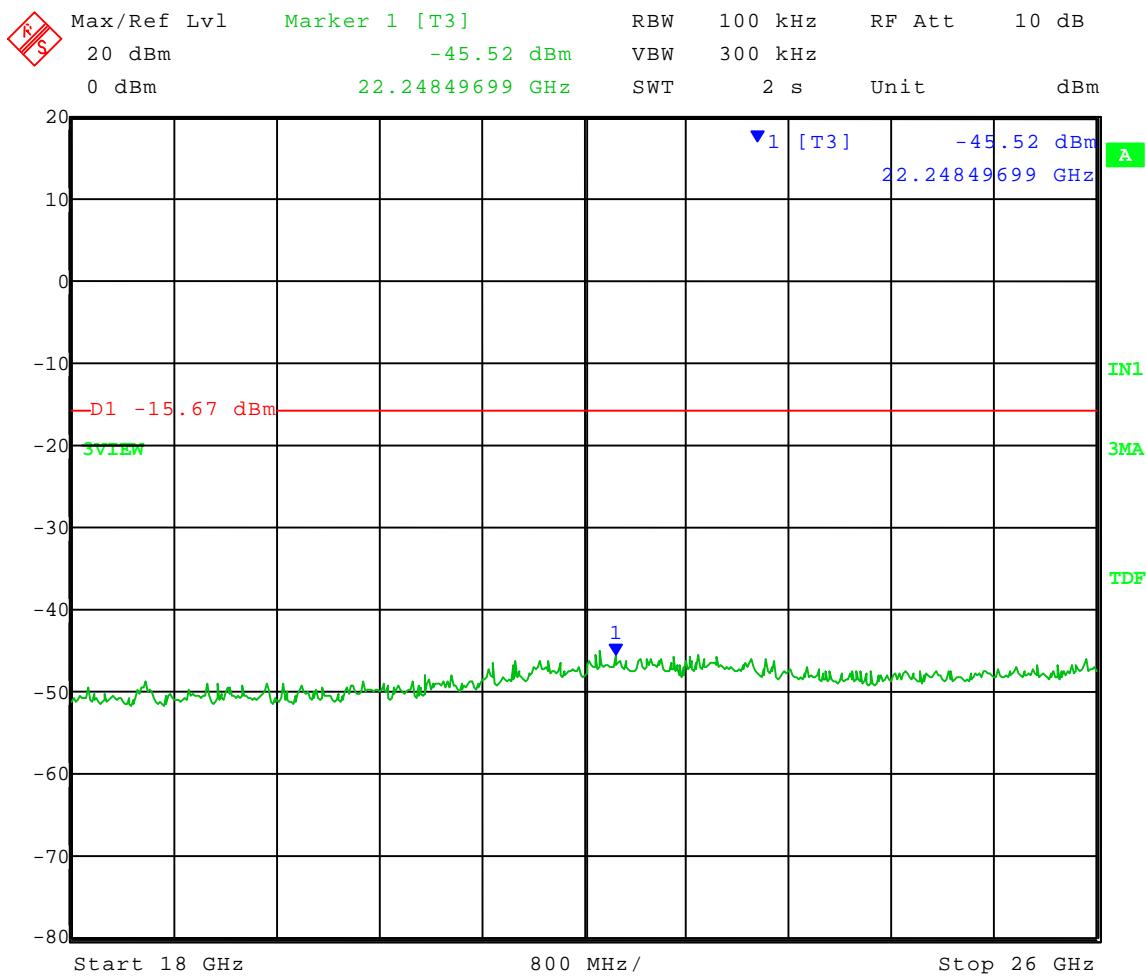



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090


## APPENDIX B

Test Date: 8-07-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Conducted Spurious Emissions  
Operator: Adam A  
Comment: **High Channel:** Frequency – 2.480 GHz

Frequency Range: 30 to 1000 MHz

Limit = -15.6 dBm

All Spurious Emissions at Least 20 dB below Peak Level of In Band Frequency

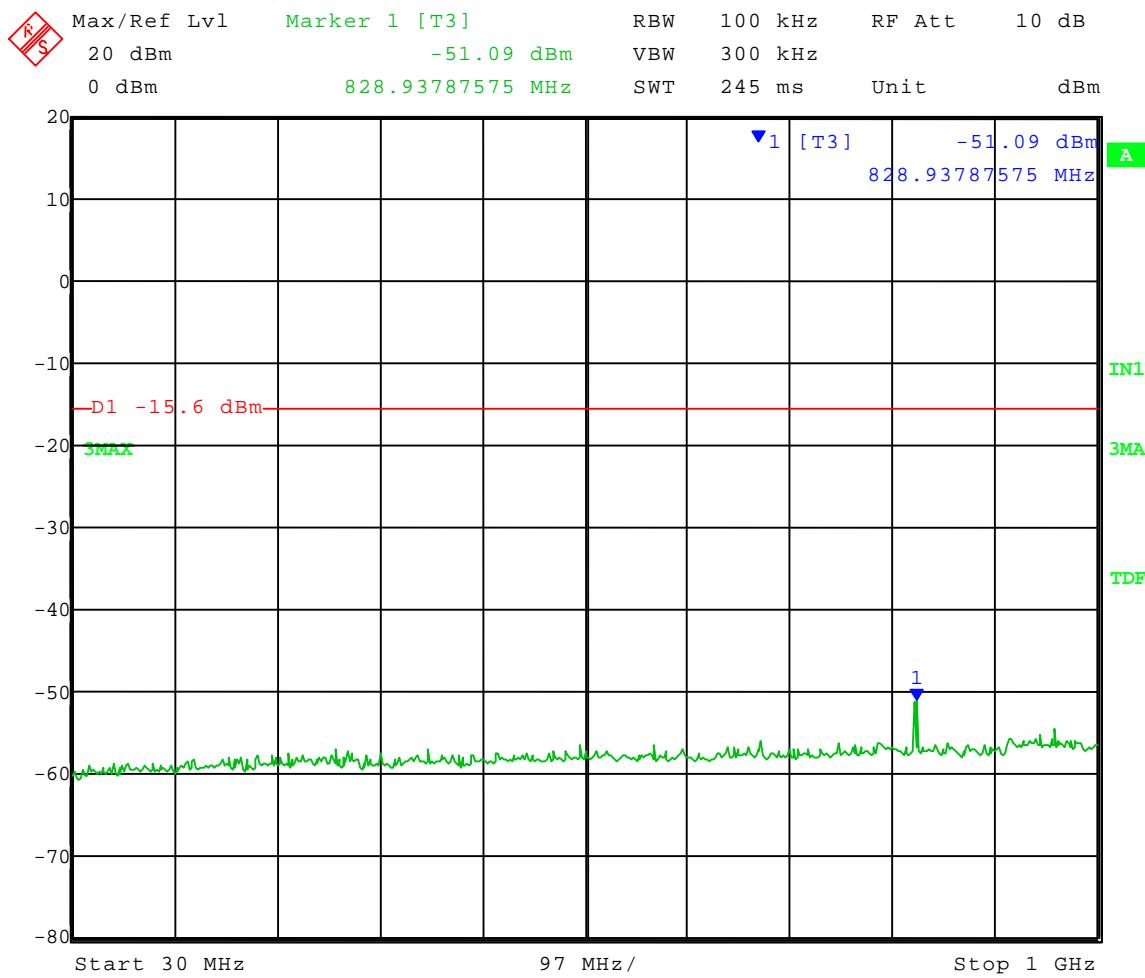

Date: 7.AUG.2009 14:07:27



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090


## APPENDIX B

Test Date: 8-07-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Conducted Spurious Emissions  
Operator: Adam A  
Comment: **High Channel:** Frequency – 2.480 GHz

Frequency Range: 1 to 10 GHz

Limit = -15.6 dBm

All Spurious Emissions at Least 20 dB below Peak Level of In Band Frequency

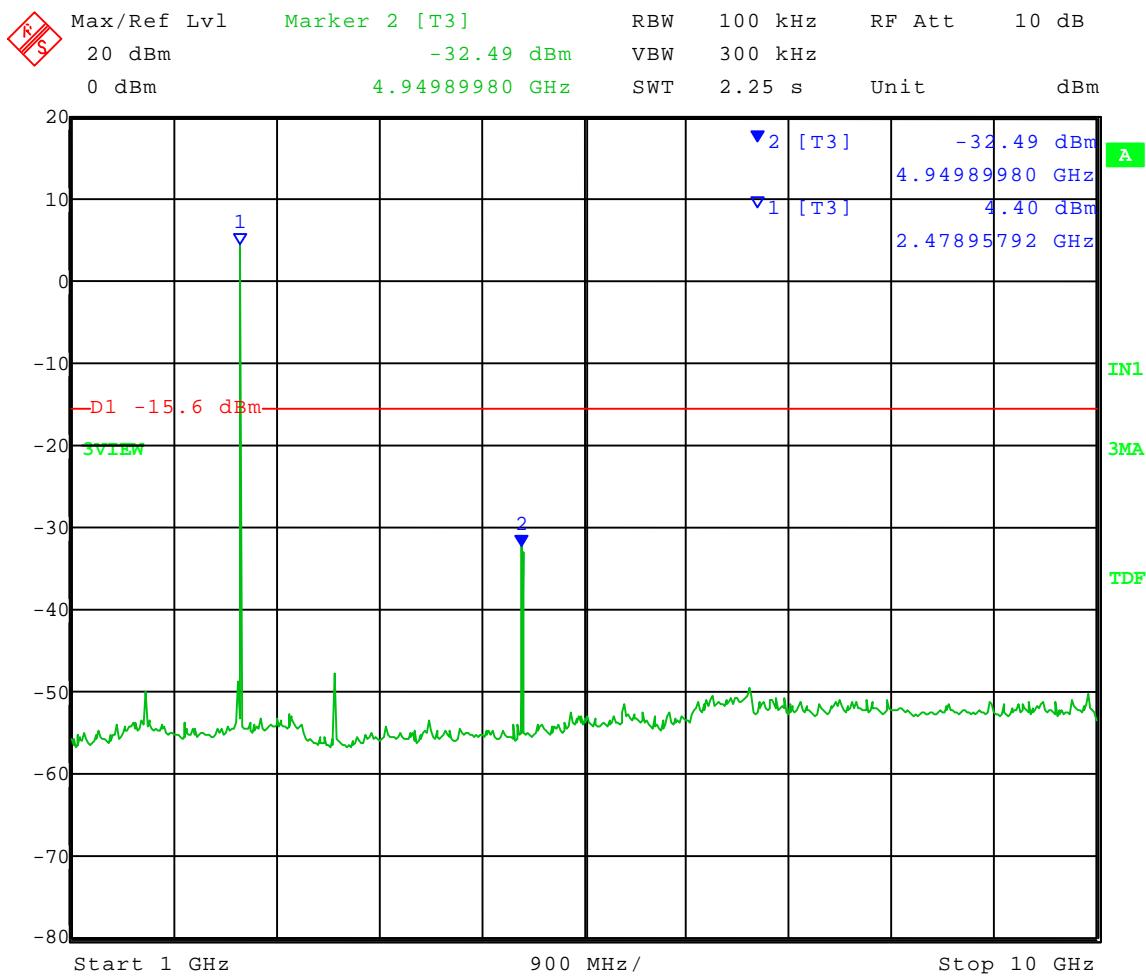

Date: 7.AUG.2009 14:03:01



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090


## APPENDIX B

Test Date: 8-07-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Conducted Spurious Emissions  
Operator: Adam A  
Comment: **High Channel:** Frequency – 2.480 GHz

Frequency Range: 10 to 18 GHz

Limit = -15.6 dBm

All Spurious Emissions at Least 20 dB below Peak Level of In Band Frequency

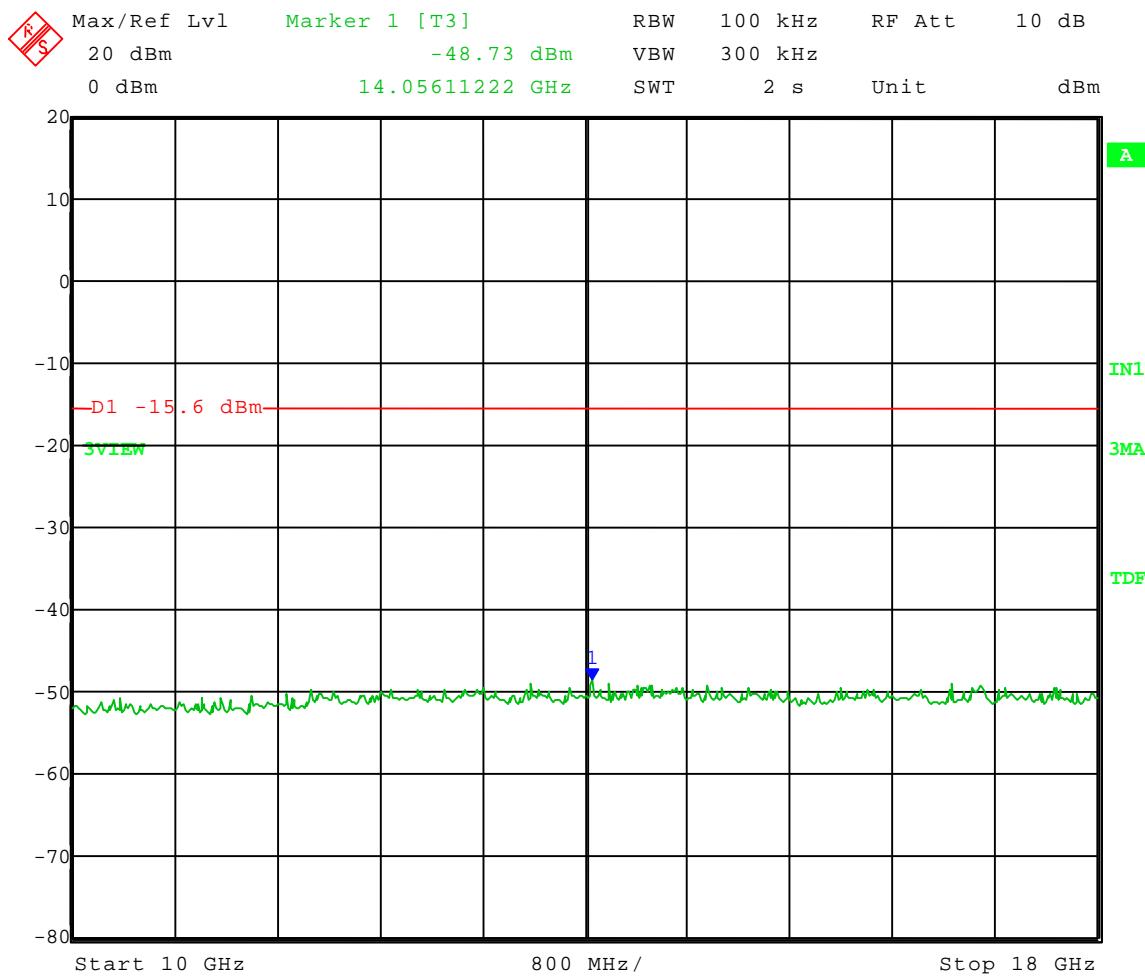

Date: 7.AUG.2009 14:04:55



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090


## APPENDIX B

Test Date: 8-07-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Conducted Spurious Emissions  
Operator: Adam A  
Comment: **High Channel:** Frequency – 2.480 GHz

Frequency Range: 18 to 26 GHz

Limit = -15.6 dBm

All Spurious Emissions at Least 20 dB below Peak Level of In Band Frequency

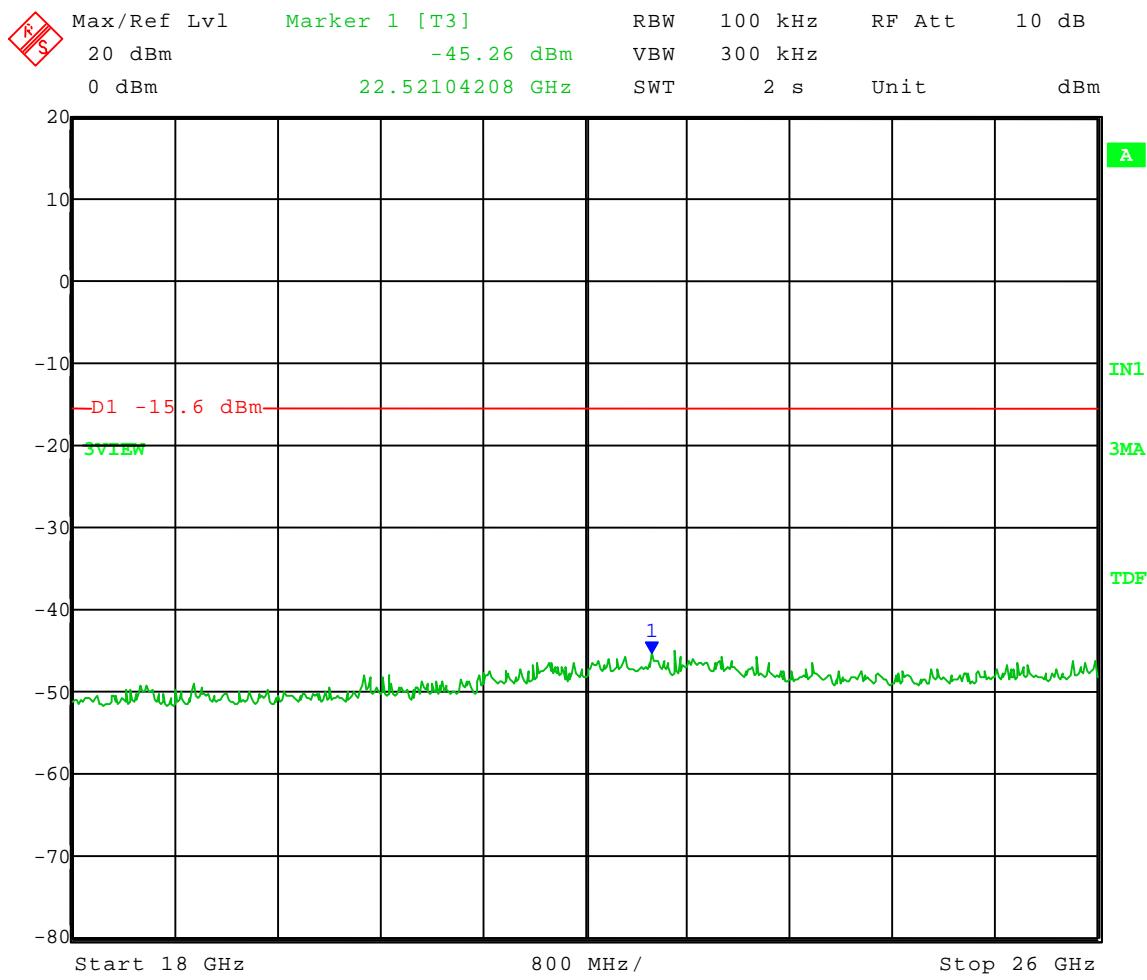

Date: 7.AUG.2009 14:06:07



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

### 2.0 RF CONDUCTED EMISSIONS (ANTENNA TERMINAL) PHOTOS TAKEN DURING TESTING



RF CONDUCTED



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

### 3.0 RESTRICTED BANDS

As stated in Section 15.205a, the fundamental emission from the Accu-Chek Aviva Combo shall not fall within any of the bands listed below:

Frequency in MHz	Frequency in MHz	Frequency in MHz	Frequency in GHz
.0900 to .1100	162.0125 to 167.17	2310.0 to 2390	9.30 to 9.50
.4900 to .5100	167.7200 to 173.20	2483.5 to 2500	10.60 to 12.70
2.1735 to 2.1905	240.000 to 285.00	2655.0 to 2900	13.25 to 13.40
8.362 to 8.3660	322.200 to 335.40	3260.0 to 3267	14.47 to 14.50
13.36 to 13.410	399.900 to 410.00	3332.0 to 3339	15.35 to 16.20
25.50 to 25.670	608.000 to 614.00	3345.8 to 3358	17.70 to 21.40
37.50 to 38.250	960.000 to 1240.00	3600.0 to 4400	22.01 to 23.13
73.00 to 75.500	1300.000 to 1427.00	4500.0 to 5250	23.60 to 24.00
108.00 to 121.94	1435.000 to 1626.50	5350.0 to 5450	31.20 to 31.80
123.00 to 138.00	1660.000 to 1710.00	7250.0 to 7750	36.43 to 36.50
149.90 to 150.00	1718.800 to 1722.20	8025.0 to 8500	ABOVE 38.60
156.70 to 156.90	2200.000 to 2300.00	9000.0 to 9200	

#### NOTE:

The noise floor within the Restricted Bands for the EMC Receiver will typically lay 20 dB below the limit.

### 4.0 RESTRICTED BAND AND BAND EDGE COMPLIANCE

In any 100 kHz bandwidth outside the frequency band in which the spread spectrum intentional radiator is operating, the attenuation below the general limits specified in 15.209 is not required.

The field strength of any **radiated emissions** which fall within the restricted bands shall not exceed the general radiated emissions limits as stated Section 15.209.

**NOTE:** See the following page(s) for the graph(s) made showing compliance for Restricted Band and Band Edge Compliance:



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

# DATA AND GRAPH(S) TAKEN SHOWING

## THE RESTRICTED BAND COMPLIANCE

PART 15.247(d) & 15.205



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

### Radiated Restricted Band – 30 MHz to 26 GHz

**30 MHz – 18 GHz Tested at a 3 Meter Distance**

**18 – 26 GHz Tested at a 1 Meter Distance**

**EUT:** Accu-Check Aviva Combo

**Manufacturer:** Roche Diagnostics

**Operating Condition:** 71 deg F; 54% R.H.

**Test Site:** Chamber G1

**Operator:** Adam A

**Test Specification:** FCC Part 15.247

**Comment:** Continuous transmit – Low channel: 2402 MHz

**Date:** 8/06/2009

**Notes:** (1) Peak measurements were taken with RBW = 1 MHz, VBW = 3 MHz

(2) Average measurements were taken with RBW = 1 MHz, VBW = 10 Hz

(3) All other restricted band emissions at least 20 dB under the limit.

Frequency (GHz)	Measurement Type	Ant. Pol.	Level (dBuV)	Antenna Factor (dB/m)	System Loss (dB)	Total Level (dBuV/m)	Duty Cycle Correction (dB)	Final Corrected (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Comment
4.804	Average	Vert	56.32	32.88	-31.9	57.30	20	37.30	54	16.7	Res. Band
4.804	Max Peak	Vert	64.03	32.88	-31.9	65.01		65.01	74	8.99	Res. Band
4.804	Average	Horz	56.38	32.88	-31.9	57.36	20	37.36	54	16.64	Res. Band
4.804	Max Peak	Horz	63.79	32.88	-31.9	64.77		64.77	74	9.23	Res. Band



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

### Radiated Restricted Band – 30 MHz to 26 GHz

**30 MHz – 18 GHz Tested at a 3 Meter Distance**

**18 – 26 GHz Tested at a 1 Meter Distance**

**EUT:** Accu-Check Aviva Combo  
**Manufacturer:** Roche Diagnostics  
**Operating Condition:** 72 deg F; 59% R.H.  
**Test Site:** Chamber G1  
**Operator:** Adam A  
**Test Specification:** FCC Part 15.247  
**Comment:** Continuous transmit – **Mid channel:** 2441 MHz  
**Date:** 8/07/2009

**Notes:** (1) Peak measurements were taken with RBW = 1 MHz, VBW = 3 MHz  
(2) Average measurements were taken with RBW = 1 MHz, VBW = 10 Hz  
(3) All other restricted band emissions at least 20 dB under the limit.

Frequency (GHz)	Measurement Type	Ant. Pol.	Level (dBuV)	Antenna Factor (dB/m)	System Loss (dB)	Total Level (dBuV/m)	Duty Cycle Correction (dB)	Final Corrected (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Comment
4.882	Average	Vert	57.57	32.98	-31.8	58.75	20	38.75	54	15.25	Res. Band
4.882	Max Peak	Vert	65.46	32.98	-31.8	66.64		66.64	74	7.36	Res. Band
4.882	Average	Horz	55.42	32.98	-31.8	56.60	20	36.60	54	17.4	Res. Band
4.882	Max Peak	Horz	63.01	32.98	-31.8	64.17		64.17	74	9.83	Res. Band
7.323	Average	Vert	44.72	36.09	-28.8	52.01	20	32.01	54	21.99	Res. Band
7.323	Max Peak	Vert	54.04	36.09	-28.8	61.33		61.33	74	12.67	Res. Band
7.323	Average	Horz	44.07	36.09	-28.8	51.36	20	31.36	54	22.64	Res. Band
7.323	Max Peak	Horz	53.53	36.09	-28.8	60.82		60.82	74	13.18	Res. Band



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

### Radiated Restricted Band – 30 MHz to 26 GHz

**30 MHz – 18 GHz Tested at a 3 Meter Distance**

**18 – 26 GHz Tested at a 1 Meter Distance**

**EUT:** Accu-Check Aviva Combo

**Manufacturer:** Roche Diagnostics

**Operating Condition:** 72 deg F; 59% R.H.

**Test Site:** Chamber G1

**Operator:** Adam A

**Test Specification:** FCC Part 15.247

**Comment:** Continuous transmit – **High channel:** 2480 MHz

**Date:** 8/07/2009

**Notes:** (1) Peak measurements were taken with RBW = 1 MHz, VBW = 3 MHz

(2) Average measurements were taken with RBW = 1 MHz, VBW = 10 Hz

(3) All other restricted band emissions at least 20 dB under the limit.

Frequency (GHz)	Measurement Type	Ant. Pol.	Level (dBuV)	Antenna Factor (dB/m)	System Loss (dB)	Total Level (dBuV/m)	Duty Cycle Correction (dB)	Final Corrected (dBuV/m)	Limit (dBuV/m)	Margin (dB)	Comment
4.960	Average	Vert	59.45	33.08	-31.9	60.63	20	40.63	54	13.37	Res. Band
4.960	Max Peak	Vert	67.58	33.08	-31.9	68.76		68.76	74	5.24	Res. Band
4.960	Average	Horz	57.95	33.08	-31.9	59.13	20	39.13	54	14.87	Res. Band
4.960	Max Peak	Horz	65.88	33.08	-31.9	67.06		67.06	74	6.94	Res. Band
7.440	Average	Vert	45.48	36.4	-28.0	53.88	20	33.88	54	20.12	Res. Band
7.440	Max Peak	Vert	54.49	36.4	-28.0	62.89		62.89	74	11.11	Res. Band
7.440	Average	Horz	42.23	36.4	-28.0	50.63	20	30.63	54	23.37	Res. Band
7.440	Max Peak	Horz	52.23	36.4	-28.0	60.63		60.63	74	13.37	Res. Band



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

### 20 dB BANDWIDTH

### DATA AND GRAPH(S)

### PART 15.247

#### **NOTE:**

Per the FCC's Public Notice "Filing and Measurement Guidelines for Frequency Hopping Spread Spectrum Systems under DA 00-705 - March 30, 2000", as indicated in the test data section of this test report.




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: 20 dB Bandwidth  
Operator: Adam A  
Comment: 2.402 GHz Transmit Frequency; Basic Data Rate

20 dB Bandwidth = 1.16 MHz

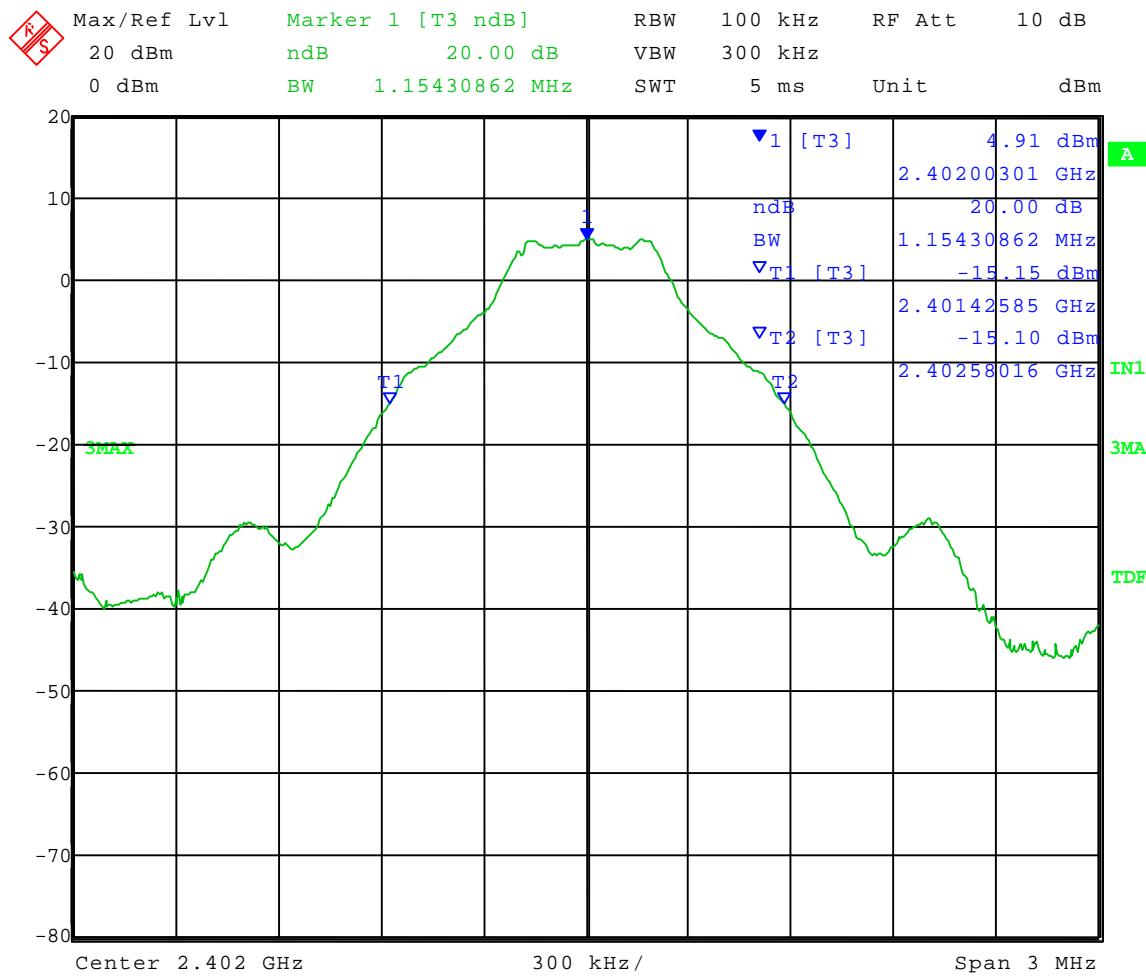




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: 20 dB Bandwidth  
Operator: Adam A  
Comment: 2.402 GHz Transmit Frequency; Enhanced Data Rate 1

20 dB Bandwidth = 1.40 MHz

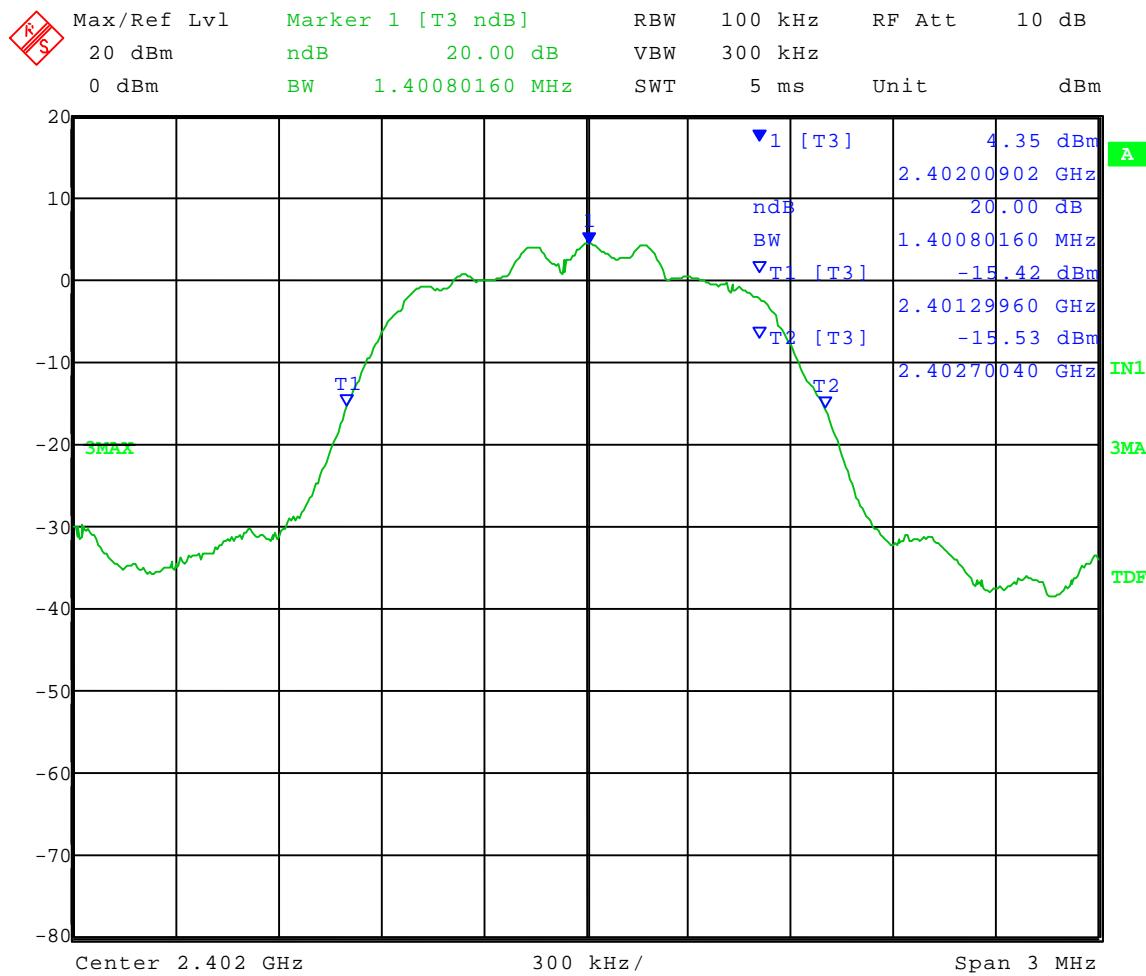

Date: 10.AUG.2009 14:21:10




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: 20 dB Bandwidth  
Operator: Adam A  
Comment: 2.402 GHz Transmit Frequency; Enhanced Data Rate 2

20 dB Bandwidth = 1.40 MHz

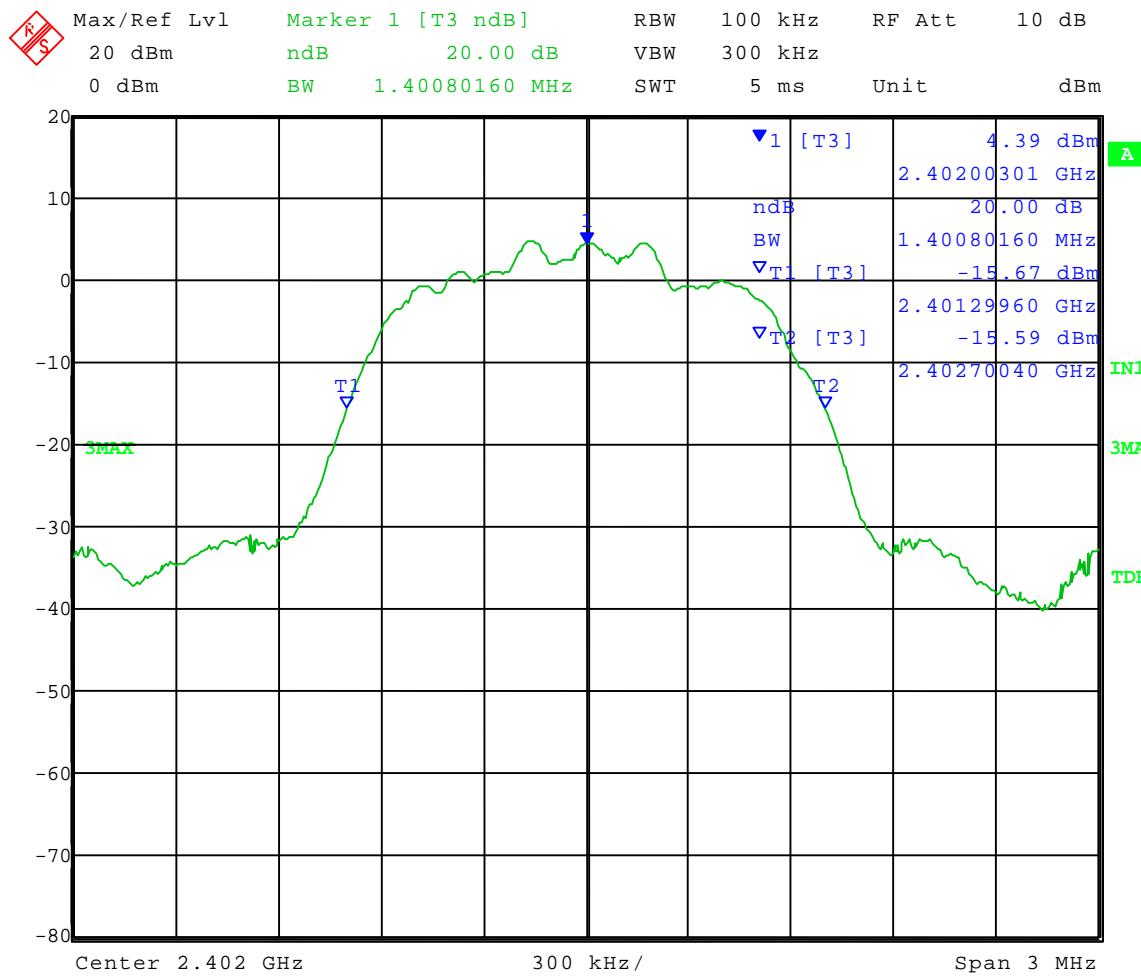




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: 20 dB Bandwidth  
Operator: Adam A  
Comment: 2.441 GHz Transmit Frequency; Basic Data Rate

20 dB Bandwidth = 1.16 MHz

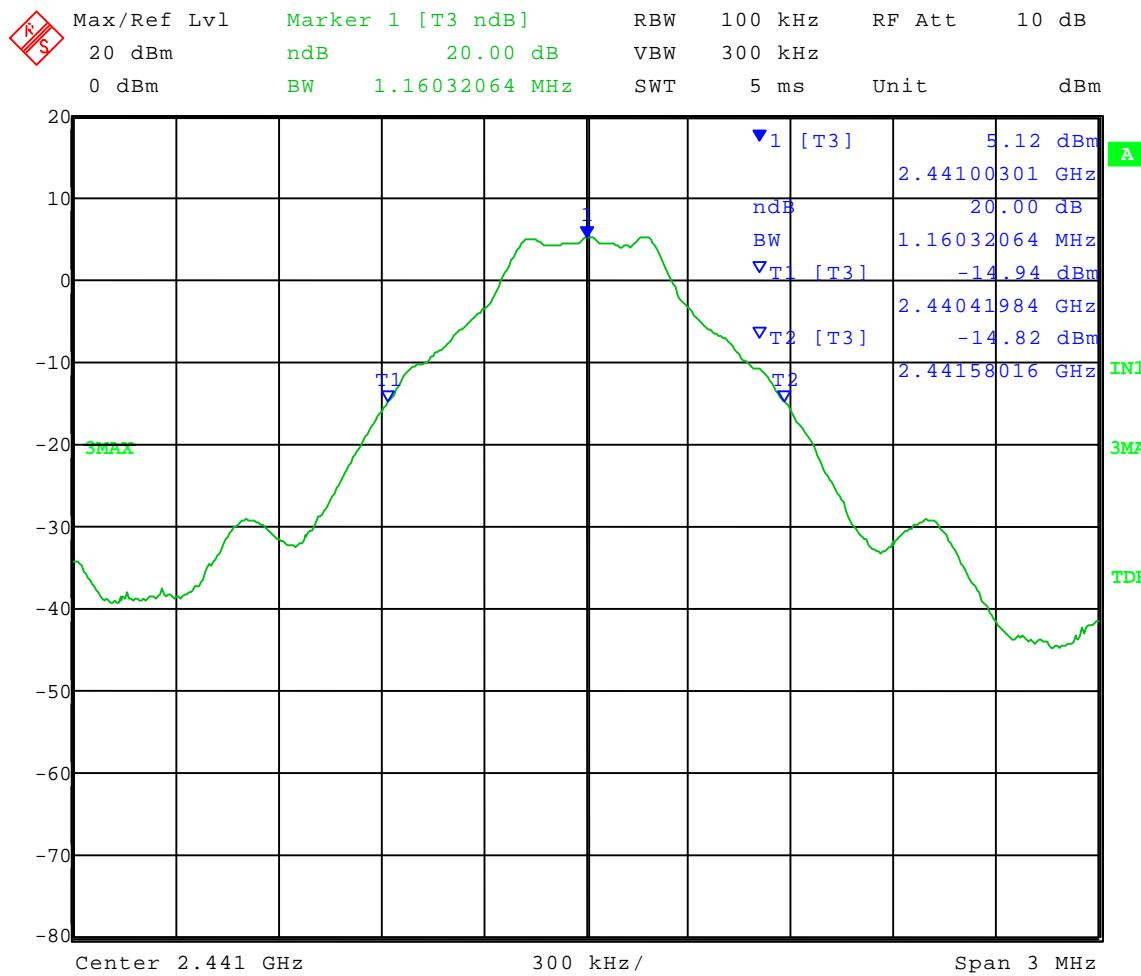




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: 20 dB Bandwidth  
Operator: Adam A  
Comment: 2.441 GHz Transmit Frequency; Enhanced Data Rate 1

20 dB Bandwidth = 1.39 MHz

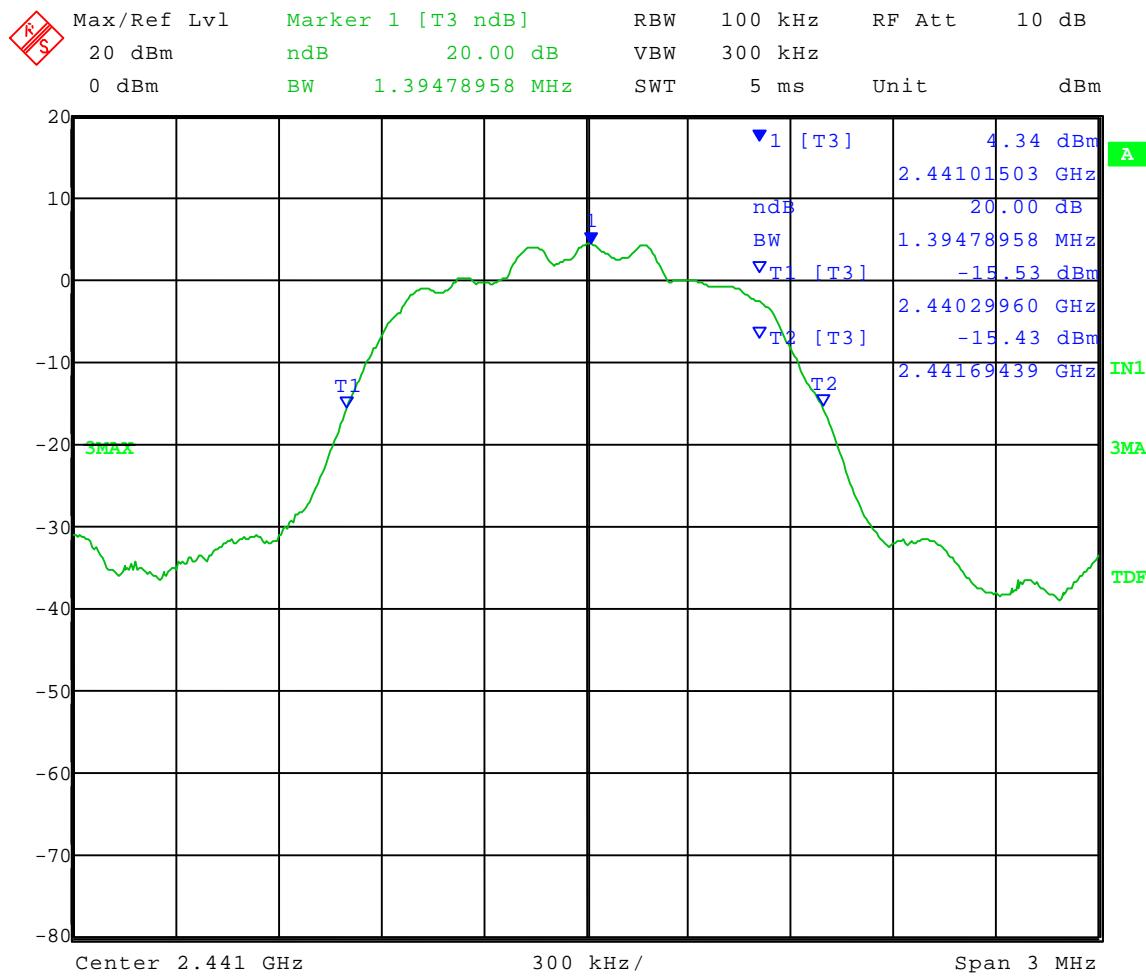

Date: 10.AUG.2009 13:40:56




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: 20 dB Bandwidth  
Operator: Adam A  
Comment: 2.441 GHz Transmit Frequency; Enhanced Data Rate 2

20 dB Bandwidth = 1.40 MHz

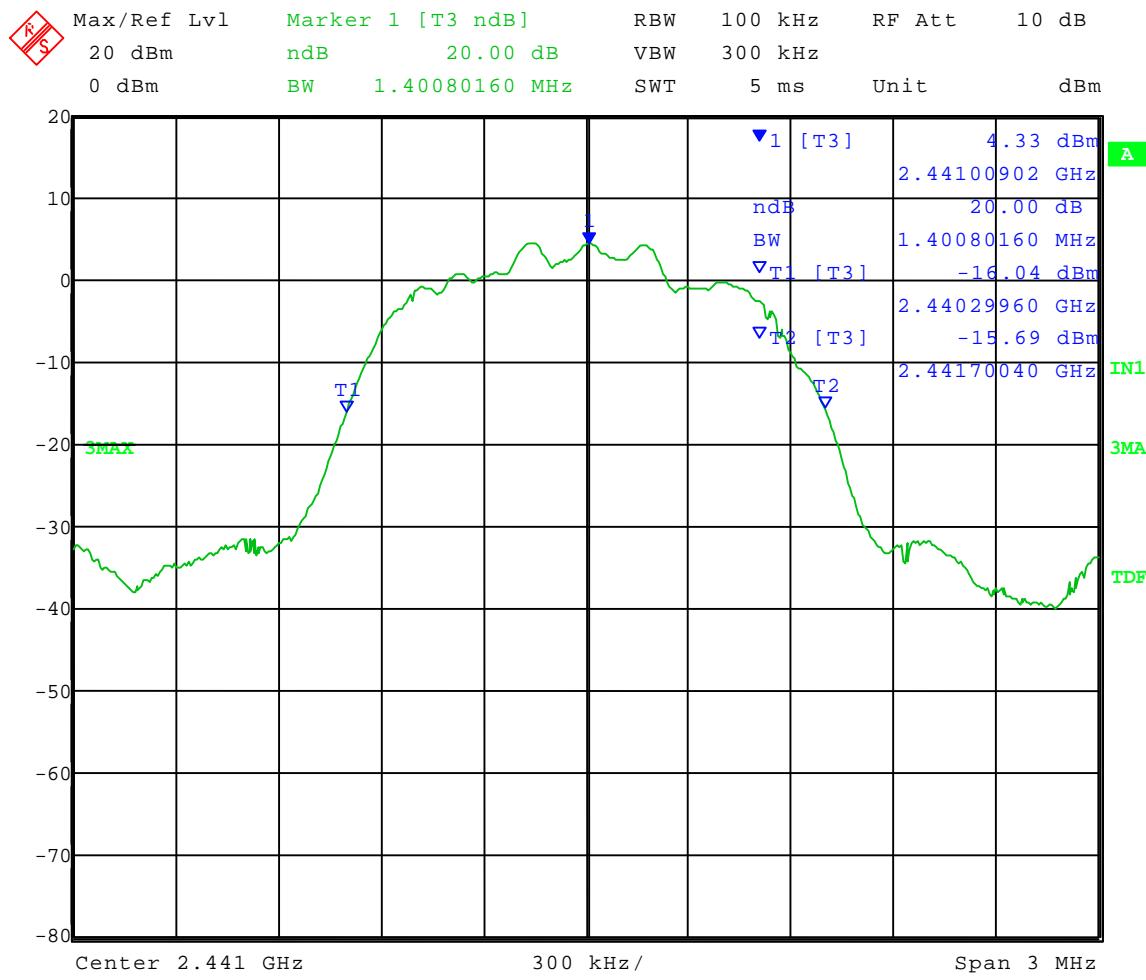




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 8-07-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: 20 dB Bandwidth  
Operator: Adam A  
Comment: **2.480 GHz** Transmit Frequency; Basic Data Rate

20 dB Bandwidth = 1.16 MHz

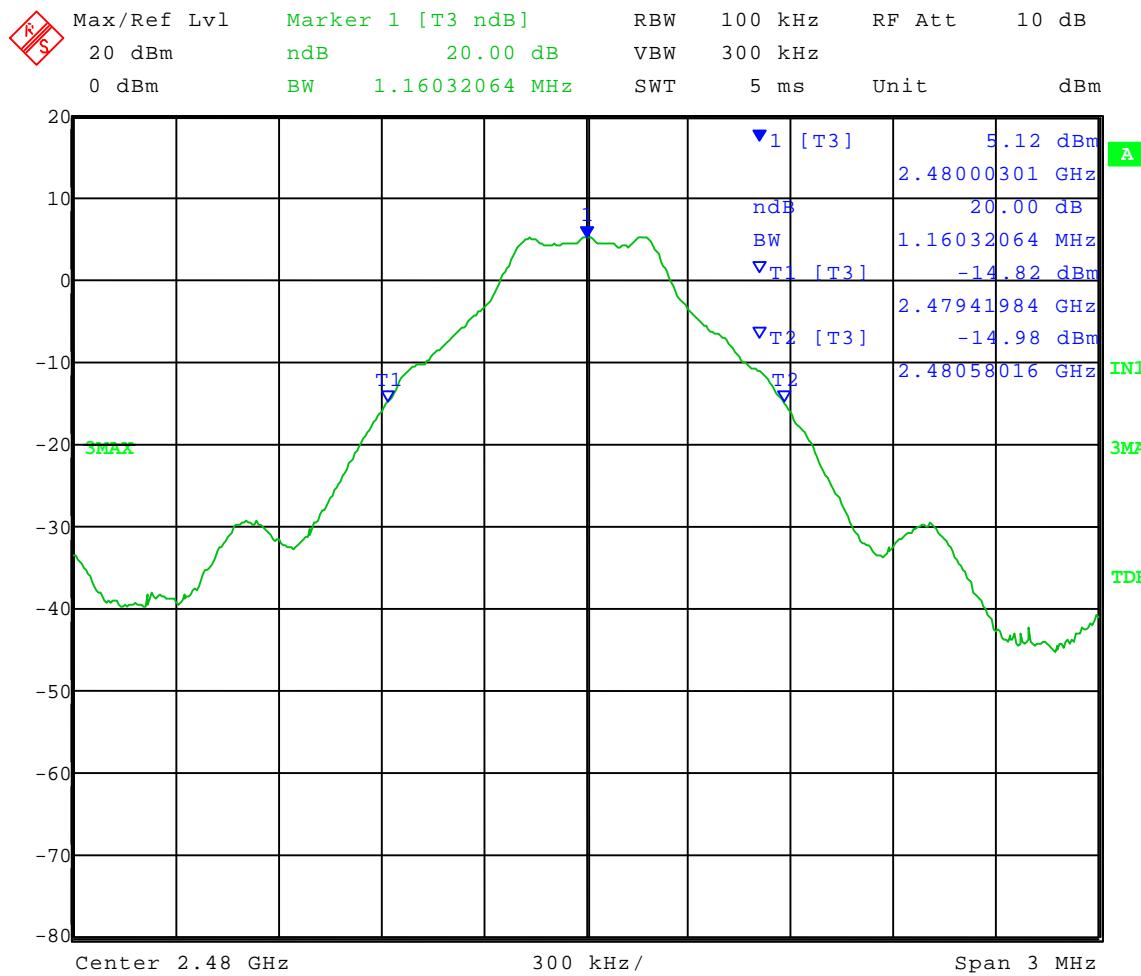




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 8-07-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: 20 dB Bandwidth  
Operator: Adam A  
Comment: **2.480 GHz** Transmit Frequency; Enhanced Data Rate 1

20 dB Bandwidth = 1.4008 MHz

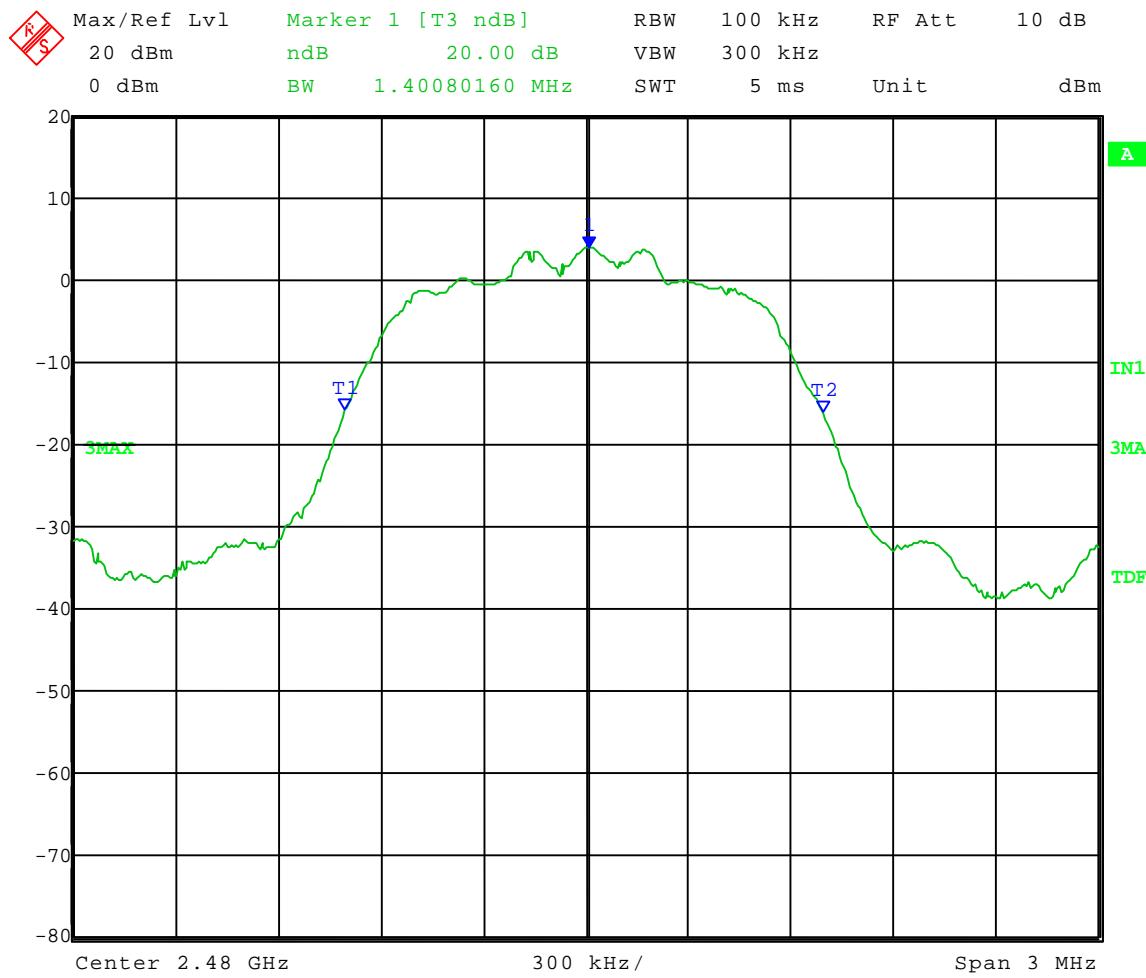




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 8-07-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: 20 dB Bandwidth  
Operator: Adam A  
Comment: **2.480 GHz** Transmit Frequency; Enhanced Data Rate 2

20 dB Bandwidth = 1.407 MHz

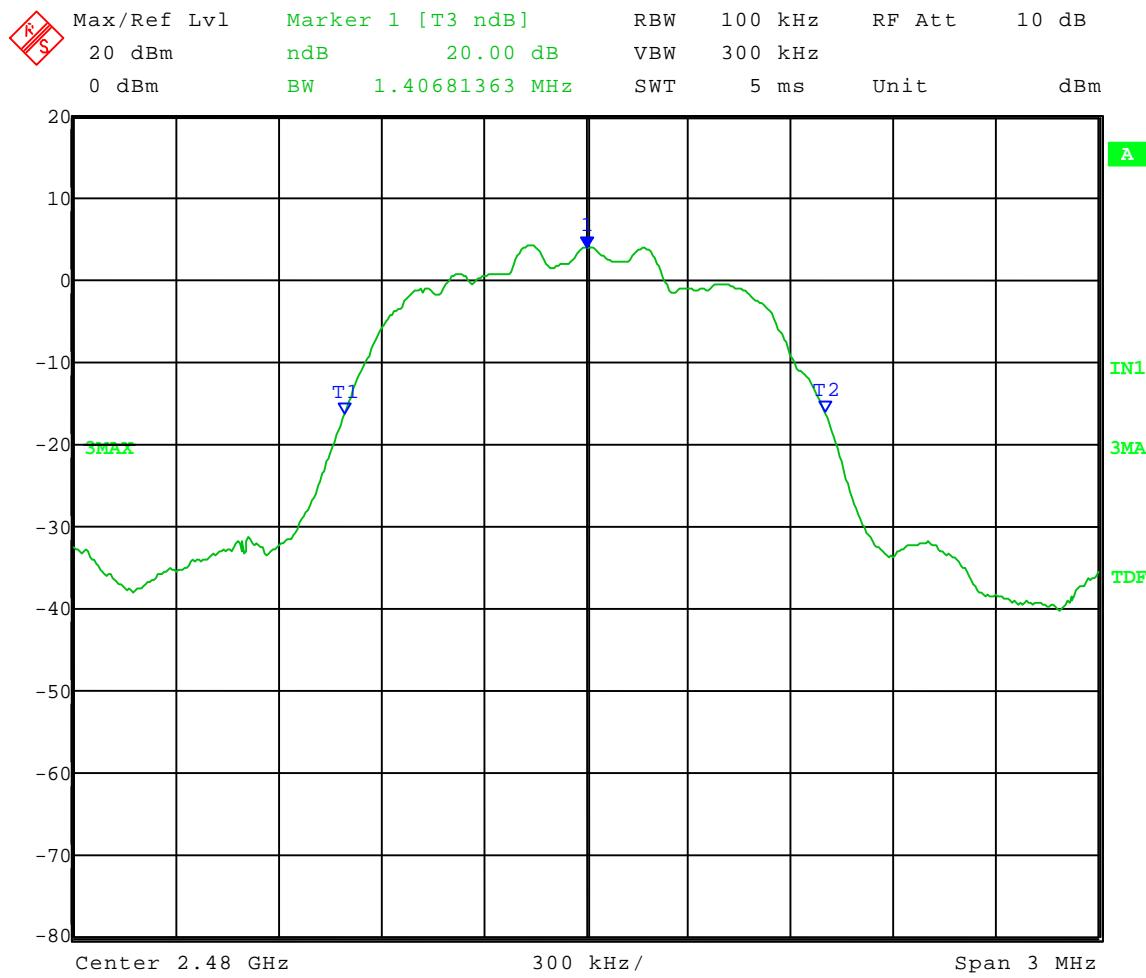



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

# DATA AND GRAPH(S) TAKEN SHOWING THE BAND EDGE CONDUCTED COMPLIANCE

## PART 15.247

### NOTE:

Per the FCC's Public Notice "Filing and Measurement Guidelines for Frequency Hopping Spread Spectrum Systems under DA 00-705 - March 30, 2000", as indicated in the test data section of this test report.




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Band-Edge  
Operator: Adam A  
Comment: **Low Channel:** Frequency – 2.402 GHz

Band-Edge Frequency = 2.402 GHz  
Band-Edge > 20 dB Below Peak In-Band Emission

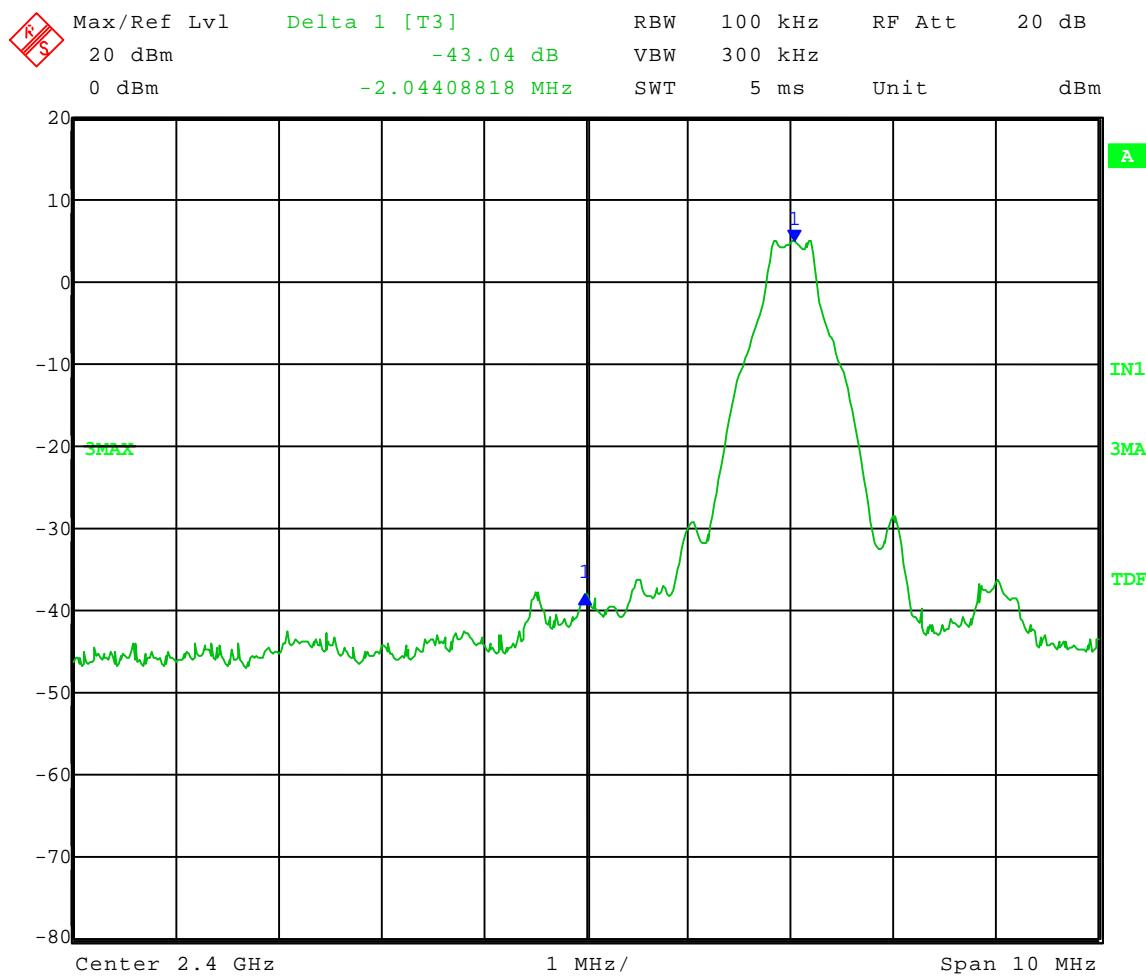

Date: 10.AUG.2009 11:03:13




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 8-07-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Band-Edge  
Operator: Adam A  
Comment: **High Channel:** Frequency – 2.480 GHz

Band-Edge Frequency = 2.4835 GHz  
Band-Edge > 20 dB Below Peak In-Band Emission

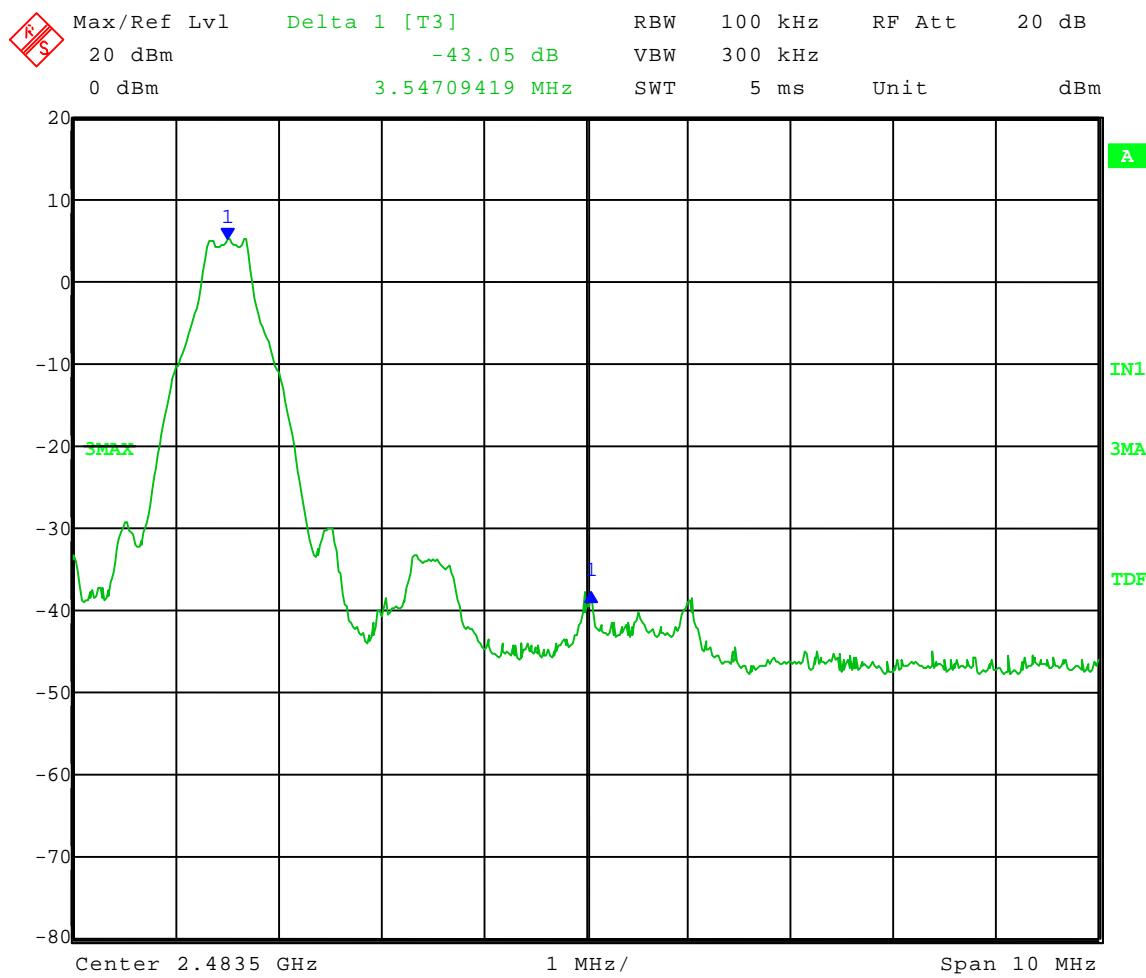

Date: 7.AUG.2009 13:57:52



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

# DATA AND GRAPH(S) TAKEN SHOWING

## UPPER BAND EDGE

# COMPLIANCE WITH RESTRICTED BAND

## PART 15.247

### **NOTE:**

Per the FCC's Public Notice "Filing and Measurement Guidelines for Frequency Hopping Spread Spectrum Systems under DA 00-705 - March 30, 2000", as indicated in the test data section of this test report.



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

### Radiated Upper Band-Edge measurement

Per the FCC's Public Notice "Filing and Measurement Guidelines for Frequency Hopping Spread Spectrum Systems under DA 00-705 - March 30, 2000", as indicated in the test data section of this test report.

The EUT was investigated at the low and high channels of operation to determine band-edge compliance. Because the upper band-edge coincides with a restricted band, bandedge compliance for the upper band-edge was determined using the radiated mark-delta method. The radiated field strength of the fundamental emission was first determined and then the mark-delta method was used to determine the field strength of the band-edge emissions. The lower band-edge compliance was determined using the marker-delta method in which the radio frequency power that is produced by the EUT is at least 20 dB below that in the 100 kHz bandwidth within the band that contains the highest level of desired power.

#### Upper Band-Edge Marker Delta Method

Frequency (MHz)	Antenna Polarit y (H/V)	Fundamental Field Strength (dB $\mu$ V/m)	Duty Cycle Correcti on (dB)	Delta- Marke r (dB)	Band- Edge Field Strength (dB $\mu$ V/m)	Limit (dB $\mu$ V /m)	Margi n (dB)
2480 (Peak)	H	105.38	N/A	-38.59	63.79	74	10.21
2480 (Avg)	H	95.06	17.65	-38.59	38.82	54	15.18




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 8-28-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Upper Band-Edge Radiated – Marker Delta Method  
Operator: Adam A  
Comment: High Channel: Frequency – 2.480 GHz

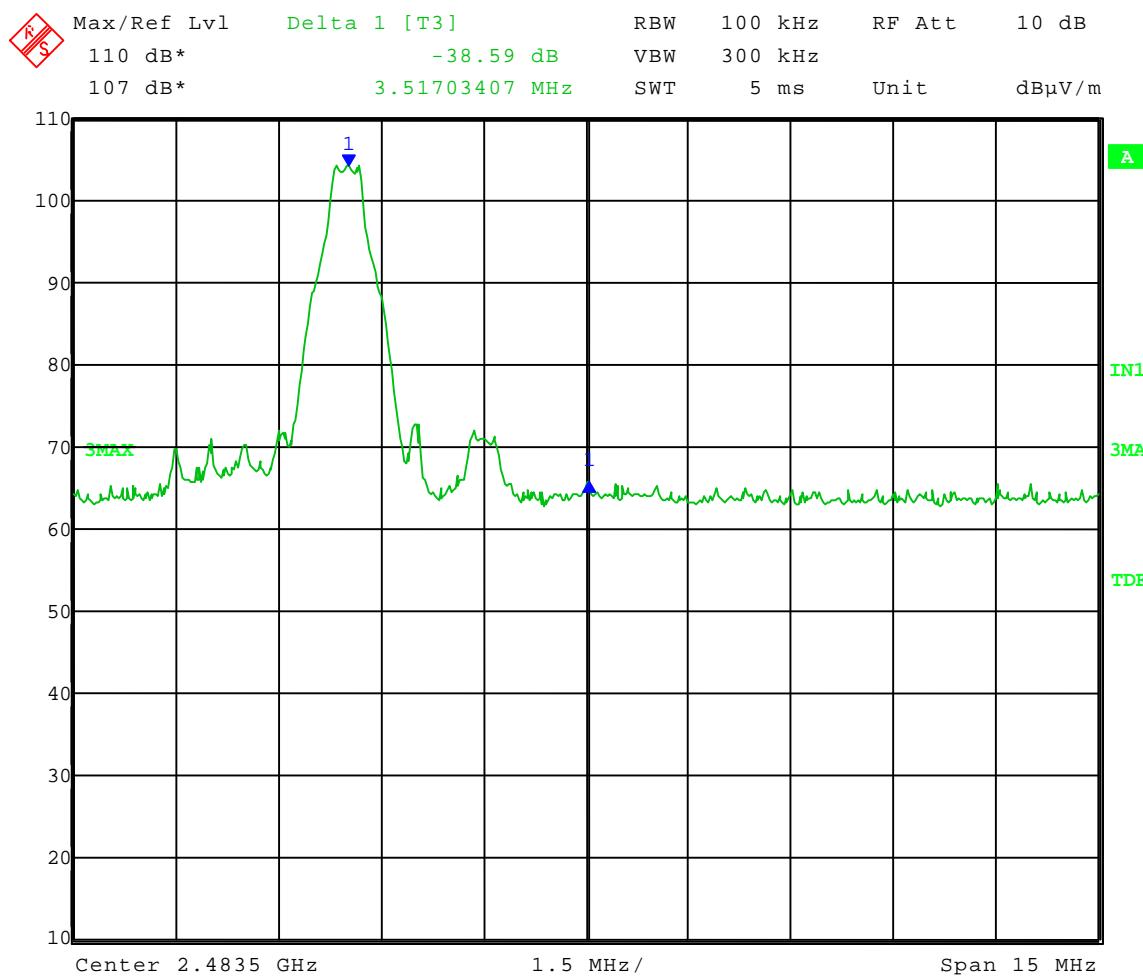



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

### 5.0 FIELD STRENGTH OF FUNDAMENTAL AND SPURIOUS EMISSION MEASUREMENTS

The radiated measurements made at D.L.S. Electronic Systems, Inc., for the Accu-Chek Aviva Combo, Model Number: Aviva: 670, are shown in tabulated and graph form. Preliminary radiation measurements were performed at a 3 meter test distance with the limits adjusted linearly when required. The frequency range from 30 MHz to over 960 MHz, depending upon the fundamental frequency as stated in Part 15.33a, was automatically scanned and plotted at various angles.

Measurements for the Accu-Chek Aviva Combo were made up to 26000 MHz, in accordance with Section 15.33a for Intentional Radiators with a fundamental frequency of 2402 - 2480 MHz. For intentional radiators, the frequency range to be investigated is determined by the lowest radio frequency generated by the device without going below 30 MHz, up to at least the tenth harmonic of the highest fundamental frequency or 10 GHz, whichever is lower. At those frequencies where significant signals were detected, measurements were made over the entire frequency range specified in FCC Part 15, Subpart C, Section 15.247 at the open field test site, located at Genoa City, Wisconsin, FCC file number **31040/SIT**. When required, limits were extrapolated using a linear extrapolation.

All signals in the frequency range of 30 MHz to 2000 MHz were measured with a Biconical Antenna or tuned dipoles and from 200 MHz to 1000 MHz, a Log Periodic or Tuned Dipoles were used. From 1000 MHz to 25 GHz Horn Antennas were used. During the test the equipment was rotated and the antenna was raised and lowered from 1 meter to 4 meters to find the maximum level of emissions. In order to find maximum emissions, the cables were moved through all the positions the equipment would be expected to experience in the field. The EUT, peripheral equipment and cables were configured to meet the conditions in ANSI C63.4-2003, Clauses 6 & 8, Test procedures for the radiated field strength of spurious emissions is the FCC's Public Notice "Filing and Measurement Guidelines for Frequency Hopping Spread Spectrum Systems under DA 00-705 - March 30, 2000", as indicated in the test data section of this test report. Tests were made with the receive antenna(s) in both the horizontal and vertical planes of polarization. In each case, the table was rotated to find the maximum emissions.



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

### 5.0 FIELD STRENGTH OF FUNDAMENTAL AND SPURIOUS EMISSION MEASUREMENTS (CON'T)

As stated in Section 15.247(b) the allowed maximum peak output power of the transmitter shall not exceed 1 Watt. In any 100 kHz bandwidth outside these frequency bands (the power that is produced by the modulation products of the spreading sequence), the information sequence and the carrier frequency shall be either at least 20 dB below that in the 100 kHz bandwidth within the band that contains the highest level of the desired power. Attenuation below the general limits specified in 15.209 is not required.

Field strength limits are at a distance of 3 meters. The emission limits shown are based on measurement instrumentation employing an average detector.

Emissions radiated outside of the specified frequency bands, except for harmonics are attenuated by at least 50 dB below the level of the fundamental or to the general radiated emission limits in Section 15.209, whichever is the lesser attenuation.

Preliminary radiated emission measurements were performed at a 3 meter test distance. The frequency range from 30 MHz to 1000 MHz was automatically scanned and plotted at various angles.

#### **NOTE:**

**All radiated emissions measurements were made at a test room temperature of 71°F at 54% relative humidity.**



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

# RADIATED DATA AND GRAPH(S) TAKEN FOR E.I.R.P. OF FUNDAMENTAL EMISSION MEASUREMENTS

## PART 15.247

### NOTE:

Per the FCC's Public Notice "Filing and Measurement Guidelines for Frequency Hopping Spread Spectrum Systems under DA 00-705 - March 30, 2000", as indicated in the test data section of this test report.



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

DLS Electronic Systems, Inc.

Company: Roche Diagnostics

Operator: Adam A

Date of test: 8-07-2009

Temperature: 72 deg. F

Humidity: 53% R.H.

### EIRP - Substitution Method

Model: Accu-Check Aviva Combo								
Channel: 2402 MHz								
Frequency and Polarization (MHz)	Max. Field Strength of EUT @ 3 meters (dBuV/m)	Output of Signal Generator when field strength equals that of EUT (dBm)	Correction factor for cable between Signal Gen. and subst. antenna (dB)	Gain of subst. antenna (dBi)	Strength of emission [EIRP] (dBm)	Limit (dBm)	Margin (dB)	Strength of emission [EIRP] (mW)
2402 vertical	100.52	-4.70	3.07	9.38	1.61	30.00	28.39	1.45
2402 horizontal	101.55	-4.50	3.07	9.38	1.81	30.00	28.19	1.52

EIRP = Signal generator output - cable loss + antenna gain

ERP<sub>(ref. to 1/2λ dipole)</sub> = Signal generator output - cable loss + antenna gain - 2.15



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

DLS Electronic Systems, Inc.

Company: Roche Diagnostics

Operator: Adam A

Date of test: 8-07-2009

Temperature: 72 deg. F

Humidity: 53% R.H.

### EIRP - Substitution Method

Model: Accu-Check Aviva Combo								
Channel: 2441 MHz								
Frequency and Polarization (MHz)	Max. Field Strength of EUT @ 3 meters (dBuV/m)	Output of Signal Generator when field strength equals that of EUT (dBm)	Correction factor for cable between Signal Gen. and subst. antenna (dB)	Gain of subst. antenna (dBi)	Strength of emission [EIRP] (dBm)	Limit (dBm)	Margin (dB)	Strength of emission [EIRP] (mW)
2441 vertical	101.57	-3.60	3.11	9.43	2.72	30.00	27.28	1.87
2441 horizontal	103.13	-2.70	3.11	9.43	3.62	30.00	26.38	2.30

EIRP = Signal generator output - cable loss + antenna gain

ERP<sub>(ref. to 1/2λ dipole)</sub> = Signal generator output - cable loss + antenna gain - 2.15



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

DLS Electronic Systems, Inc.

Company: Roche Diagnostics

Operator: Adam A

Date of test: 8-07-2009

Temperature: 72 deg. F

Humidity: 53% R.H.

### EIRP - Substitution Method

Model: Accu-Check Aviva Combo								
Channel: 2480 MHz								
Frequency and Polarization (MHz)	Max. Field Strength of EUT @ 3 meters (dBuV/m)	Output of Signal Generator when field strength equals that of EUT (dBm)	Correction factor for cable between Signal Gen. and subst. antenna (dB)	Gain of subst. antenna (dBi)	Strength of emission [EIRP] (dBm)	Limit (dBm)	Margin (dB)	Strength of emission [EIRP] (mW)
2480 vertical	104.81	-0.60	3.10	9.49	5.79	30.00	24.21	3.79
2480 horizontal	105.45	-0.60	3.10	9.49	5.79	30.00	24.21	3.79

EIRP = Signal generator output - cable loss + antenna gain

ERP<sub>(ref. to 1/2λ dipole)</sub> = Signal generator output - cable loss + antenna gain - 2.15



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

# TRANSMITTER DUTY CYCLE GRAPHS

## PART 15.35(c)



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090


## APPENDIX B

Test Date: 9-30-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Duty Cycle – worst case during normal operation  
Operator: Craig B

Comment: Total on Time = 436.87 us  
 $20 \log (.43687 / 100) = -47.2 \text{ dB}$

### Maximum Useful Duty Cycle Correction Factor = 20 dB

100 ms sweep:

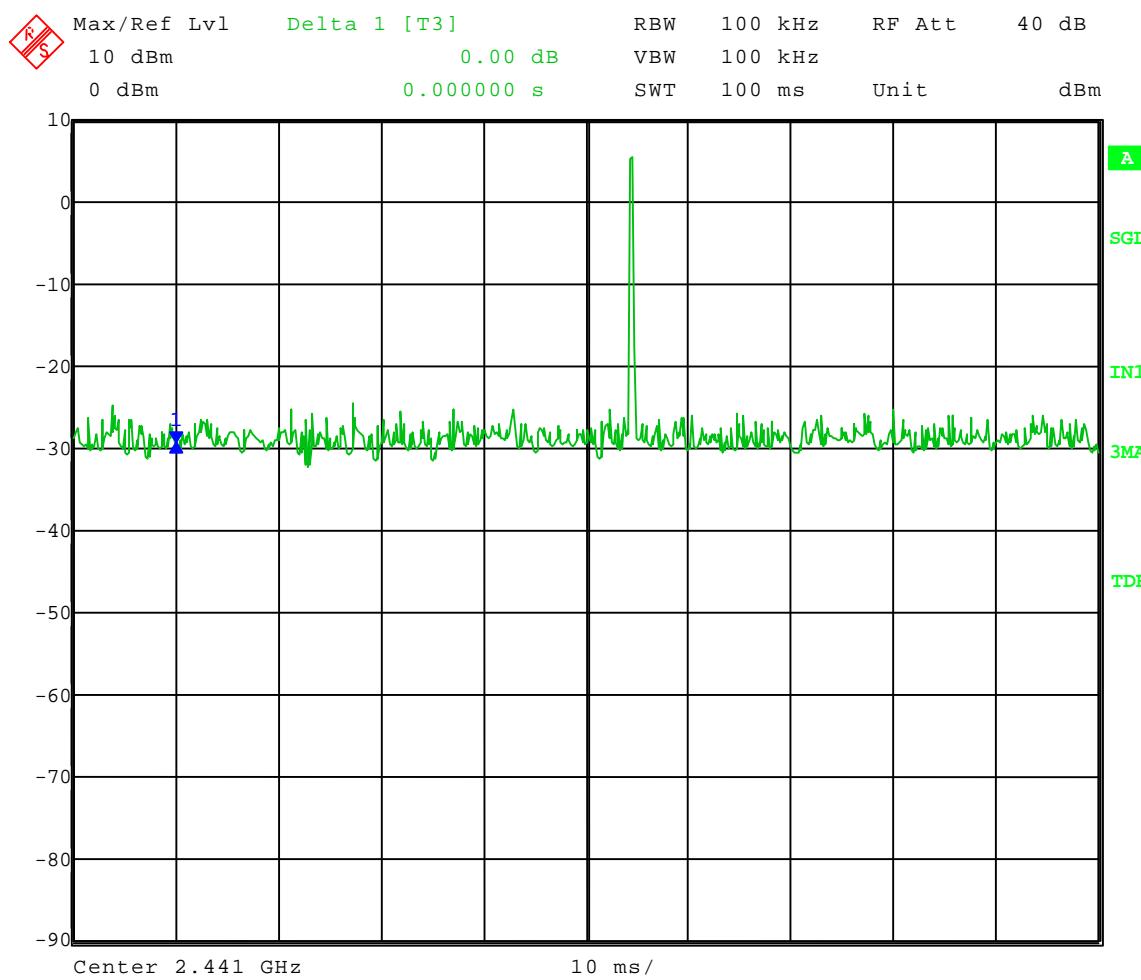



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584


1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 9-30-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Duty Cycle – worst case during normal operation  
Operator: Craig B  
  
Comment: Total on Time = 436.87 us  
 $20 \log (.43687 / 100) = -47.2 \text{ dB}$

### Maximum Useful Duty Cycle Correction Factor = 20 dB

Duration of one pulse:

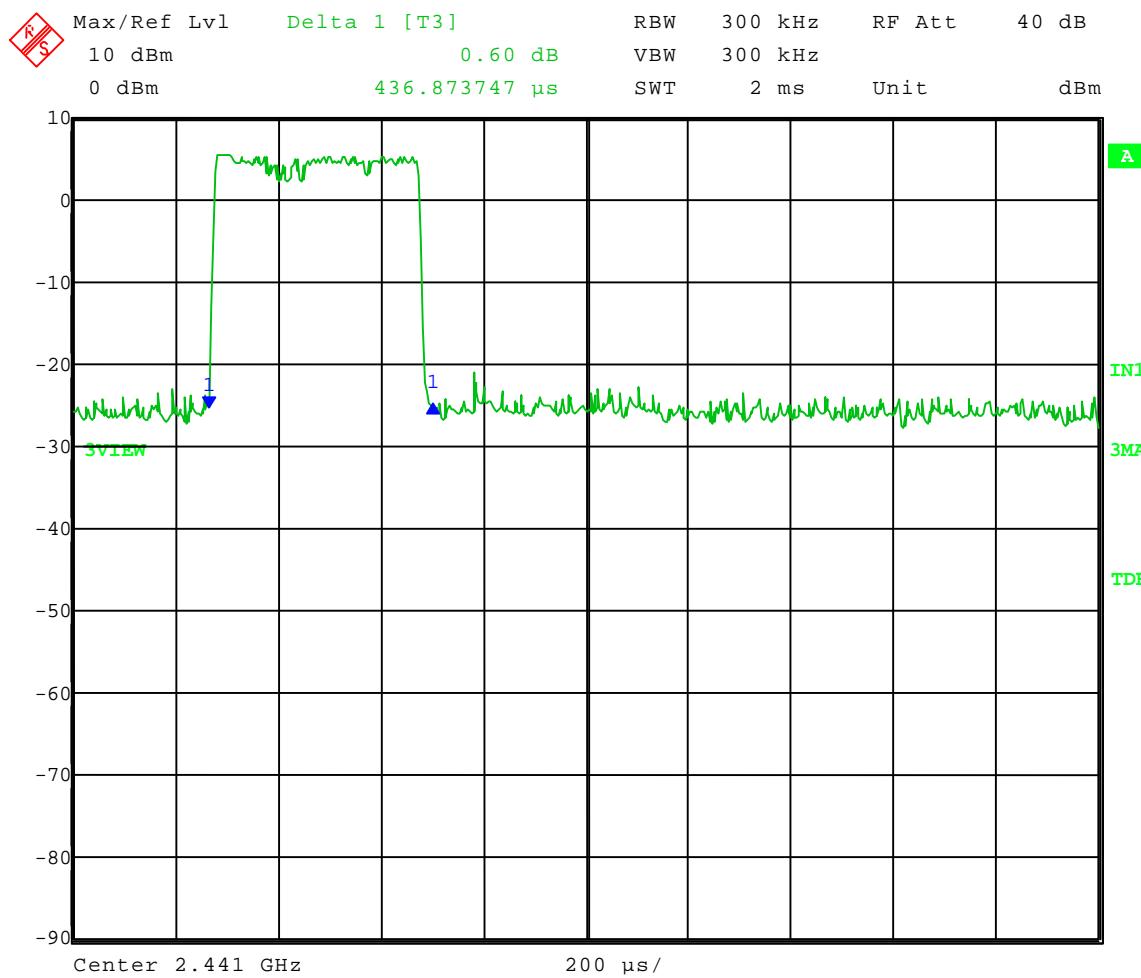




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 9-30-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Duty Cycle – worst case during normal operation  
Operator: Craig B

Comment: 162 hops in 16 sec. = 324 hops in 32 sec.  
0.4 X 79 channels = 31.6.  
Limit = 0.4 sec. ON time in 31.6 sec.  
Time of occupancy of one hop = 436.87 us  
Dwell time = 436.87 us per hop X 324 hops = **0.14** sec.

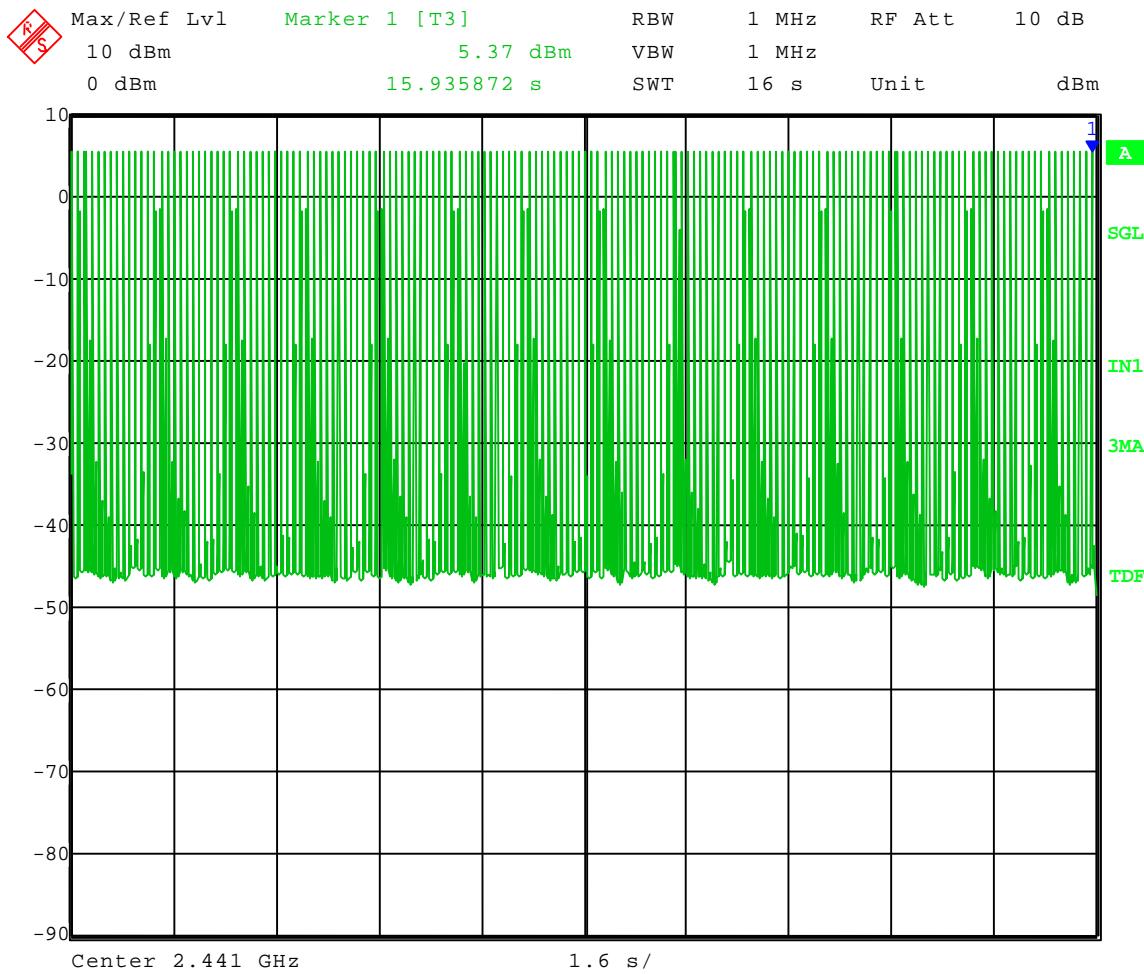




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 9-30-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Duty Cycle – worst case during normal operation  
Operator: Craig B

Comment: 162 hops in 16 sec. = 324 hops in 32 sec.  
0.4 X 79 channels = 31.6.  
Limit = 0.4 sec. ON time in 31.6 sec.  
Time of occupancy of one hop = 436.87 us  
Dwell time = 436.87 us per hop X 324 hops = **0.14** sec.

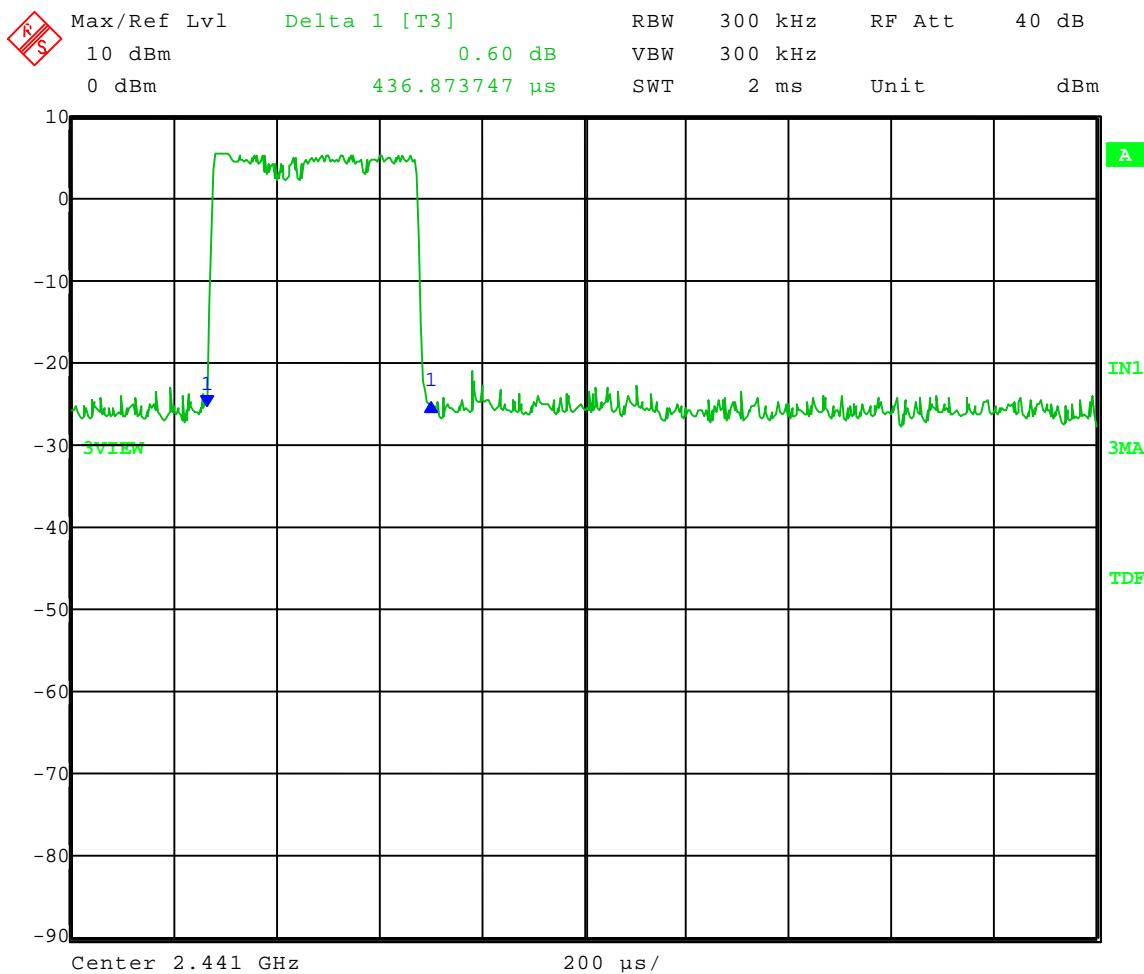



Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

# CARRIER FREQUENCY SEPARATION GRAPH(S)

## PART 15.247




Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX B

Test Date: 8-07-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Channel Separation  
Operator: Adam A  
Comment: Frequency Hopping On Maximum Data Rate

Carrier Freq Separation = 1.00 MHz

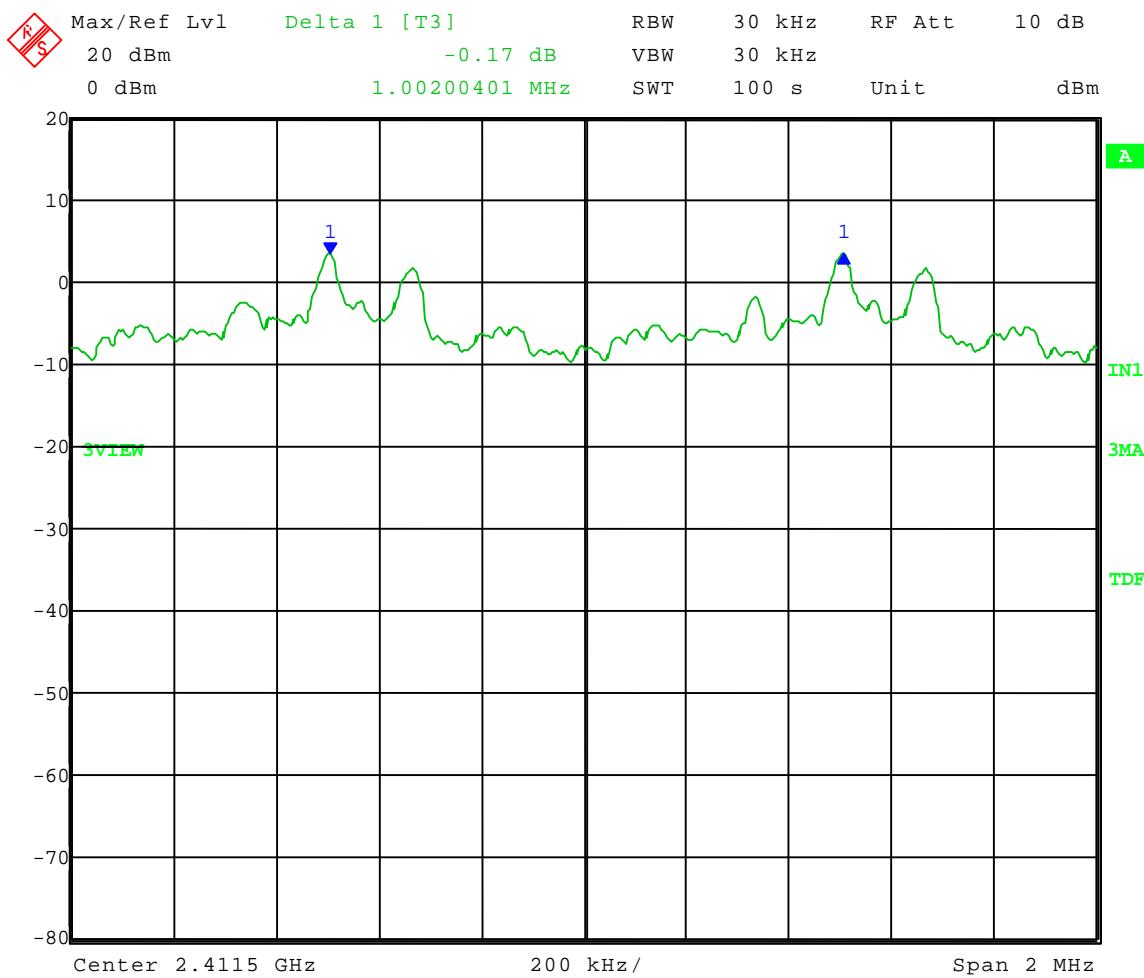




1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

Test Date: 8-07-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Channel Separation  
Operator: Adam A  
Comment: Frequency Hopping On Minimum Data Rate

Carrier Freq Separation = 1.00 MHz

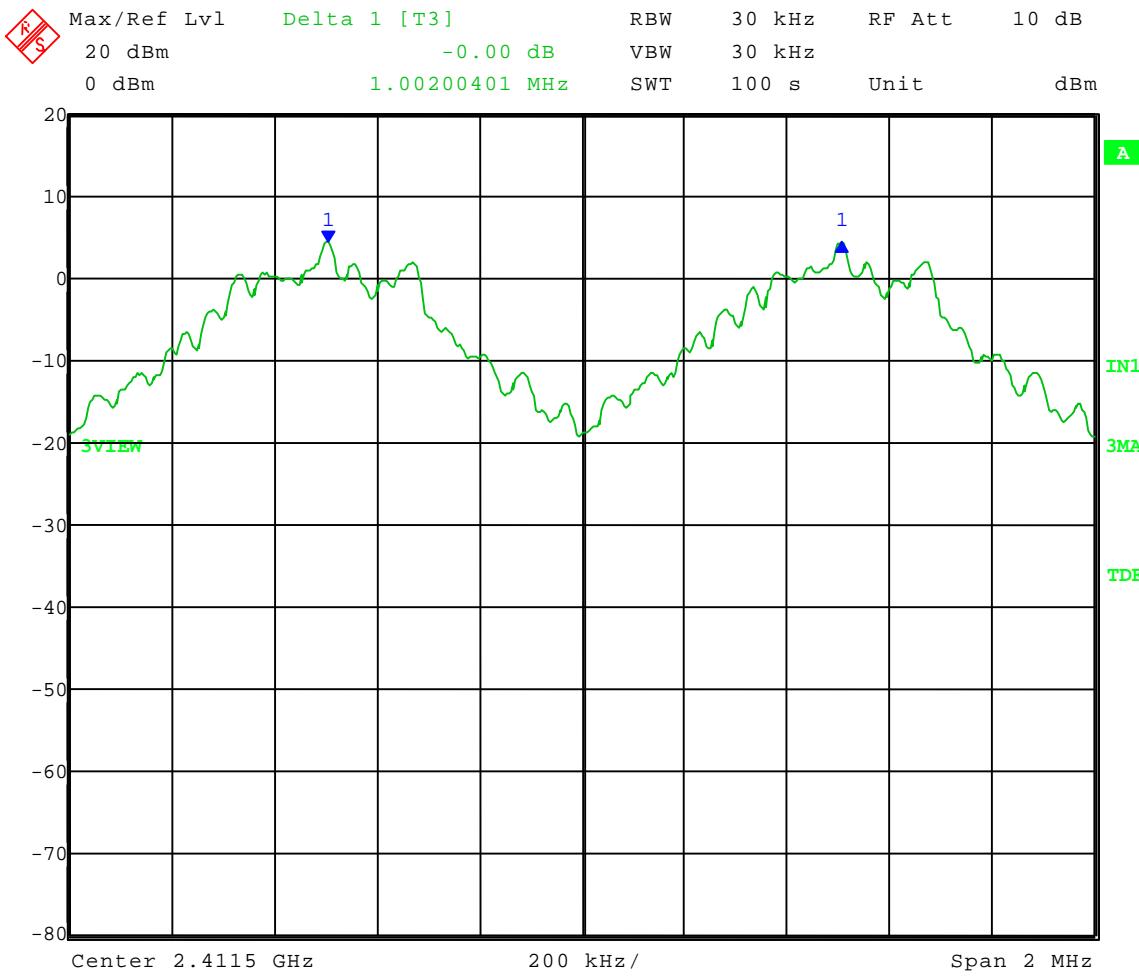



1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

## NUMBER OF HOPPING CHANNELS GRAPH(S)

### PART 15.247




1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

Test Date: 8-07-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Number of Hopping Channels  
Operator: Adam A  
Comment: Normal Transmit Operation

Number of hopping channels: 79

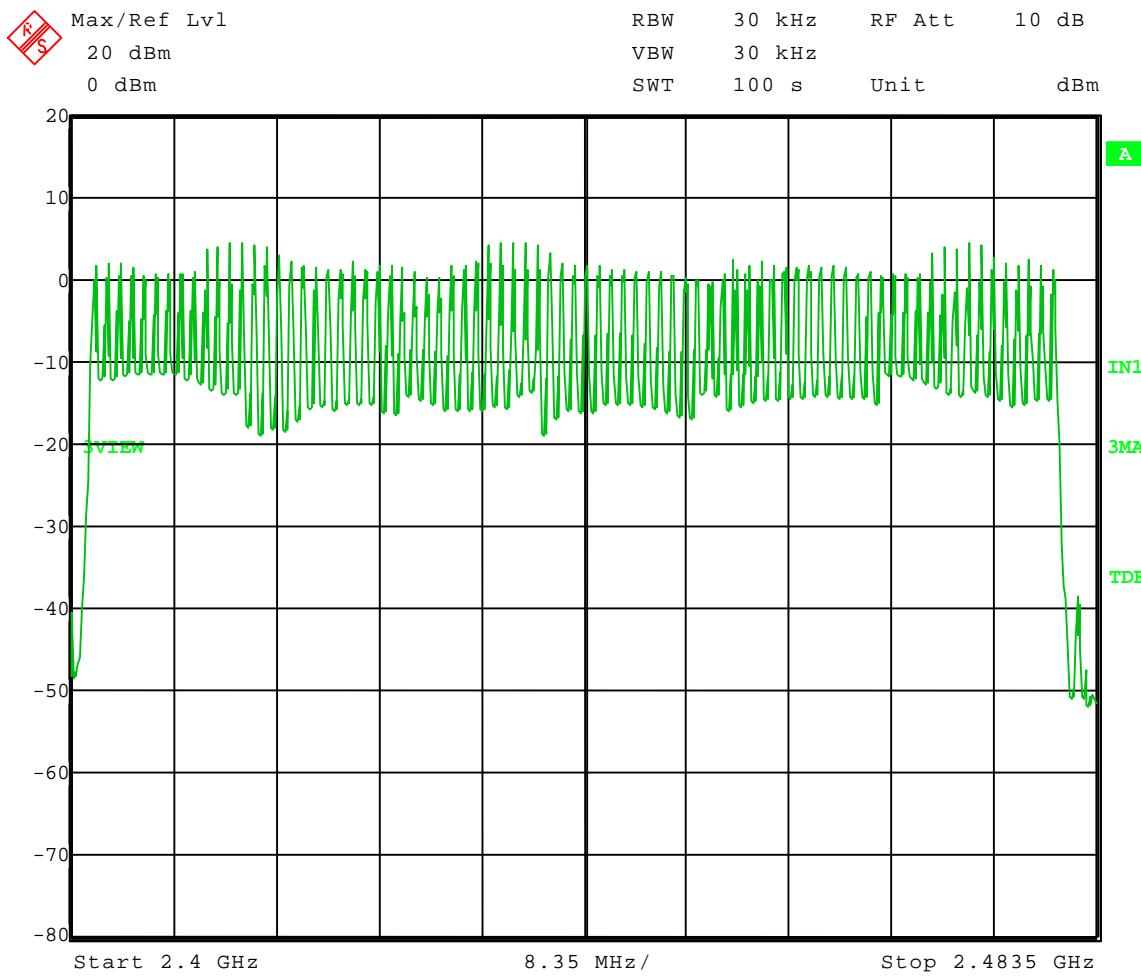

Date: 7.AUG.2009 15:28:58



1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

## TIME OF OCCUPANCY GRAPHS

### PART 15.247




1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Dwell Time  
Operator: Adam A  
Comment: Normal Transmit Operation

Dwell time: time of occupancy \* number of hopping channels < .4 seconds

436 us \* 79 (channels) = .0344 sec

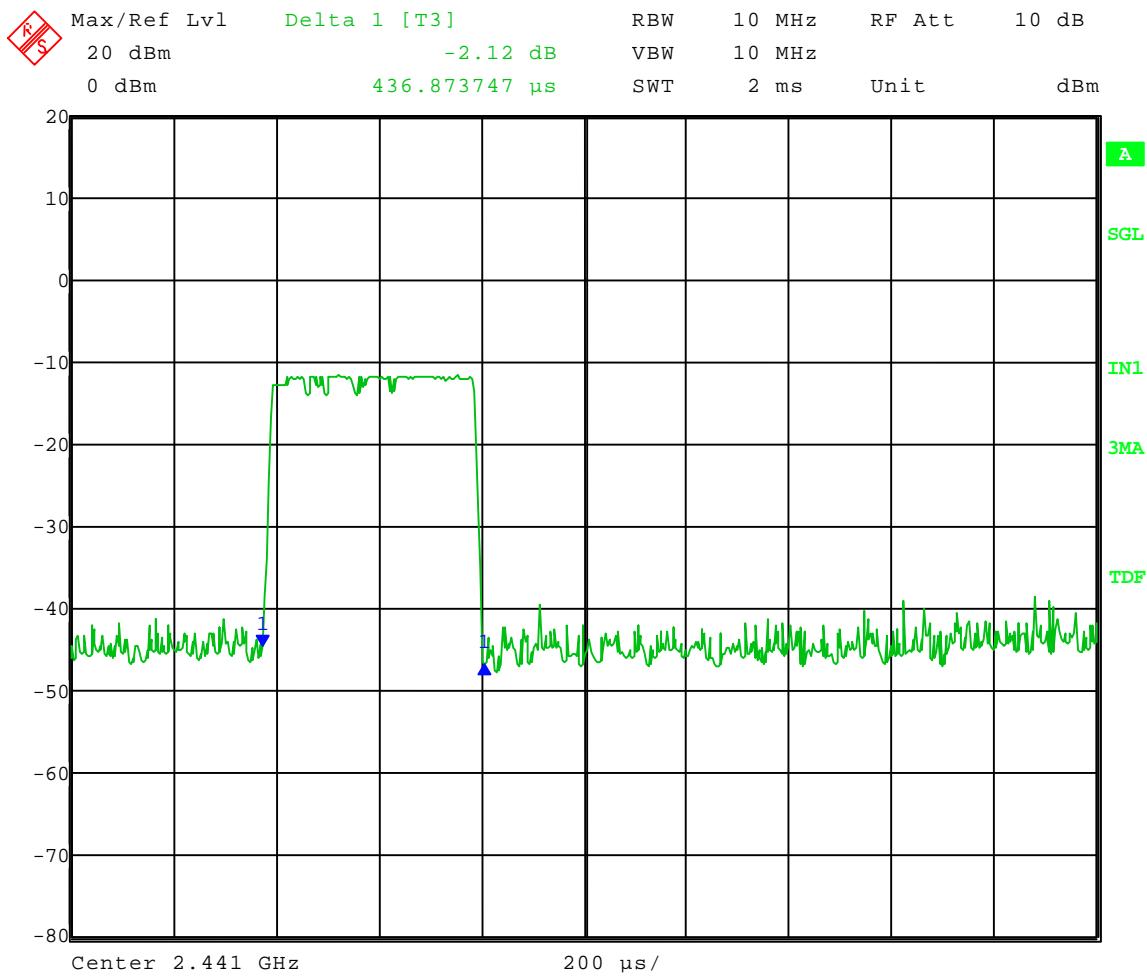

Date: 10.AUG.2009 08:34:00



1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

## CONDUCTED PEAK OUTPUT POWER GRAPHS

### PART 15.247




1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Peak Power Output - Conducted  
Operator: Adam A  
Comment: **Low Channel: Frequency – 2.402 GHz**

Peak Output Power = 5.06 dBm = **3.21 mW**

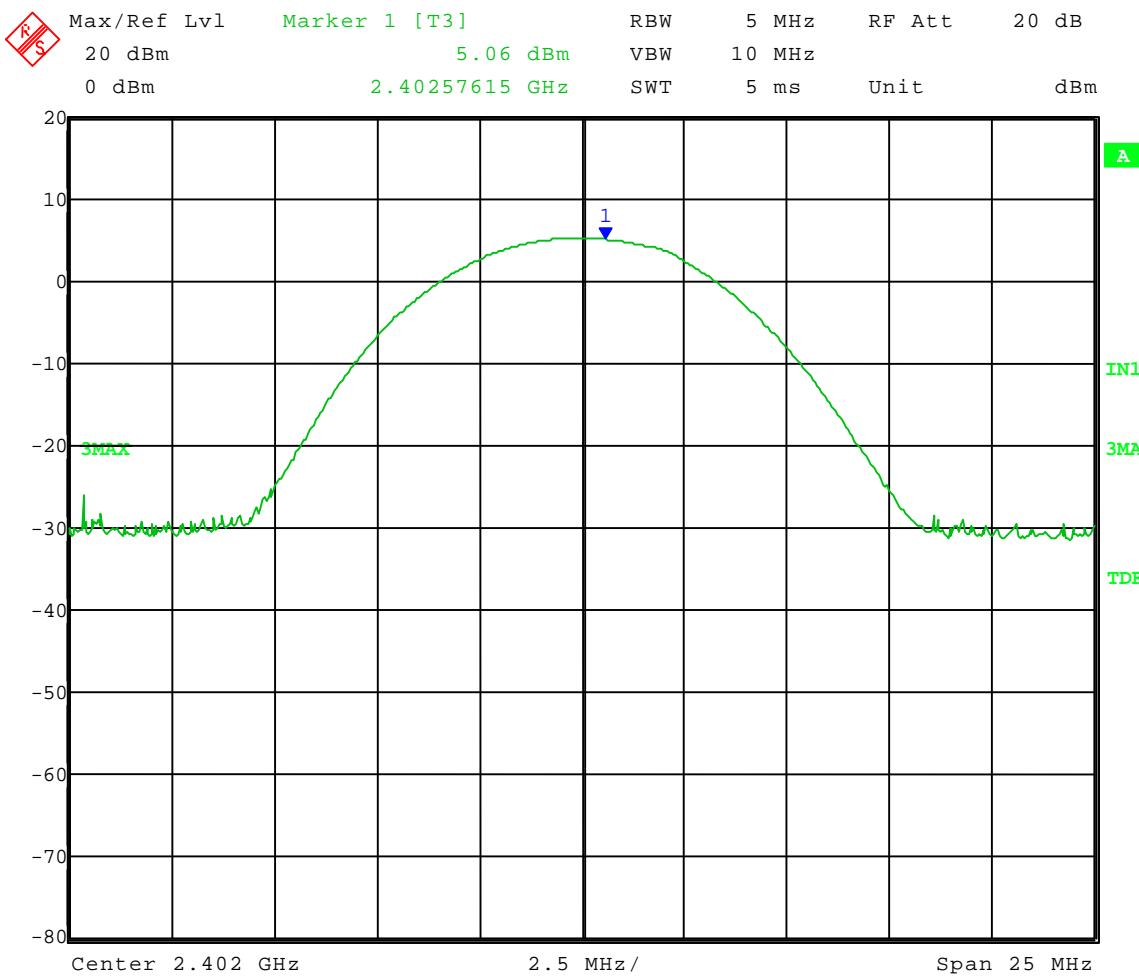




1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

Test Date: 8-10-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Peak Power Output - Conducted  
Operator: Adam A  
Comment: **Mid Channel:** Frequency – 2.441 GHz

Peak Output Power = 5.20 dBm = **3.31 mW**

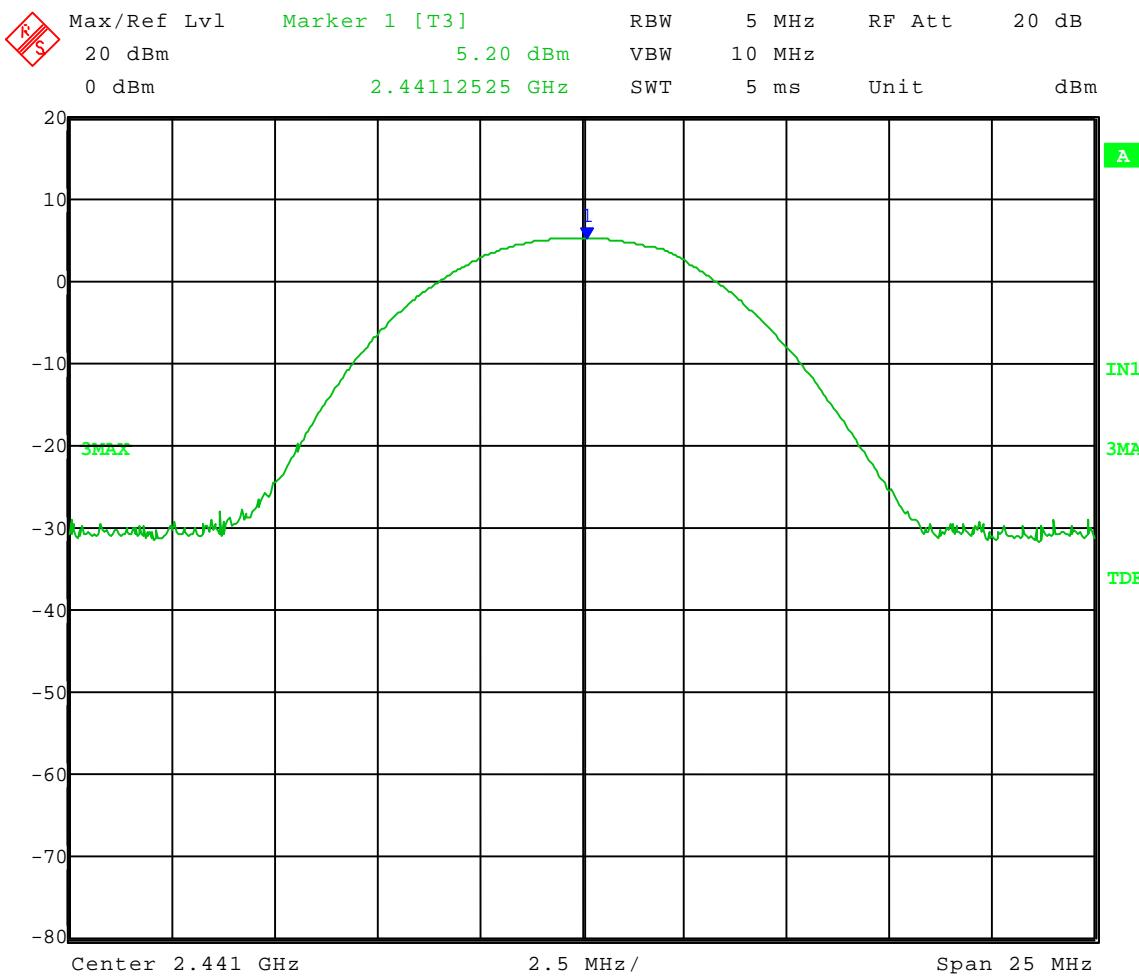

Date: 10.AUG.2009 10:46:59



1250 Peterson Dr., Wheeling, IL 60090

Company: Roche Diagnostics  
Model Tested: Aviva: 670  
Report Number: 15584

Test Date: 8-07-2009  
Company: Roche Diagnostics  
EUT: Accu-Check Aviva Combo  
Test: Peak Power Output - Conducted  
Operator: Adam A  
Comment: **High Channel:** Frequency – 2.480 GHz

Peak Output Power = 5.16 dBm = **3.28 mW**

