


**ATTACHMENT A to File No.: T33405**


**Test setup description for EMC and EMI measurements**



**Test setup photo for radiated emission measurement**

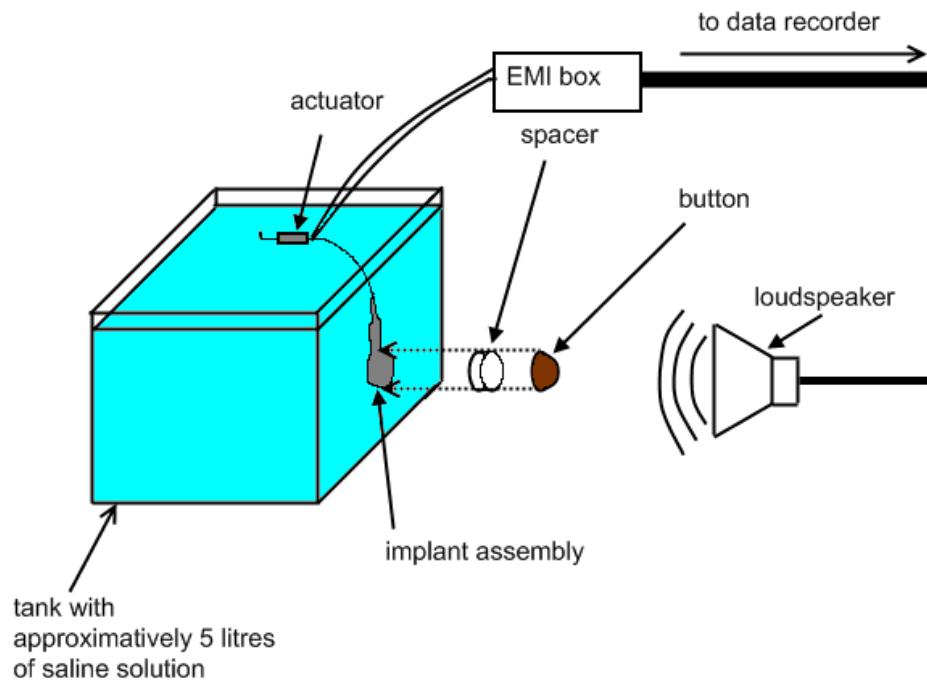

**ATTACHMENT A to File No.: T33405**

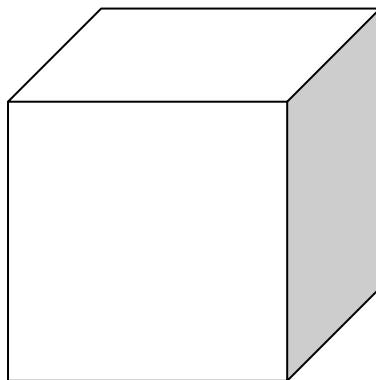

**tank dimensions**  
171mm X 171mm X 171mm

**Test setup description**

The implant assembly is placed into a tank with saline solution of 0.9% NaCl w/v to simulate the human body. The actuator remains outside the bath. From the side of the tank, the button is place on the implant coil separated by a spacer.