


	<p>The FCC Wants You to Know</p> <p>This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment.</p> <p></p> <p>This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications.</p> <p>Operation of this equipment in a residential area is likely to cause harmful interference, in which case the user will be required to correct the interference at his own expense.</p>	6
--	--	---

2.3 INDICATIONS

The ORLocate™ Packing system is indicated for use in detecting RFID-tagged surgical instruments and set tags. The product is indicated for providing a method of packing surgical items to create surgical sets.

2.4 SYSTEM LABELS

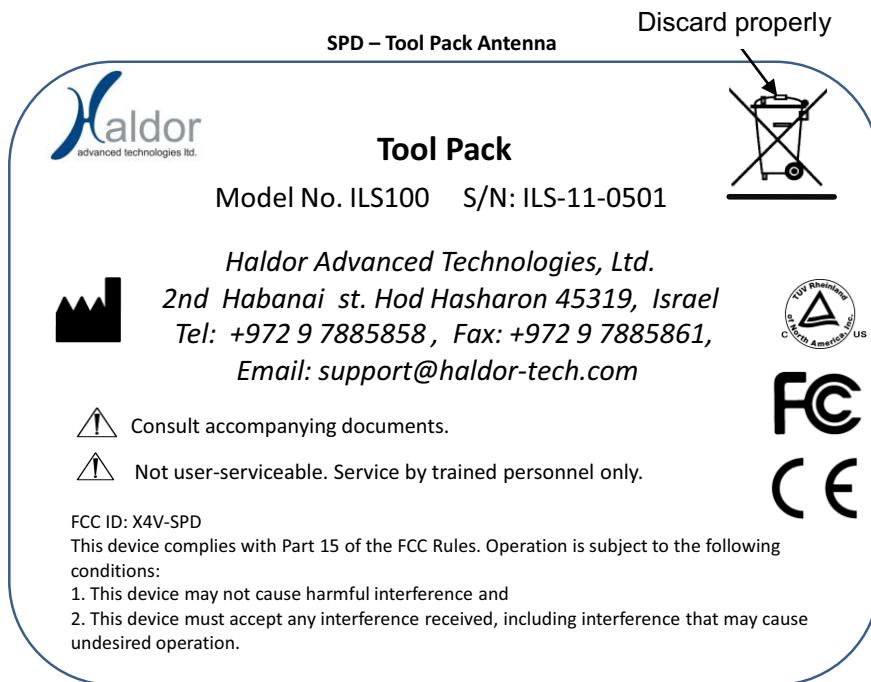

Warning Label on Tool Pack Antenna:

