

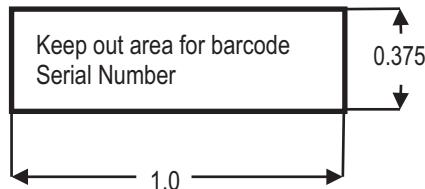


Stimulator Label

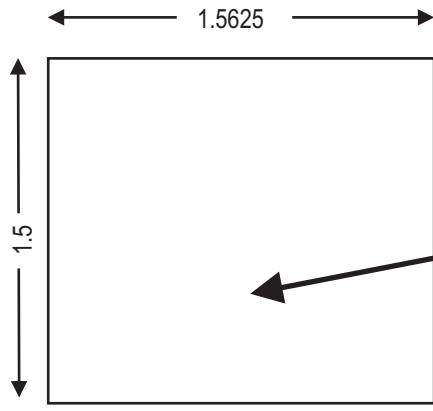

ASCEND
MN: AS-010
NEUROMetrix® Inc.
Waltham, MA 02451 USA
Tel: 1-781-890-9989

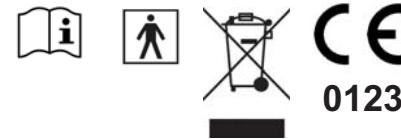

FCC ID: XUL-RF-SYNC IC: 3278A-RFSYNC

This device complies with Part 15 of the FCC Rules.

Operation is subject to the following two conditions:
(1) This device may not cause harmful interference, and
(2) This device must accept any interference received, including interference that may cause undesired operation.

Patents Pending
2202791 Rev. A




1 5 1 0 0 0 0 0

NOTES:

1. MATL: WHITE POLYESTER, DPM, CAPPED
2. PRINTING COLOR TO BE BLACK ON WHITE BACKGROUND.
3. FOR ARTWORK, SEE XXX.
4. SERIAL NUMBER AND BAR CODE AREAS LEFT BLANK. SERIAL NUMBER AND BAR CODE WILL BE PRINTED ON LABEL BY CONTRACT MANUFACTURER.
5. FIRST TWO DIGITS (15) IN SERIAL NUMBER INDICATES DEVICE, THIRD AND FOURTH DIGIT (10) INDICATE YEAR UNIT WAS MANUFACTURED.
6. Sampling plan for inspection to correspond with MIL STD 105E and ANSI/ASQC Z-1.4 with an AQL of 1.0.

DR CM	DATE 12/3/2009	MATERIAL See note 1	NEUROMetrix, Inc. 62 Fourth Avenue Waltham, MA 02451
CHECK RM	DATE 2/11/10	FINISH See notes 1 and 2	PN: 2202791
DESCRIPTION: Label, Stimulator			
REL	DATE	SCALE Measurements in inches	REV: B Sheet 1 of 1

Bioamplifier Label

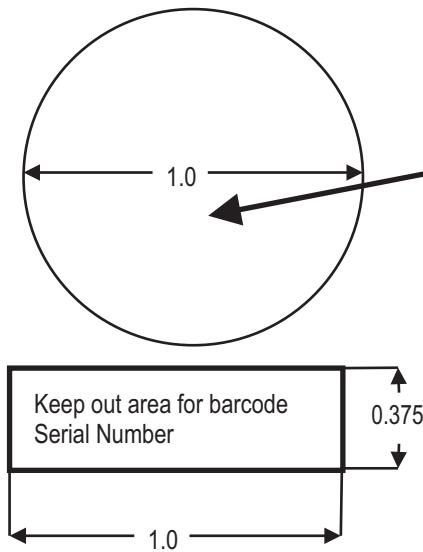

Bioamplifier
MN: AS-B01
NEUROMetrix® Inc.
Waltham, MA 02451 USA
Tel: 1-781-890-9989

    0123

FCC ID: XUL-RF-SYNC IC: 3278A-RFSYNC
This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
(1) This device may not cause harmful interference, and
(2) This device must accept any interference received,
including interference that may cause undesired operation.

Patents Pending
2202664 Rev. A



1 6 1 0 0 0 0 0

NOTES:

1. MATL: WHITE POLYESTER, DPM, CAPPED
2. PRINTING COLOR TO BE BLACK ON WHITE BACKGROUND.
3. FOR ARTWORK, SEE XXX.
4. SERIAL NUMBER AND BAR CODE AREAS LEFT BLANK. SERIAL NUMBER AND BAR CODE WILL BE PRINTED ON LABEL BY CONTRACT MANUFACTURER.
5. FIRST TWO DIGITS (16) IN SERIAL NUMBER INDICATES DEVICE, THIRD AND FOURTH DIGITS (10) INDICATE YEAR UNIT WAS MANUFACTURED.
6. Sampling plan for inspection to correspond with MIL STD 105E and ANSI/ASQC Z-1.4 with an AQL of 1.0.

DR CM	DATE 12/4/2009	MATERIAL See note 1	NEUROMetrix, Inc. 62 Fourth Avenue Waltham, MA 02451
CHECK RM	DATE 2/11/10	FINISH See notes 1 and 2	PN: 2202664
REL	DATE	SCALE Measurements in inches	DESCRIPTION: Label, Bioamplifier
			REV: B Sheet 1 of 1