


Appendix I

Photographs

- 1. SAR measurement System
- 2. Photographs of Tissue Simulate Liquid
- 3. Photographs of EUT test position
- 4. EUT Constructional Details



1. SAR measurement System

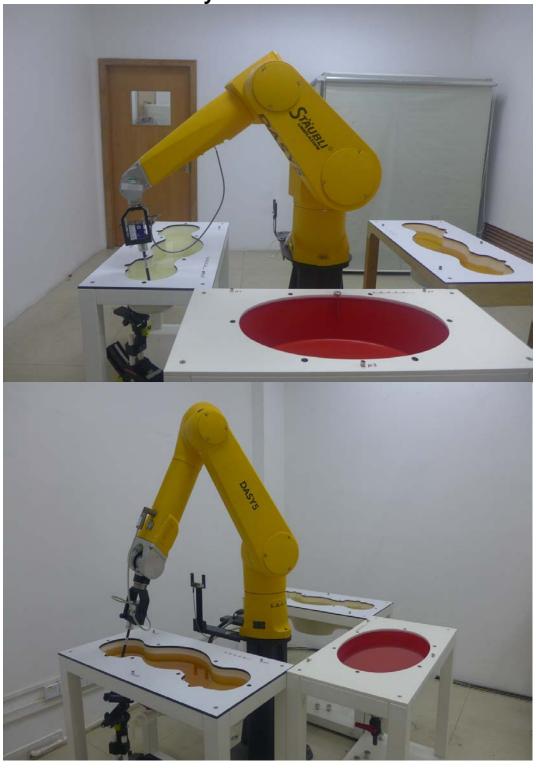



2. Photographs of Tissue Simulate Liquid

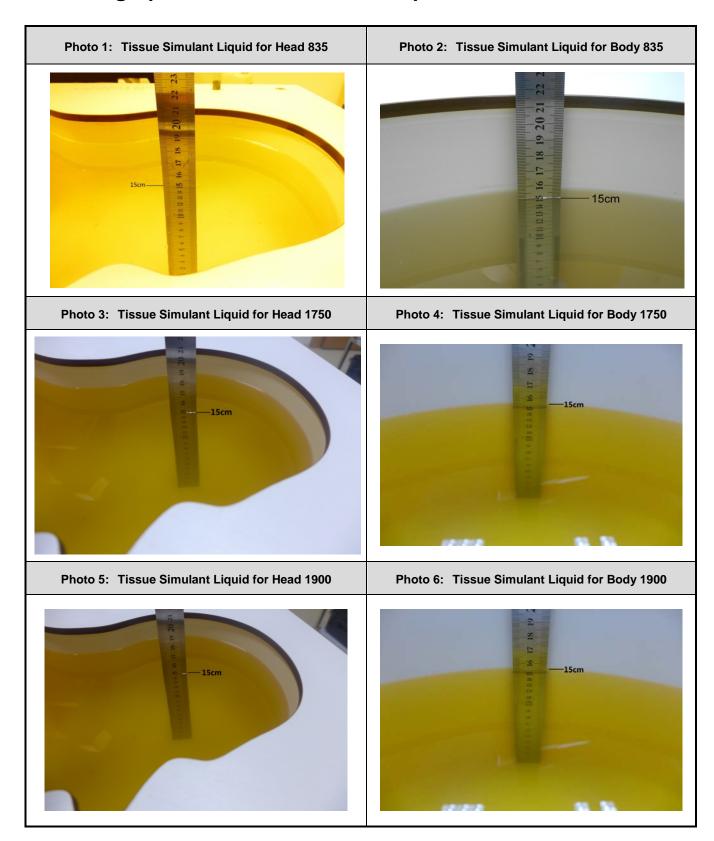




Photo 7: Tissue Simulant Liquid for Head 2300 Photo 8: Tissue Simulant Liquid for Body 2300 Photo 9: Tissue Simulant Liquid for Head 2450 Photo 10: Tissue Simulant Liquid for Body 2450 Photo 11: Tissue Simulant Liquid for Head 2600 Photo 12: Tissue Simulant Liquid for Body 2600



Photo 14: Left tilted 15 degree

3. Photographs of EUT test position

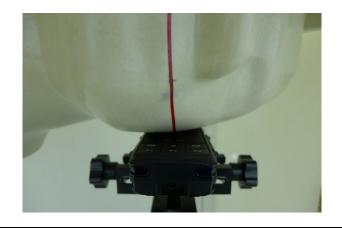


Photo 13: Left touch cheek

Photo 15: Right touch cheek

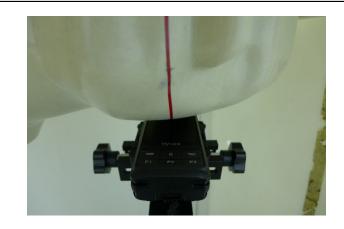


Photo 16: Right tilted 15 degree

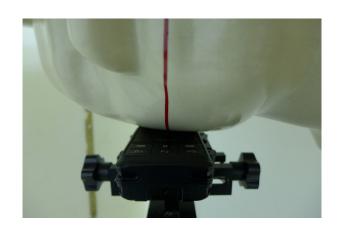


Photo 17: Front side 15mm

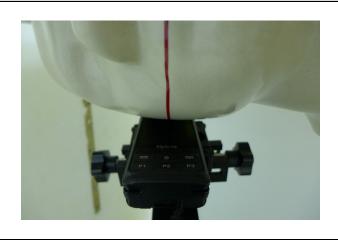


Photo 18: Back side 15mm







Photo 19: Front side 10mm



Photo 20: Back side 10mm



Photo 21: Left side 10mm



Photo 22: Right side 10mm



Photo 23: Top side 10mm



Photo 24: Bottom side 10mm





Photo 25: Back splint 0mm	NA
	NA



4. EUT Constructional Details

Photo 26: Front View	Photo 27: Back View
Hyten 1 2 3 4 5 6 7 8 9 10 1 2 3 4 5 6 7 8 9 20 1 2 1	1234567891012345678920123
Photo 28: Accessory	NA
1 2 3 4 5 6 7 8 9 10 1 2 3 4 5 6 7 8 9 20 1 2 3 4 5 6 7 8 9 30 1 2 3	NA