

Appendix D

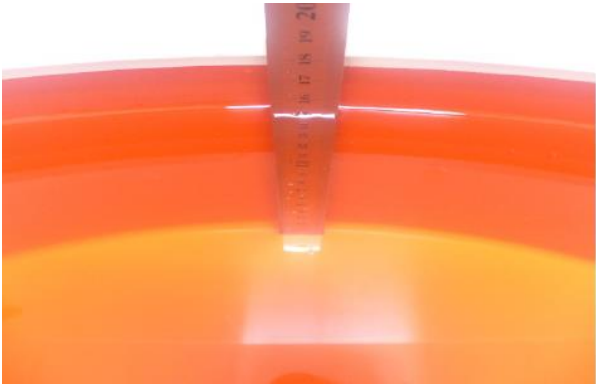
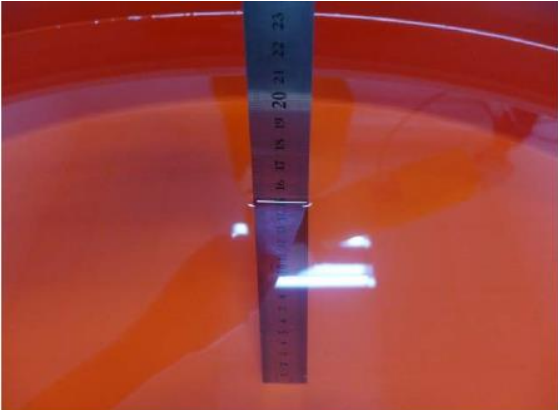
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1800	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	Photo 6: Tissue Simulant Liquid for Head 5GHz
	

3. Photographs of EUT test position

Photo 7: Bottom Face 0mm	Photo 8: Bottom Face 10mm
	
Photo 9: Edge 1 0mm	Photo 10: Edge 1 10mm
	
Photo 11: Edge 2 0mm	Photo 12: Edge 3 0mm
	

Photo 13: Edge 4 0mm



4. EUT Constructional Details

Photo 14: Front View



Photo 15: Back View

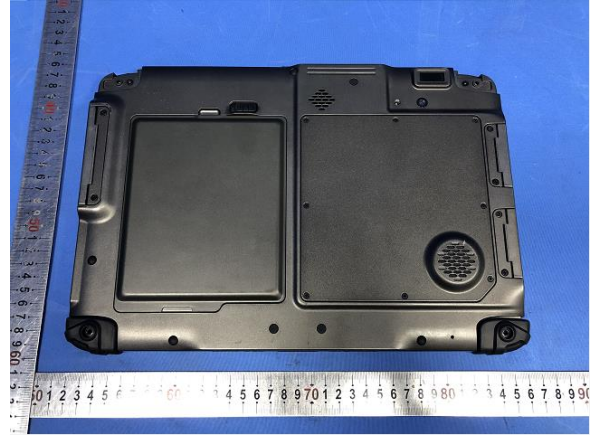


Photo 16: Left View



Photo 17: Right View



Photo 18: Top View



Photo 19: Bottom View



Photo 20: Front View	Photo 21: Back View
	
Photo 22: Back View	
	