


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

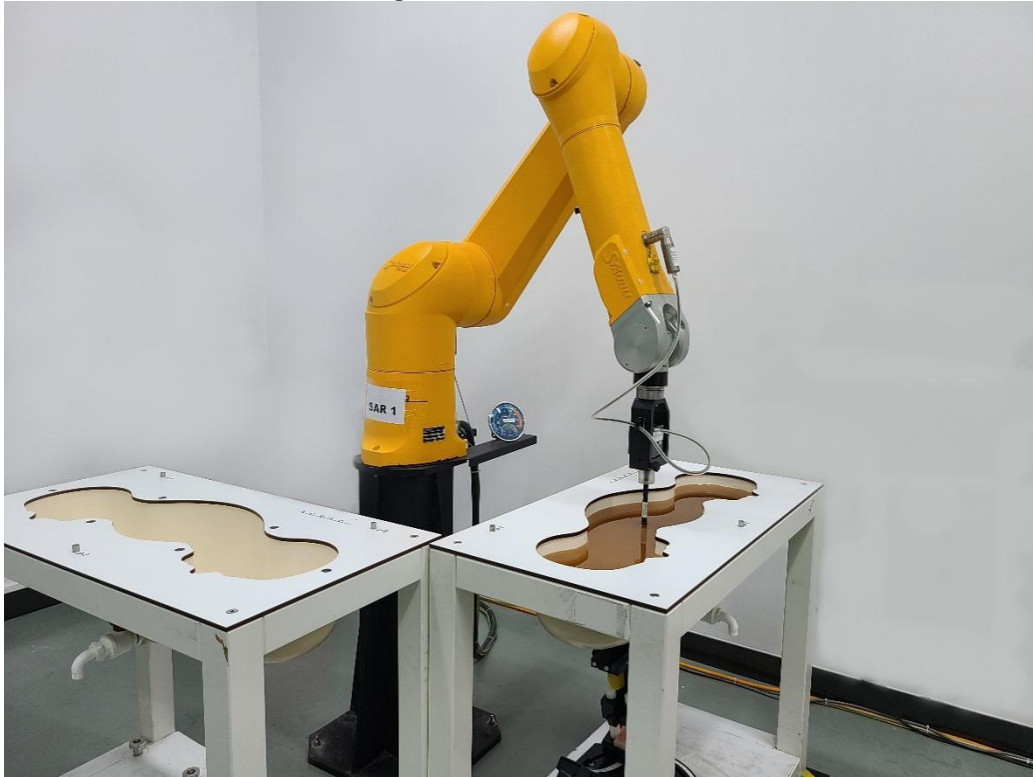

2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
 A photograph showing a cross-section of a container filled with a yellowish, translucent liquid. A metal ruler is placed vertically next to the container, with the numbers 6, 7, 8, 9, 10, 11, and 12 visible. The liquid level is approximately at the 10 cm mark. The container has a blue outer rim and a white inner lining.	NA

3. Photographs of EUT test position

Photo 2: Back side 0mm Ant1

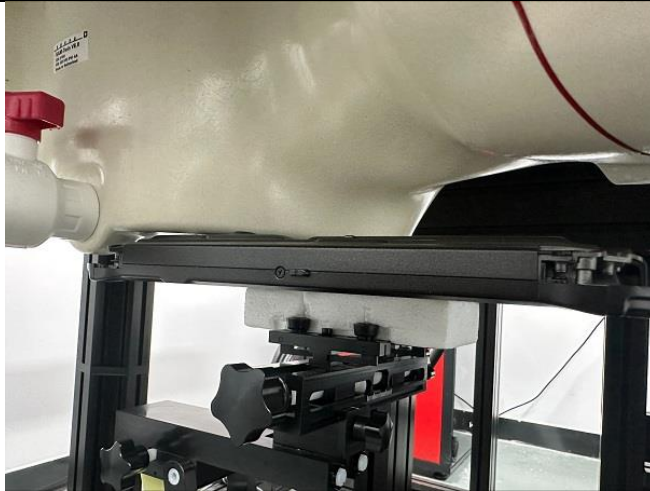


Photo 3: Back side 0mm Ant2



Photo 4: Edge 1 0mm



Photo 5: Edge 2 0mm

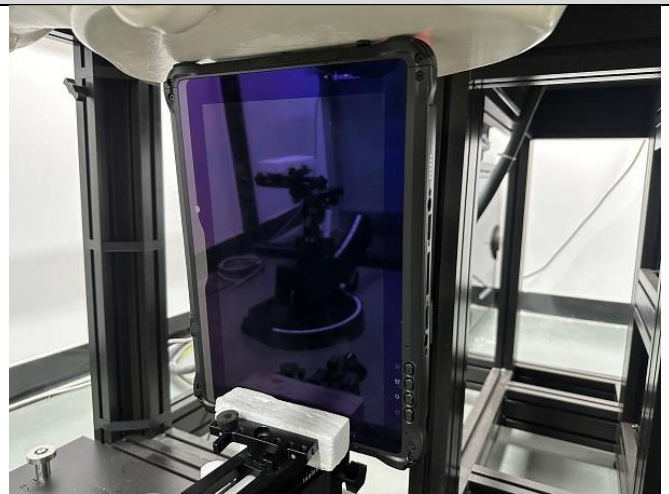


Photo 6: Edge 3 0mm

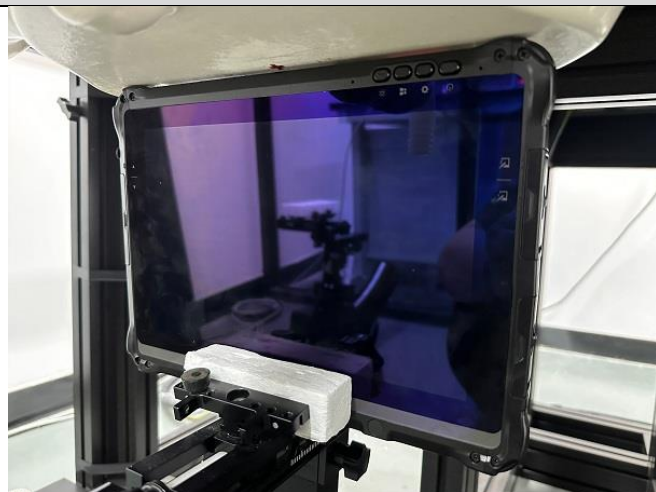


Photo 7: Edge 4 0mm

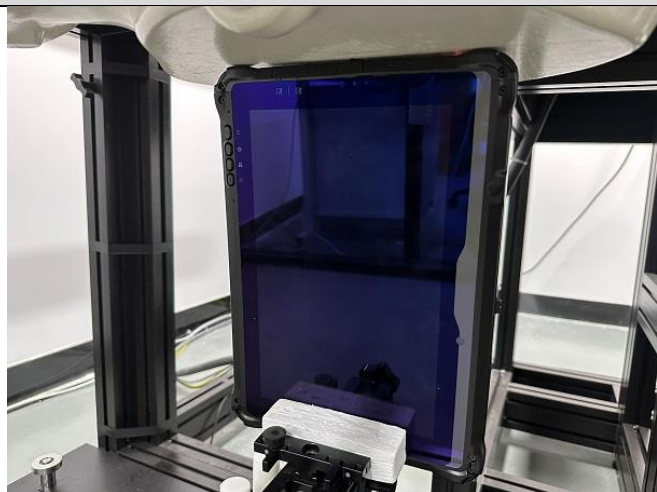


Photo 8: Edge 2 0mm+back clip


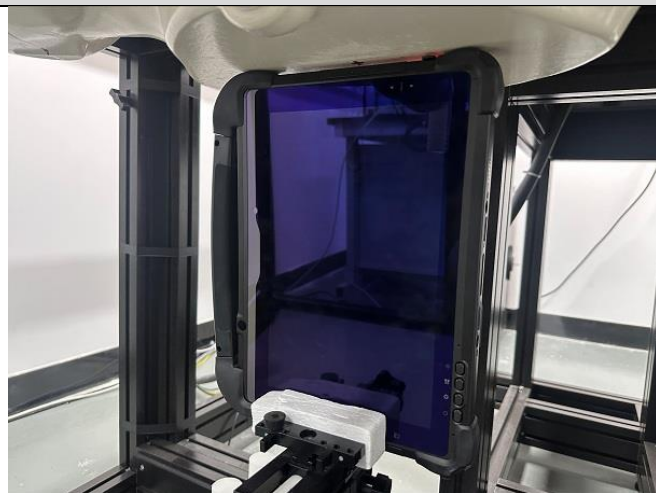


Photo 9: Edge 4 0mm+back clip



4. EUT Constructional Details

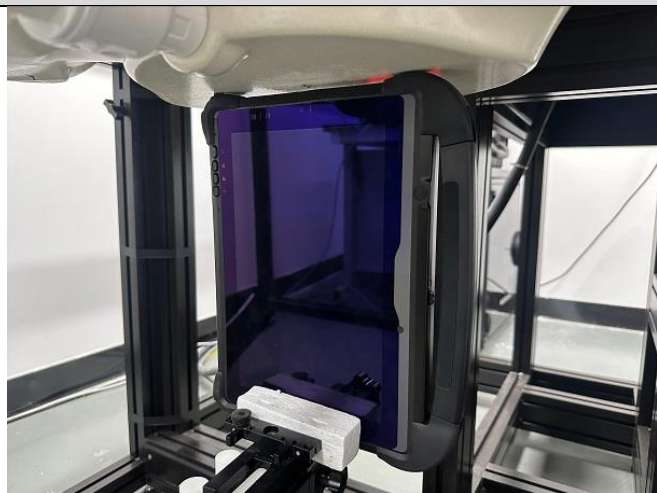