

EMV TESTHAUS

Test Report

Customer:

Esterline | LRE Medical GmbH

Georg-Brauchle-Ring 89
80992 München
Tel.: +49 89 354803-0
Fax: +49 89 354803-67

RF test report

140206-AU01+W02



Esterline | LRE Medical GmbH
Laboratory Equipment with RFID

Aspect-Reader™



The test result refers exclusively
to the tested model.
This test report may not be copied or
published in a part without the written
authorization
of the accreditation agency and/or
EMV TESTHAUS GmbH
Revision: 1.0



EMV **TESTHAUS** GmbH

Gustav-Hertz-Straße 35
94315 Straubing
Tel.: +49 9421 56868-0
Fax: +49 9421 56868-100
Email: info@emv-testhaus.com

Accreditation:



FCC facility registration number: 221458
Test Firm Type "2.948 listed": Valid until 2017-04-22
Test Firm Type "accredited": Valid until 2015-06-11
MRA US-EU, FCC designation number: DE0010
BnetzA-CAB-02/21-02/04 Valid until 2018-11-27

Industry Canada test site number: 3472A-1
Registration expiry date: 2015-10-02

Test Laboratory:

EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany

The technical accuracy is guaranteed through the quality management of the
EMV **TESTHAUS** GmbH



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

Table of contents

1	Test regulations	5
2	Equipment under Test (EUT)	6
3	AC power line conducted emissions	9
4	Radiated emission measurement (<1 GHz)	17
5	Radiated emission measurement (>1 GHz)	29
6	Carrier frequency stability	30
7	Bandwidths	34
8	Equipment calibration status	39
9	Measurement uncertainty	40
10	Summary	41
11	Revision History	42

List of pictures

Picture 1: Outline of conducted emission test setup	10
Picture 2: Graphic - Conducted emission on mains, phase 1 (without termination).....	11
Picture 3: Table - Conducted emission on mains, phase 1 (without termination)	12
Picture 4: Graphic - Conducted emission on mains, neutral (without termination).....	13
Picture 5: Table - Conducted emission on mains, neutral (without termination)	14
Picture 6: Graphic - Conducted emission on mains, phase 1 (with termination 50 Ω)	15
Picture 7: Graphic - Conducted emission on mains, neutral (with termination 50 Ω).....	16
Picture 8: Test setup for radiated emission measurement (< 30 MHz).....	20
Picture 9: Test setup for radiated emission measurement (< 1 GHz).....	20
Picture 10: Radiated emission 9 kHz – 30 MHz @ 3m distance (13.56 MHz)	22
Picture 11: Radiated emission 30 MHz - 1000MHz @ 3m distance	26
Picture 12: Spectrum mask for 13.56 MHz @ 3m distance.....	28
Picture 13: Test setup for carrier frequency stability measurement.....	31
Picture 14: Occupied bandwidth (99 %).....	36
Picture 15: -6 dB emission bandwidth.....	37
Picture 16: -20 dB emission bandwidth.....	38

List of tables

Table 1: Equipment calibration status.....	39
Table 2: Measurement uncertainty	40

1 Test regulations

47 CFR Part 2: 10-2013	Code of Federal Regulations Part 2 (Frequency allocation and radio treaty matters; General rules and regulations) of the Federal Communication Commission (FCC)
47 CFR Part 15: 10-2013	Code of Federal Regulations Part 15 (Radio Frequency Devices) of the Federal Communication Commission (FCC)
ANSI C63.4: September 2009	American National Standard for Methods of Measurement of Radio-Noise Emissions from Low-Voltage Electrical and Electronic Equipment in the Range of 9 kHz to 40 GHz
ICES-003 Issue 5, August 2012	Spectrum Management and Telecommunications Interference-Causing Equipment Standard Information Technology Equipment (ITE) – Limits and methods of measurement
RSS-Gen Issue 3, December 2010	Spectrum Management and Telecommunications Radio Standards Specification General Requirements and Information for the Certification of Radiocommunication Equipment
RSS-102 Issue 4, March 2010, updated December 2010	Spectrum Management and Telecommunications Radio Standards Specification Radio Frequency (RF) Exposure Compliance of Radiocommunication Apparatus (All Frequency Bands)
RSS-210 Issue 8, December 2010	Spectrum Management and Telecommunications Radio Standards Specification Licence-exempt Radio Apparatus (All Frequency Bands): Category I Equipment

1.1 Summary of test results

Standard	Test result
47 CFR Part 15, sections 15.207 and 15.225	Passed
RSS-210 Issue 8 Annex A2.6 (with appropriate references to RSS-Gen Issue 3)	Passed



2 Equipment under Test (EUT)

Product type:	Laboratory Equipment with RFID
Model Name:	Aspect-Reader™
Manufacturer:	Esterline LRE Medical GmbH
Serial number:	00001012
FCC ID:	YMQ-8048000
IC Canada:	- - -
Application frequency band:	13.110 to 14.010 MHz
Frequency range:	13.560 MHz
Operating frequency:	13.560 MHz
Number of RF-channels:	1
Modulation:	ASK
Antenna types:	2 PCB antennas: - Cartridge-antenna - User-antenna <input type="checkbox"/> detachable <input checked="" type="checkbox"/> not detachable
Power supply:	External power source nominal: 6.0 VDC
Temperature range:	+15°C to +30°C

Remark:

The tests were performed with 120V AC / 60Hz.



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

2.1 Photo documentation

For photos of the EUT, see annex B.

For photos taken during testing and the EUT-positions, see annex A.

2.2 Short description of the EUT

The EUT is an evaluation system for laboratories which operates with two separate RFID-antennas. One is for identifying the operator (“User-antenna”), the other is for reading data from an OP-cartridge (“Cartridge-antenna”).

2.3 Operation mode

During the pre-tests it was observed that the “continuous-tag-reading-mode” is the respective worst- case with the User-antenna. Therefore this mode was selected for final testing. The device was configured by manufacturer to activate the RFID reader for continuous transmission via RFID card.

The EUT was tested in the 3 orthogonal positions. This is documented in annex A.



2.4 Configuration

The following peripheral devices and interface cables were connected during the tests:

Device	Model:	Serial or inventory number
Laboratory Equipment with RFID	Aspect-Reader™	00001012
SINPRO Switching Power Supply	MPU30-102	07092581
RFID tag	User-tag	0103
RFID tag	OP-cartridge	n/a
Power Supply	Statron 3231.1	E00017
Multimeter	Gossen METRAhit 29S	E00099

2.5 Used cables

Numbers:	Description: (type / lengths / remarks)	Serial No
2	Laboratory cables with banana connector, 2.0m	n/a

Note: As declared by applicant ethernet and USB ports are not used during normal operation but for service purposes only. Therefore during testing no cables were connected to these ports.

3 AC power line conducted emissions

according to 47 CFR Part 15, section 15.207, and
RSS-210, section 2.1 with RSS-Gen, section 7.2.4

3.1 Test location

Description	Manufacturer	Inventory No.
Shielded room	Siemens - Matsushita	E00107

3.2 Test instruments

	Description	Manufacturer	Inventory No.
<input checked="" type="checkbox"/>	ESCS 30	Rohde & Schwarz	E00003
<input type="checkbox"/>	ESU 26	Rohde & Schwarz	W00002
<input type="checkbox"/>	ESCI	Rohde & Schwarz	E00001
<input checked="" type="checkbox"/>	ESH2-Z5	Rohde & Schwarz	E00004
<input type="checkbox"/>	ESH2-Z5	Rohde & Schwarz	E00005

3.3 Limits


Frequency [MHz]	Quasi-peak [dB μ V]	Avarage [dB μ V]
0.15 – 0.5	66 – 56	56 – 46
0.5 – 5.0	56	46
5 – 30	60	50

3.4 Test procedure

1. The tests of conducted emission were carried out in a shielded room using a line impedance stabilization network (LISN) 50 μ H/50 Ohms and an EMI test receiver.
2. The EMI test receiver was connected to the LISN and set to a measurement bandwidth of 9 kHz in the frequency range from 0.15 MHz to 30 MHz.
3. The EUT was placed on a wooden table and connected to the LISN.
4. To accelerate the measurement the detector of the EMI test receiver was set to peak and the whole frequency range from 0.15 MHz to 30 MHz was scanned.
5. After that all peaks values with less margin than 10 dB to quasi-peak limit or exceeding the limit were marked and re-measured with quasi-peak detector.
6. If after that all values are under the average limit no addition measurement is necessary. In case there are still values between quasi-peak and average limit then these values were re-measured with average detector.
7. These measurements were done on all power lines.

According to ANSI C63.4, section 13.3.1 testing of intentional radiators with detachable antennas shall be done with a dummy load otherwise the tests should be done with connected antenna and if adjustable fully extended.

3.5 Test setup

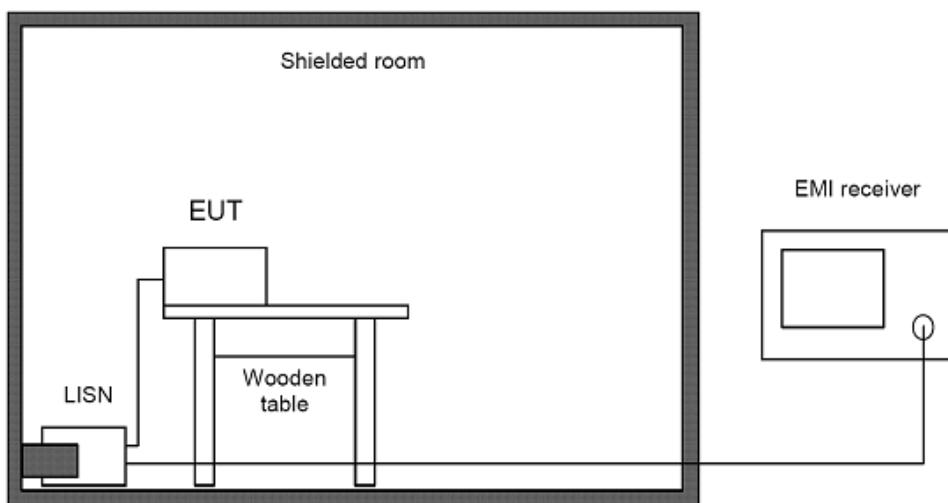


Picture 1: Outline of conducted emission test setup

Comments: All peripheral devices were additionally decoupled by means of a line stabilization network.

3.6 Test results

Temperature:	22°C	Humidity:	43%
Tested by:	Martin Müller	Test date:	2014-09-30

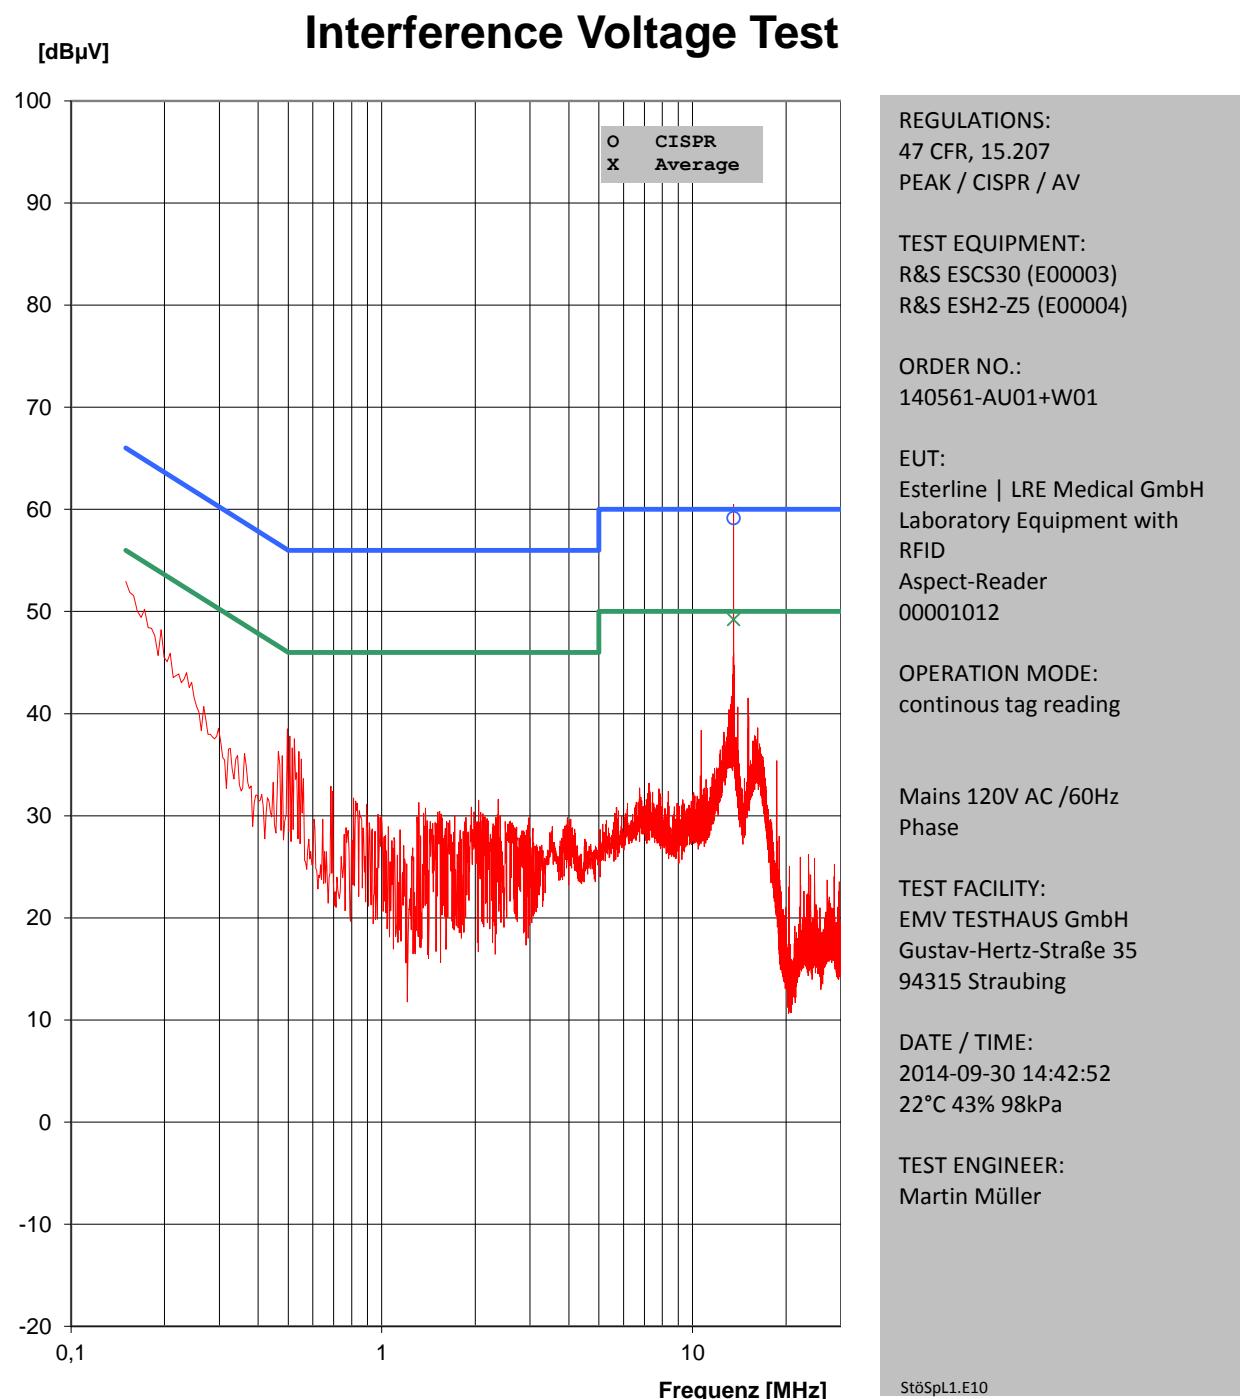

Picture 2: Graphic - Conducted emission on mains, phase 1 (without termination)



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

Interference Voltage Test

Freq. [MHz]	U_CISPR [dB μ V]	Limit [dB μ V]	delta_U [dB]	U_AV [dB μ V]	Limit [dB μ V]	delta_U [dB]	Corr. [dB]	Remark
13,56	59,1	60,0	0,9	49,2	50,0	0,8	0,0	St6Spl1.F10


Picture 3: Table - Conducted emission on mains, phase 1 (without termination)



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

Interference Voltage Test

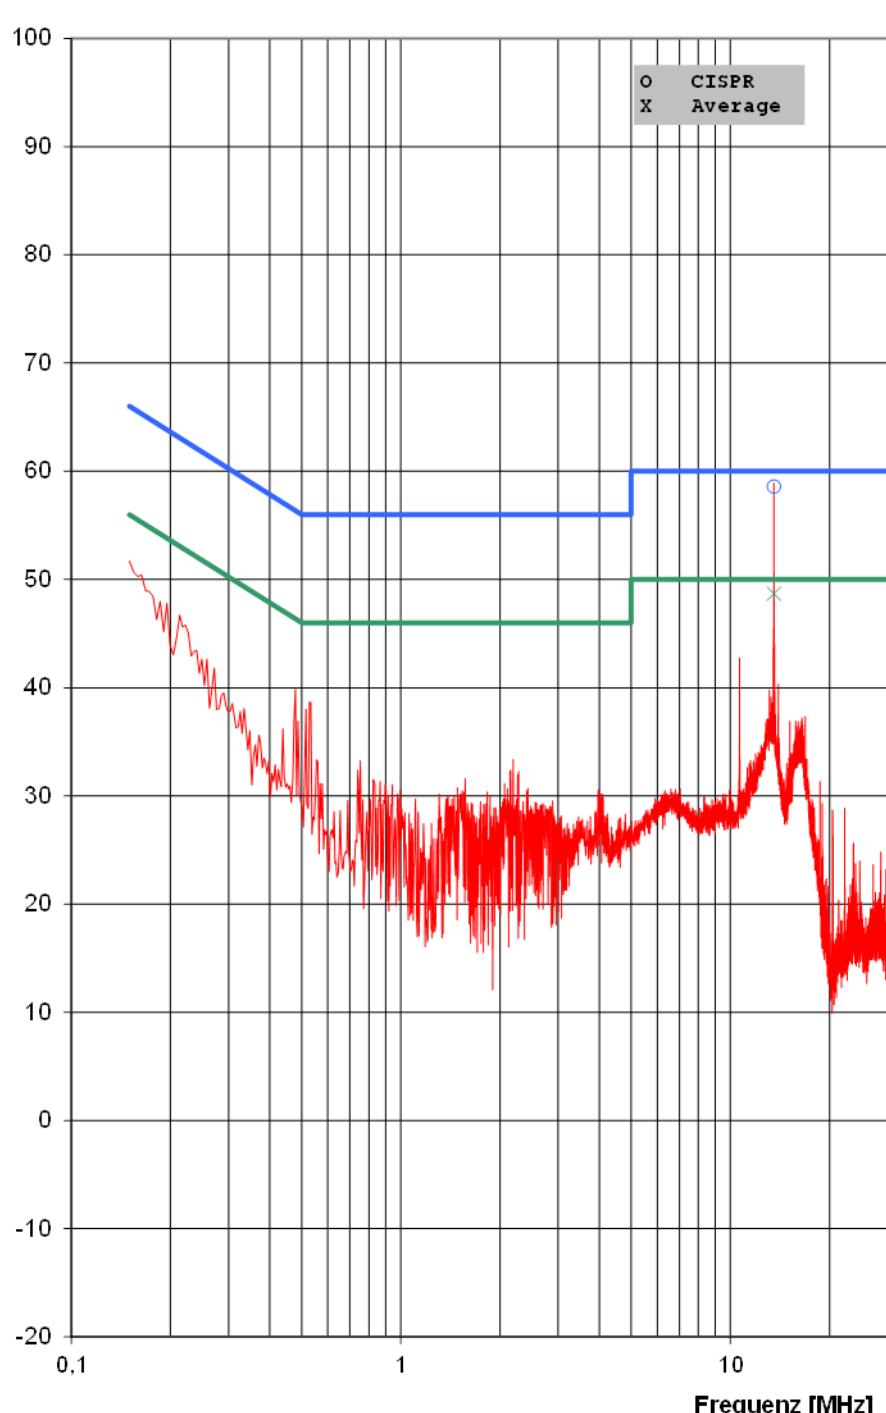

REGULATIONS:
47 CFR, 15.207
PEAK / CISPR / AV

TEST EQUIPMENT:
R&S ESCS30 (E00003)
R&S ESH2-Z5 (E00004)

ORDER NO.:
140561-AU01+W01

EUT:
Esterline | LRE Medical GmbH
Laboratory Equipment with
RFID
Aspect-Reader
00001012

OPERATION MODE:
continuous tag reading

Mains 120V AC /60Hz
Neutral

TEST FACILITY:
EMV TESTHAUS GmbH
Gustav-Hertz-Straße 35
94315 Straubing

DATE / TIME:
2014-09-30 14:52:27
22°C 43% 98kPa

TEST ENGINEER:
Martin Müller

StöSpN.E10

Picture 4: Graphic - Conducted emission on mains, neutral (without termination)



EMV TESTHAUS GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

Interference Voltage Test

Freq. [MHz]	U_CISPR [dB μ V]	Limit [dB μ V]	delta_U [dB]	U_AV [dB μ V]	Limit [dB μ V]	delta_U [dB]	Corr. [dB]	Remark
13,56	58,6	60,0	1,4	48,7	50,0	1,3	0,0	St6SpN F10


Picture 5: Table - Conducted emission on mains, neutral (without termination)



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

Interference Voltage Test

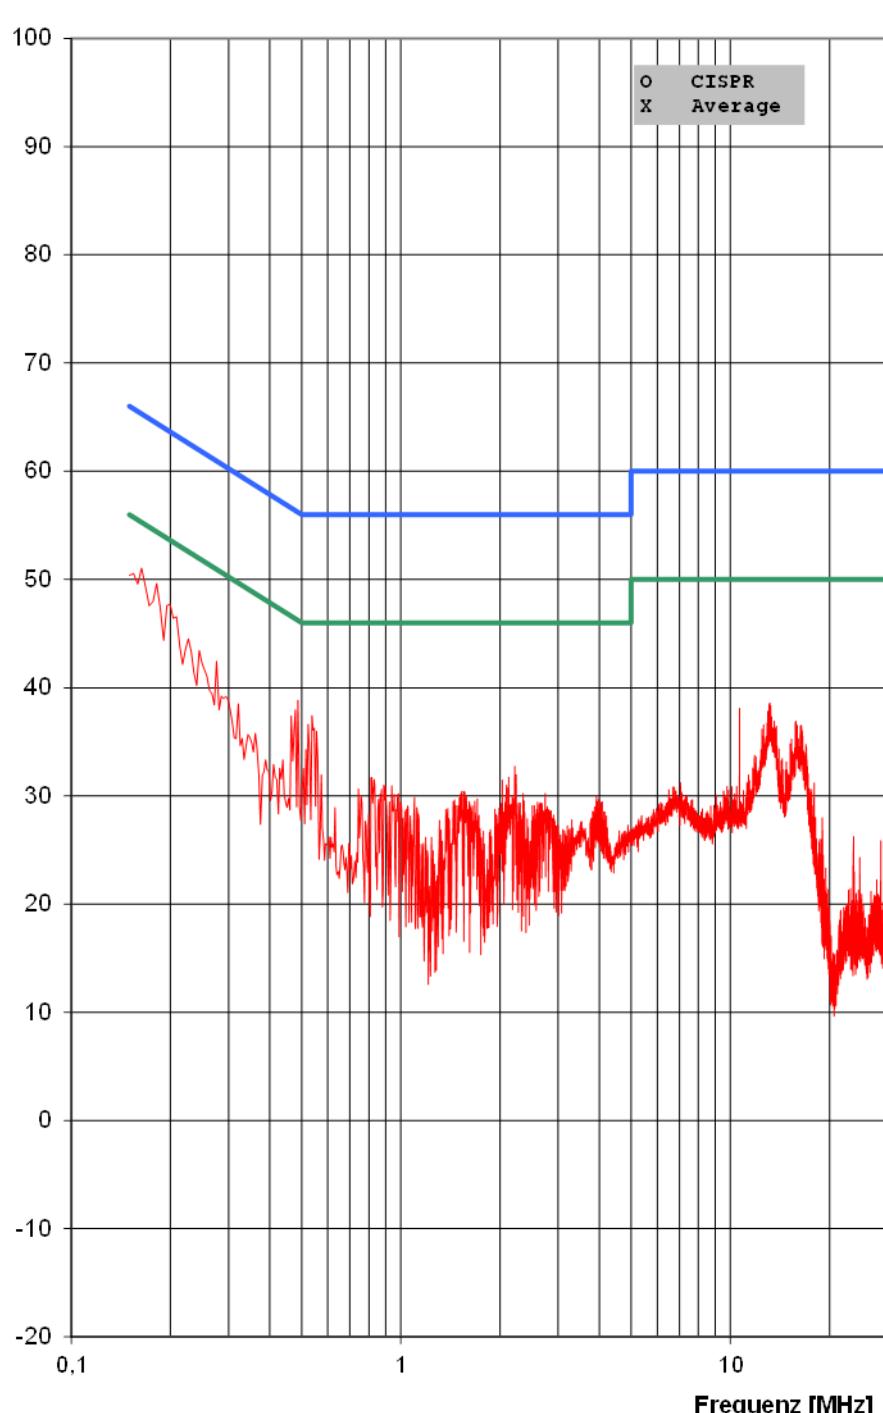

REGULATIONS:
47 CFR, 15.207
PEAK / CISPR / AV

TEST EQUIPMENT:
R&S ESCS30 (E00003)
R&S ESH2-Z5 (E00004)

ORDER NO.:
140561-AU01+W01

EUT:
Esterline | LRE Medical GmbH
Laboratory Equipment with
RFID
Aspect-Reader
00001012

OPERATION MODE:
antenna terminated with
50Ω

Mains 120V AC /60Hz
Phase

TEST FACILITY:
EMV TESTHAUS GmbH
Gustav-Hertz-Straße 35
94315 Straubing

DATE / TIME:
2014-09-30 15:05:20
22°C 43% 98kPa

TEST ENGINEER:
Martin Müller

StöSpL1_02.E10


Picture 6: Graphic - Conducted emission on mains, phase 1 (with termination 50 Ω)



EMV TESTHAUS GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

Interference Voltage Test

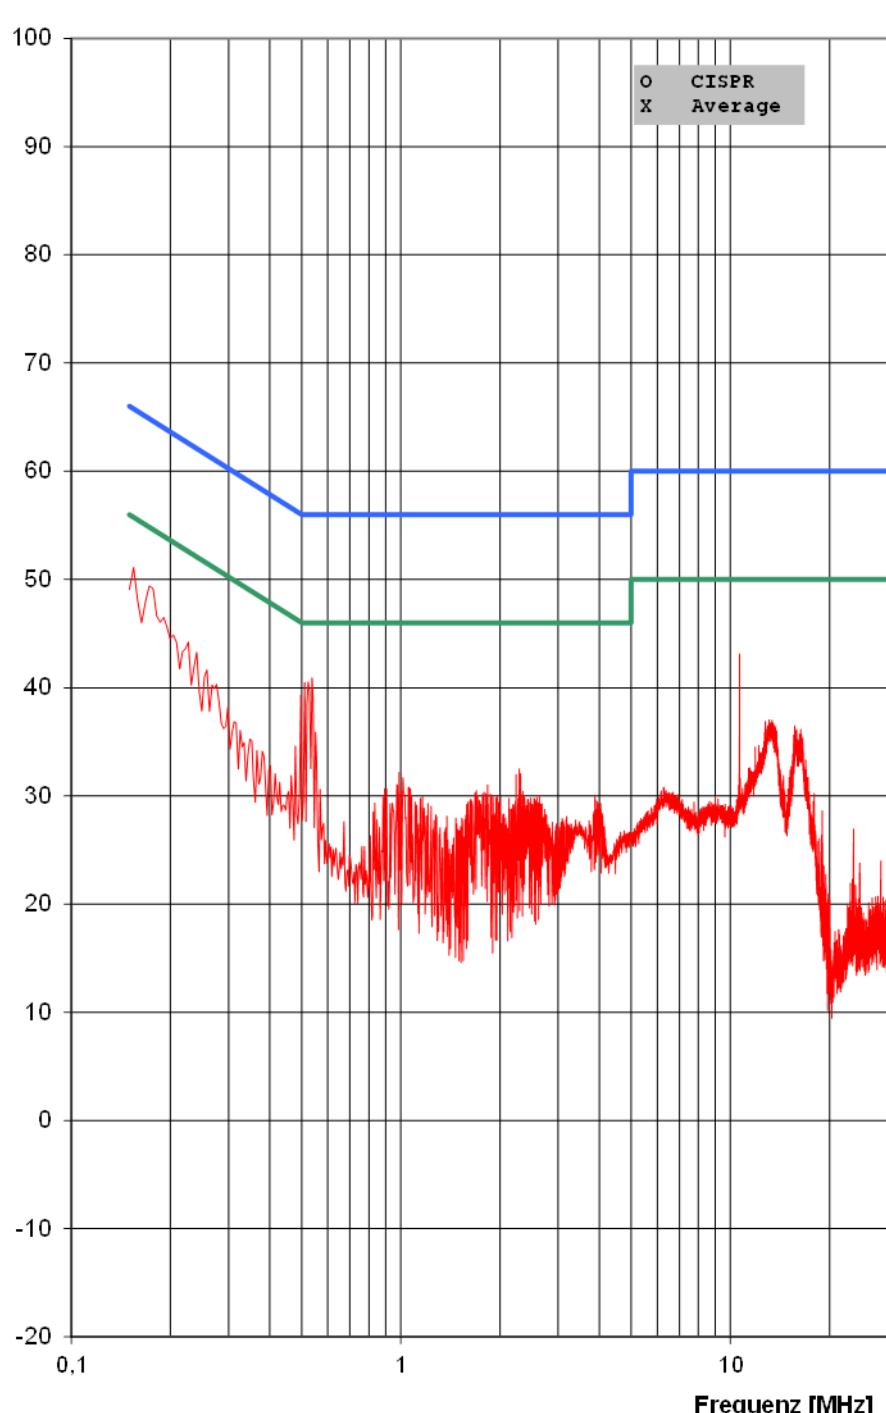

REGULATIONS:
47 CFR, 15.207
PEAK / CISPR / AV

TEST EQUIPMENT:
R&S ESCS30 (E00003)
R&S ESH2-Z5 (E00004)

ORDER NO.:
140561-AU01+W01

EUT:
Esterline | LRE Medical GmbH
Laboratory Equipment with
RFID
Aspect-Reader
00001012

OPERATION MODE:
antenna terminated with
50Ω

Mains 120V AC /60Hz
Neutral

TEST FACILITY:
EMV TESTHAUS GmbH
Gustav-Hertz-Straße 35
94315 Straubing

DATE / TIME:
2014-09-30 15:05:37
22°C 43% 98kPa

TEST ENGINEER:
Martin Müller

StöSpN_02.E10

Picture 7: Graphic - Conducted emission on mains, neutral (with termination 50 Ω)



EMV TESTHAUS GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

4 Radiated emission measurement (<1 GHz)

according to 47 CFR Part 15, section 15.205(a), 15.209(a),
15.225(a) to (e), and
RSS-210, section 2.5 and Annex 2.6 with RSS-Gen, sections 7.2.2
and 7.2.5

4.1 Test Location

- Scan with peak detector in 3 m CDC.
- Final CISPR measurement with quasi peak detector on 3 m open area test site.

Description	Manufacturer	Inventory No.
CDC	Albatross Projects	E00026
Open area test site (OATS)	EMV TESTHAUS GmbH	E00354

4.2 Test instruments

	Description	Manufacturer	Inventory No.
<input checked="" type="checkbox"/>	ESCS 30 (FF)	Rohde & Schwarz	E00551
<input type="checkbox"/>	ESU 26	Rohde & Schwarz	W00002
<input checked="" type="checkbox"/>	ESCI (CDC)	Rohde & Schwarz	E00001
<input checked="" type="checkbox"/>	VULB 9163 (FF)	Schwarzbeck	E00013
<input checked="" type="checkbox"/>	VULB 9160 (CDC)	Schwarzbeck	E00011
<input checked="" type="checkbox"/>	HFH2-Z2	Rohde & Schwarz	E00060
<input checked="" type="checkbox"/>	Feedline OATS	Huber & Suhner	200024



4.3 Limits

The field strength of any emissions appearing outside of the 13.110 to 14.010 MHz band including spurious emissions falling into restricted bands as specified in 15.205(a) shall not exceed the general radiated emission limits as specified in 15.209.

Frequency [MHz]	Field strength Fs [μ V/m]	Field strength [dB μ V/m]	Measurement distance d [m]
0.009 – 0.490	266.6 – 4.9	48.5 – 13.8	300
0.490 – 1.705	48.98 – 14.08	33.8 – 22.97	30
1.705 – 30.0	30	29.54	30
30 – 88	100	40	3
88 – 216	150	43.5	3
216 - 960	200	46	3
Above 960	500	54	3

As noted in 15.205(d)(7) devices according to 15.225 are exempt from complying with restricted band requirements for the 13.36 to 13.41 MHz band. Instead they have to comply with the limits as specified in 15.225 (a) to (d):


Frequency [MHz]	Field strength Fs [μ V/m]	Field strength [dB μ V/m]	Measurement distance d [m]
13.553 - 13.567	15,848	84	30
13.410 - 13.553	334	50.47	30
13.567 - 13.710	334	50.47	30
13.110 - 13.410	106	40.51	30
13.710 - 14.010	106	40.51	30
f < 13.110			according to limits in §15.209
f > 14.010			

4.4 Test procedure


1. EUT was configured according to ANSI C63.4. It was placed on the top of the turntable 0.8 meter above ground. The receiving antenna was placed 3 meters from the turntable. The test setup was placed inside a compact diagnostic chamber.
2. EUT and all peripherals were powered on.
3. The broadband antenna was set to vertical polarization.
4. The EMI receiver performed a scan from 30 MHz to 1000 MHz with peak detector peak and measurement bandwidth set to 120 kHz.
5. The turn table was rotated to 6 different positions (360° / 6) and the antenna polarization was changed to horizontal.
6. Test procedure at step 4 and 5 was repeated.
7. The test setup was then placed in an OATS at 3 m distance and all peak values over or with less margin to the limit than 6dB were marked and re-measured with a quasi-peak detector.
8. The turntable was rotated by 360 degrees to determine the position of the highest radiation.
9. The height of the broadband receiving antenna was varied between one meter and four meters above ground to find the maximum emission field strength of both horizontal and vertical polarization. The highest value was recorded.
10. For emissions below 30 MHz measurements were done using a loop antenna. Prescan was performed with peak detector and final measurements with quasi-peak except for the frequency bands 9 to 90 kHz and 110 to 490 kHz where average detector applies. Antenna height was not changed during this test. Appropriate CISPR bandwidths of 200 Hz for frequencies up to 150 kHz and 9 or 10 kHz for frequencies above were used.



4.5 Test setup

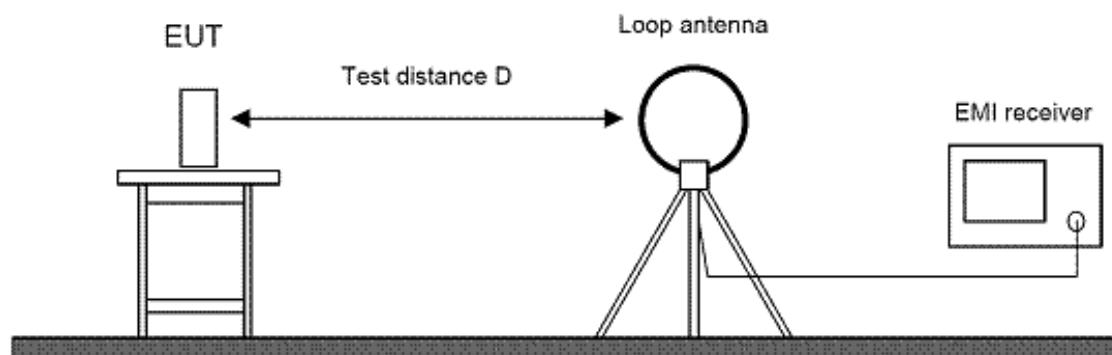

Picture 8: Test setup for radiated emission measurement (< 30 MHz)

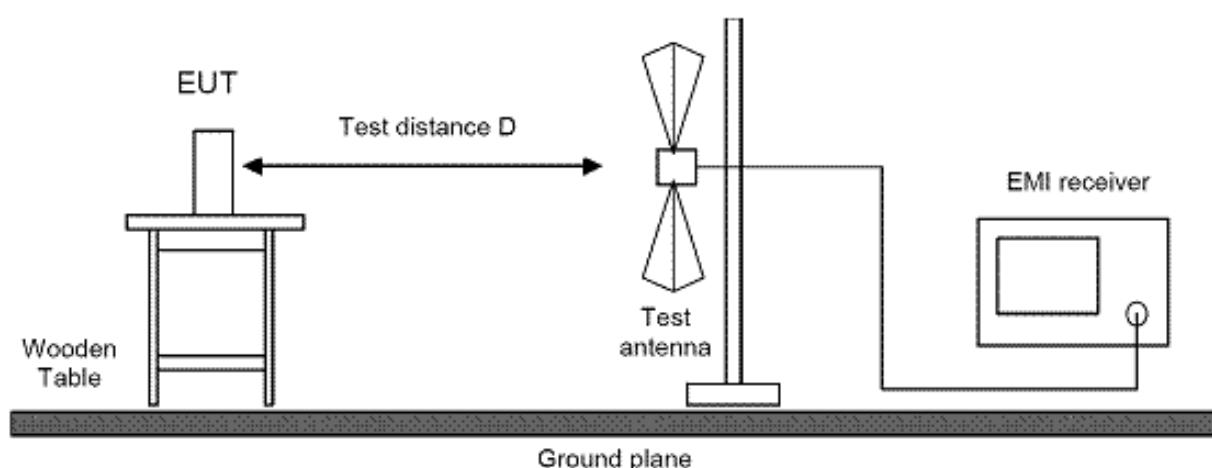

Picture 9: Test setup for radiated emission measurement (< 1 GHz)

4.6 Test deviation

There is no deviation from the standards referred to.

4.7 Test results

Temperature:	21°C	Humidity:	45%
Tested by:	Martin Müller	Test date:	2014-09-19

Radiated Emission Measurement 9 kHz - 30 MHz

Test procedure


The EUT was placed in a full anechoic chamber and the spurious emission testing was performed in accordance with ANSI C63.4, 47 CFR Part 15, Subpart C. The measurement distance was 3 m.

The following picture shows the worst-case-emissions at EUT-position 2, loop-antenna polarised to "I".



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

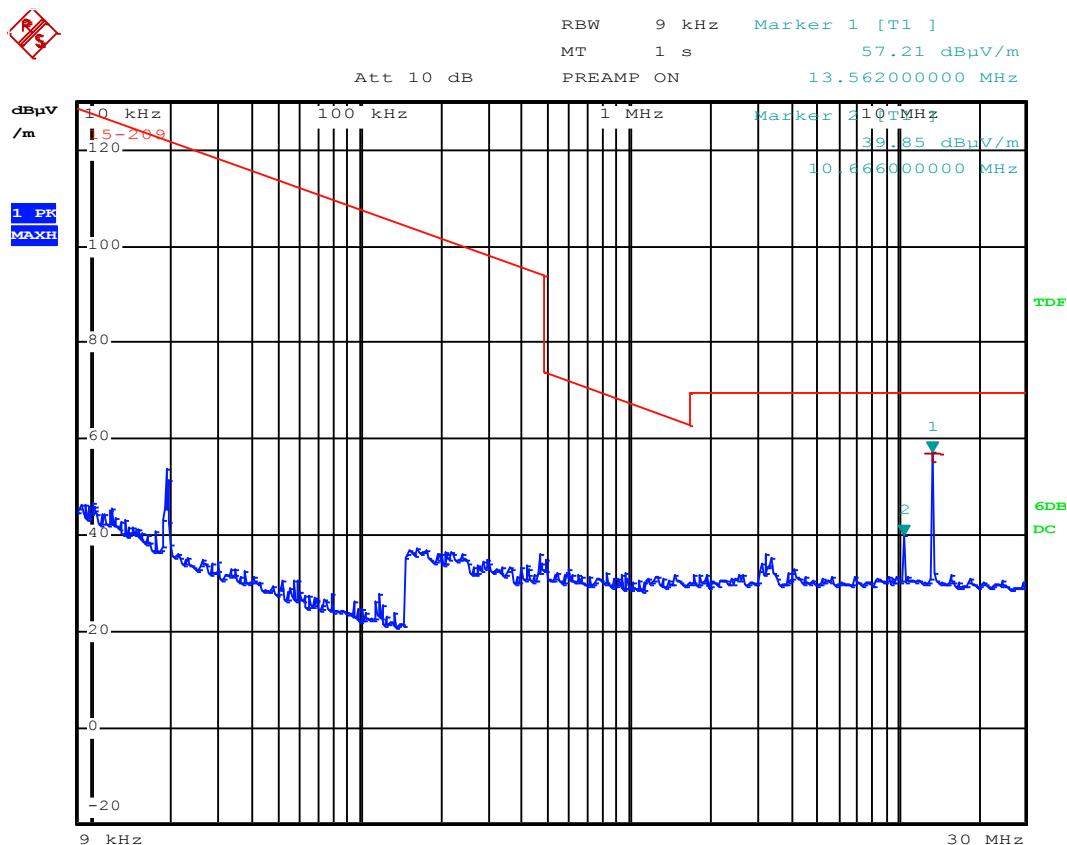

Frequency (MHz)	Measured value (dB μ V/m)	Detector	Recalculation factor (dB/decade)	Field strength (dB μ V/m)	Limit (dB μ V/m)	Margin	Result
13.56	56.88	QP	40	16.88	84	-67.12	PASS

Note:


Measured value = 56.88 dB μ V/m @ 3 m

Recalculation factor = 40 dB / decade

Recalculated value = 56.88 dB μ V/m @ 3 m - 40 dB = 16.88 dB μ V/m @ 30 m

Radiated Emission Measurement 30 MHz - 1000 MHz

The following picture shows the worst-case-emissions at EUT-position 1.

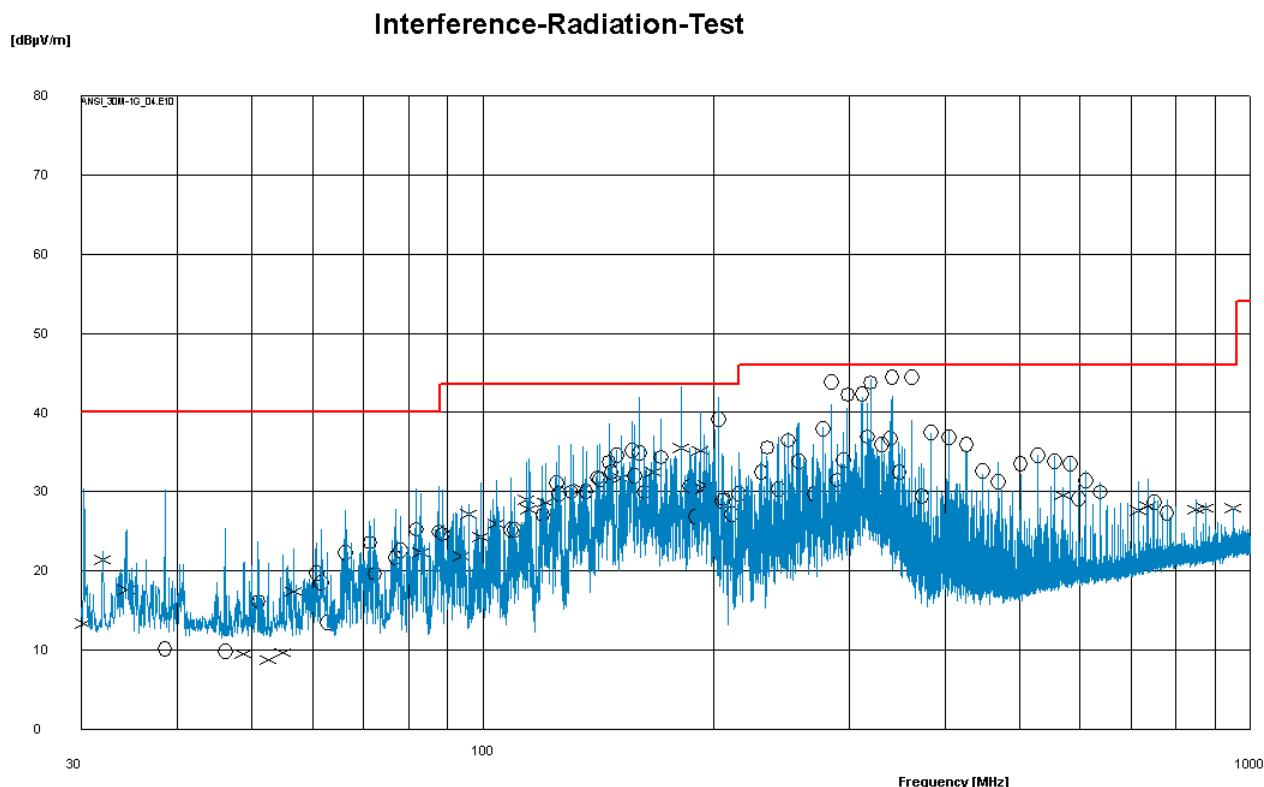

Interference Radiation Test

Freq. [MHz]	U_Rec [dB μ V/m]	Limit [dB μ V/m]	Corr. [dB]	U_Ant. [dB μ V]	delta_U [dB]	Turn- table	Antenna	Pol.	Remark
30,24	13,4	40,0	12,2	1,2	26,6	47°	100 cm	V	ANSI_30M-1G_04.F10
31,98	21,4	40,0	12,1	9,3	18,6	32°	100 cm	V	
34,38	17,7	40,0	12,1	5,6	22,3	207°	100 cm	V	
38,52	10,2	40,0	12,8	-2,6	29,8	113°	100 cm	H	
46,14	9,9	40,0	12,7	-2,7	30,1	327°	100 cm	H	
48,78	9,5	40,0	12,7	-3,2	30,5	20°	100 cm	V	
51,00	16,2	40,0	12,7	3,5	23,8	103°	100 cm	H	
52,50	8,8	40,0	12,6	-3,8	31,2	17°	100 cm	V	
54,96	9,7	40,0	12,6	-2,9	30,3	45°	100 cm	V	
56,70	17,4	40,0	12,5	4,9	22,6	29°	100 cm	V	
60,66	19,7	40,0	12,2	7,5	20,3	111°	100 cm	H	
61,62	18,6	40,0	12,0	6,6	21,4	99°	100 cm	H	
62,70	13,6	40,0	11,8	1,8	26,4	111°	100 cm	H	
66,30	22,4	40,0	11,0	11,3	17,6	99°	100 cm	H	
71,28	23,6	40,0	10,1	13,5	16,4	111°	100 cm	H	
72,30	19,7	40,0	9,9	9,8	20,3	103°	100 cm	H	
76,92	21,8	40,0	9,1	12,7	18,2	111°	100 cm	H	
78,06	22,6	40,0	8,9	13,7	17,4	315°	100 cm	H	
81,96	25,3	40,0	8,8	16,5	14,7	327°	100 cm	H	
82,98	22,4	40,0	9,0	13,4	17,6	42°	100 cm	V	
87,66	25,0	40,0	9,6	15,4	15,0	331°	100 cm	H	
88,74	24,7	43,5	9,7	15,0	18,8	-1°	100 cm	H	
93,90	21,9	43,5	10,1	11,8	21,6	274°	100 cm	V	
96,00	27,2	43,5	10,2	17,0	16,3	290°	100 cm	V	
99,36	24,3	43,5	10,4	13,9	19,2	318°	100 cm	V	
104,34	26,0	43,5	10,9	15,1	17,5	331°	100 cm	V	
108,96	25,2	43,5	11,4	13,9	18,3	33°	100 cm	H	
110,04	25,2	43,5	11,5	13,7	18,3	45°	100 cm	H	
113,94	29,0	43,5	11,9	17,1	14,5	340°	100 cm	V	
115,02	27,8	43,5	12,0	15,8	15,7	343°	100 cm	V	
119,70	27,1	43,5	12,5	14,6	16,4	58°	100 cm	H	
120,72	28,7	43,5	12,5	16,1	14,9	355°	100 cm	V	
124,62	31,2	43,5	12,6	18,5	12,4	70°	100 cm	H	
125,70	29,7	43,5	12,6	17,1	13,8	61°	100 cm	H	
130,32	30,0	43,5	12,8	17,2	13,5	70°	100 cm	H	
135,30	30,4	43,5	13,0	17,4	13,2	343°	100 cm	V	
136,32	30,1	43,5	13,1	17,0	13,4	61°	100 cm	H	
141,00	31,8	43,5	13,3	18,5	11,7	70°	100 cm	H	
142,02	31,5	43,5	13,4	18,2	12,0	61°	100 cm	H	
145,98	33,8	43,5	13,6	20,2	9,7	70°	100 cm	H	



EMV TESTHAUS GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

Interference Radiation Test

Freq. [MHz]	U_Rec [dB μ V/m]	Limit [dB μ V/m]	Corr. [dB]	U_Ant. [dB μ V]	delta_U [dB]	Turn- table	Antenna	Pol.	Remark
147,00	32,5	43,5	13,7	18,8	11,0	58°	100 cm	H	ANSI_30M-1G_04.F10
149,34	34,6	43,5	13,9	20,7	8,9	73°	100 cm	H	
151,62	31,7	43,5	14,0	17,8	11,8	353°	100 cm	V	
156,60	35,3	43,5	14,1	21,2	8,3	58°	100 cm	H	
157,68	32,0	43,5	14,1	17,9	11,5	70°	100 cm	H	
160,02	34,9	43,5	14,1	20,8	8,6	74°	100 cm	H	
162,36	30,0	43,5	14,0	16,0	13,5	70°	100 cm	H	
167,28	32,5	43,5	13,6	18,9	11,0	361°	100 cm	V	
170,70	34,4	43,5	13,2	21,2	9,1	61°	100 cm	H	
181,32	35,5	43,5	11,2	24,3	8,0	130°	107 cm	V	
186,24	30,7	43,5	11,1	19,7	12,8	70°	100 cm	H	
189,18	26,9	43,5	10,8	16,1	16,7	61°	100 cm	H	
192,00	35,1	43,5	11,7	23,5	8,4	129°	103 cm	V	
194,34	30,4	43,5	10,4	20,0	13,1	353°	100 cm	V	
195,42	30,9	43,5	10,3	20,5	12,7	331°	100 cm	V	
202,68	39,1	43,5	12,1	27,0	4,4	69°	158 cm	H	
205,02	28,9	43,5	10,0	18,8	14,7	61°	100 cm	H	
206,10	29,1	43,5	10,0	19,1	14,4	70°	100 cm	H	
210,96	27,2	43,5	10,0	17,1	16,4	62°	100 cm	H	
215,64	29,8	43,5	10,1	19,7	13,7	57°	100 cm	H	
230,58	32,5	46,0	10,8	21,7	13,5	75°	100 cm	H	
234,66	35,6	46,0	11,0	24,6	10,4	57°	100 cm	H	
243,06	30,4	46,0	11,3	19,1	15,7	61°	100 cm	H	
250,02	36,5	46,0	11,4	25,1	9,5	327°	100 cm	H	
258,30	33,9	46,0	11,6	22,3	12,1	62°	100 cm	H	
270,00	29,8	46,0	12,0	17,8	16,2	70°	100 cm	H	
277,38	38,0	46,0	12,2	25,8	8,0	62°	100 cm	H	
284,82	43,9	46,0	14,5	29,3	2,2	332°	105 cm	H	
290,10	31,5	46,0	12,6	19,0	14,5	62°	100 cm	H	
295,32	34,0	46,0	12,7	21,4	12,0	57°	100 cm	H	
298,68	42,3	46,0	14,9	27,4	3,8	58°	107 cm	H	
311,94	42,3	46,0	15,2	27,1	3,7	76°	102 cm	H	
316,62	37,0	46,0	13,1	23,8	9,1	57°	100 cm	H	
319,98	43,8	46,0	15,4	28,4	2,2	51°	107 cm	H	
330,66	35,9	46,0	13,4	22,6	10,1	58°	100 cm	H	
339,06	36,8	46,0	13,5	23,3	9,2	260°	100 cm	H	
341,34	44,5	46,0	16,0	28,5	1,5	51°	107 cm	H	
348,60	32,5	46,0	13,7	18,8	13,5	46°	100 cm	H	
362,64	44,5	46,0	16,5	28,1	1,5	56°	101 cm	H	
373,38	29,4	46,0	14,2	15,3	16,6	124°	100 cm	H	



Interference Radiation Test

Freq. [MHz]	U_Rec [dB μ V/m]	Limit [dB μ V/m]	Corr. [dB]	U_Ant. [dB μ V]	delta_U [dB]	Turn- table	Antenna	Pol.	Remark
384,00	37,5	46,0	14,4	23,1	8,6	115°	100 cm	H	ANSI_30M-1G_04_E10
405,36	36,9	46,0	14,8	22,1	9,1	111°	100 cm	H	
426,66	35,9	46,0	15,3	20,7	10,1	103°	100 cm	H	
448,02	32,7	46,0	15,8	16,9	13,3	111°	100 cm	H	
469,32	31,3	46,0	16,1	15,2	14,7	154°	100 cm	H	
501,78	33,5	46,0	16,5	17,0	12,5	258°	100 cm	H	
528,90	34,7	46,0	17,0	17,7	11,4	223°	100 cm	H	
556,02	33,9	46,0	17,5	16,3	12,1	245°	100 cm	H	
569,58	29,5	46,0	17,8	11,7	16,5	207°	100 cm	V	
583,14	33,6	46,0	18,1	15,5	12,4	236°	100 cm	H	
596,70	29,1	46,0	18,3	10,8	16,9	260°	100 cm	H	
610,32	31,5	46,0	18,5	12,9	14,6	125°	100 cm	H	
637,44	30,0	46,0	18,9	11,1	16,0	-1°	100 cm	H	
714,66	27,7	46,0	19,9	7,8	18,3	343°	100 cm	V	
735,96	28,2	46,0	20,2	8,0	17,8	352°	100 cm	V	
750,00	28,8	46,0	20,4	8,4	17,3	288°	100 cm	H	
778,74	27,3	46,0	20,8	6,6	18,7	303°	100 cm	H	
850,02	27,7	46,0	21,3	6,4	18,3	180°	100 cm	V	
874,98	27,9	46,0	21,5	6,4	18,1	311°	100 cm	V	
949,98	27,9	46,0	22,6	5,3	18,1	141°	100 cm	V	

Picture 11: Radiated emission 30 MHz - 1000MHz @ 3m distance



Spectrum Mask

Test procedure

The EUT was placed in a fully anechoic chamber and the testing was performed in accordance with ANSI C63.4 and 47 CFR Part 15, section 15.225 (a) to (d). The measurement distance was 3 m. To find the closest margin of the spectrum to the limit mask adapted to the test distance the EUT was rotated by 360 degrees with detector of the test receiver set to peak. The loop antenna placed in a fixed height of 1 meter was rotated by 360 degrees to get the maximum of emission. In case of exceeding the limits the detector is switched to quasi peak for final testing in position of maximum emission.




EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

Test result

Temperature:	21°C	Humidity:	45%
Tested by:	Martin Müller	Test date:	2014-09-19

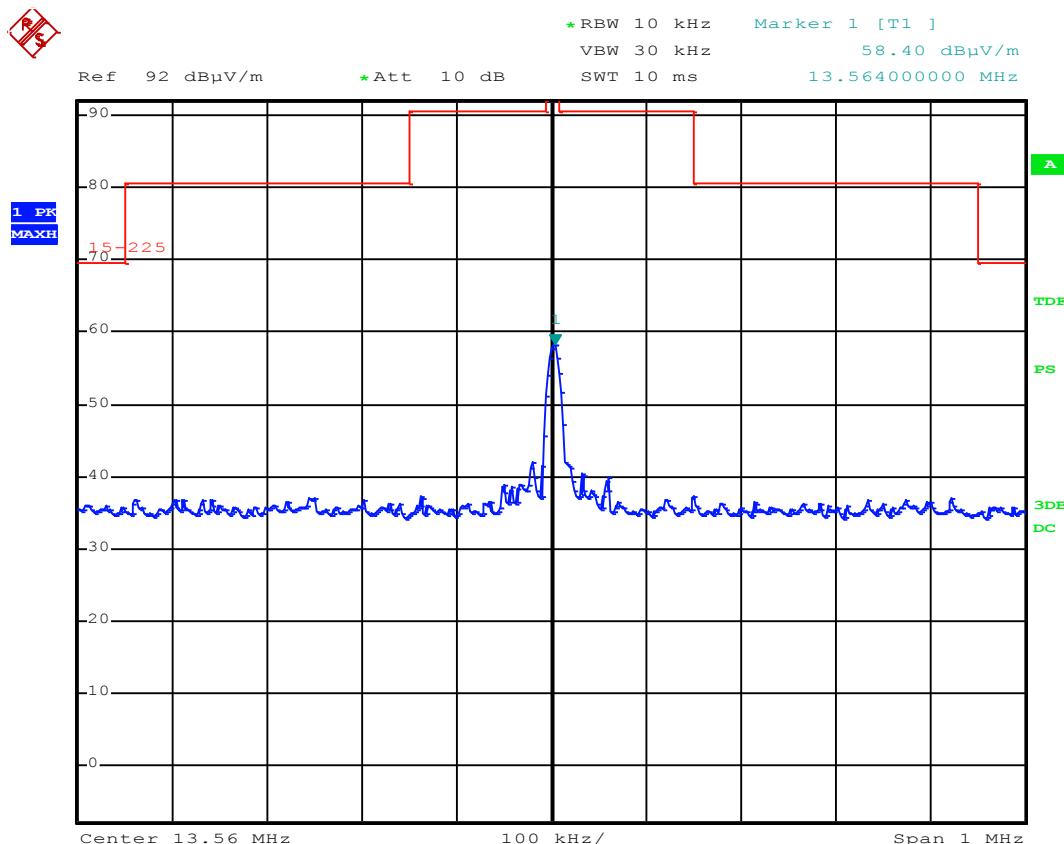

Picture 12: Spectrum mask for 13.56 MHz @ 3m distance

f _{meas} [MHz]	E _{meas} @ 3m [dBµV/m]	Correction 3m -> 30m	Calc. Value [dBµV/m]	Limit @ 30m	Result
13.560	58.40	-40 dB	18.40	84 dBµV/m	Pass

5 Radiated emission measurement (>1 GHz)

according to 47 CFR Part 15, section 15.209(a),
RSS-210, section 2.5 and Annex 2.6 with RSS-Gen, section 7.2.5

Remark:

This measurement needs not to be applied because

- the intentional radiator operates below 10 GHz and tenth harmonic of the highest fundamental frequency is lower than 1 GHz (see 47 CFR Part 15, section 15.33(a)(1), and RSS-Gen, section 4.9), and
- the digital part of the device does not generate or use internal frequencies higher than 108 MHz (see 47 CFR Part 15 section 15.33(b)(1), and RSS-Gen, section 7.1.4 with ICES-003, section 6.2).



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

6 Carrier frequency stability

according to CFR 47 Part 15, section 15.225(e), and
RSS-210, Annex A2.6 with RSS-Gen, section 4.7

6.1 Test Location

Description		Manufacturer	Inventory No.
<input checked="" type="checkbox"/>	Climatic chamber VC 4100	Vötsch Industrietechnik	C00014
<input type="checkbox"/>	Climatic chamber VC ³ 4034	Vötsch Industrietechnik	C00015

6.2 Test instruments

	Description	Manufacturer	Inventory No.
<input type="checkbox"/>	ESU 26	Rohde & Schwarz	W00002
<input checked="" type="checkbox"/>	ESCI 3	Rohde & Schwarz	E00552
<input checked="" type="checkbox"/>	RF-R 400-1	Langer EMV-Technik	E00270

6.3 Limits

The frequency tolerance of the carrier signal shall be maintained within $\pm 0.01\%$ (100 ppm) of the operating frequency over a temperature variation of -20 degrees to +50 degrees C at normal supply voltage, and for a variation in the primary supply voltage from 85% to 115% of the rated supply voltage at a temperature of 20 degrees C.

For battery operated equipment, the equipment tests shall be performed using a new battery. Alternatively, an external supply voltage can be used and set at the battery nominal voltage, and again at the battery operating end point voltage which must be specified by the equipment manufacturer.




EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

6.4 Test procedure

1. If possible EUT is operating providing an unmodulated carrier. The peak detector of the spectrum analyzer is selected and resolution as well as video bandwidth are set to values appropriate to the shape of the spectrum of the EUT. The frequency counter mode of the spectrum analyzer is used to maximize the accuracy of the measured frequency tolerance.
If an unmodulated carrier is not available a significant and stable point on the spectrum is selected and the span is reduced to a value that delivers an accuracy which shall be better than 1% of the maximum frequency tolerance allowed for the carrier signal. This method may be performed as long as the margin to the frequency tolerance allowed is larger than the uncertainty of the measured frequency tolerance.
2. The carrier frequency is measured depending on the variation in the primary supply voltage from 85% to 115% of the rated supply voltage at a temperature of 20 degrees C. For battery operated equipment an external supply voltage can be used and set at the battery nominal voltage, and again at the battery operating end point voltage which must be specified by the equipment manufacturer. Alternatively, tests shall be performed using a new battery.
3. The carrier frequency is measured over a temperature variation of -20 degrees to +50 degrees C at normal supply voltage.

6.5 Test setup

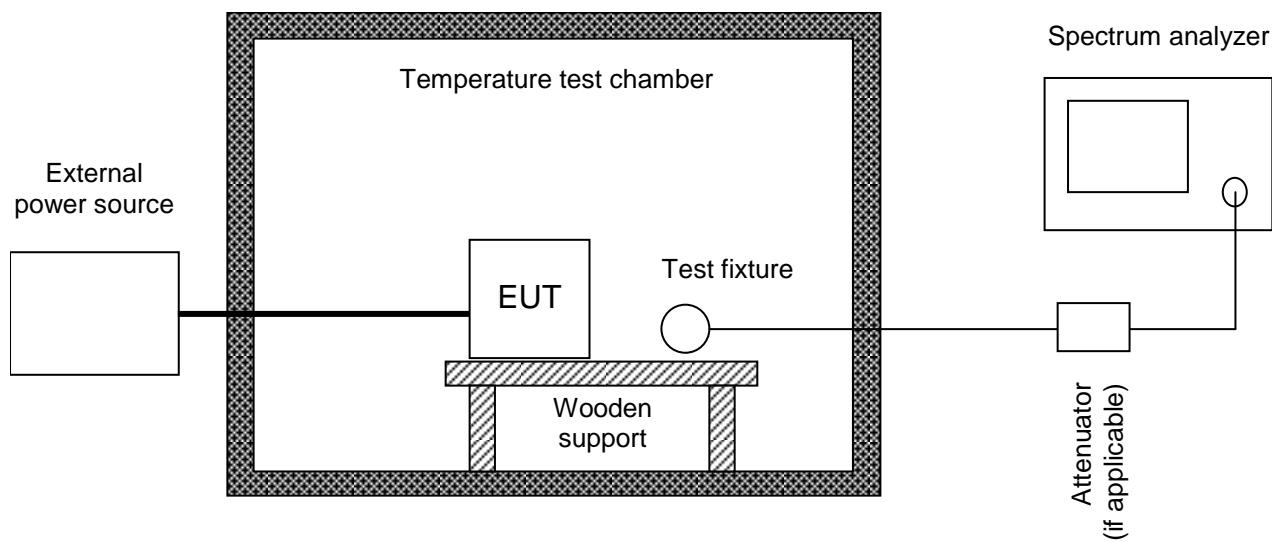

Picture 13: Test setup for carrier frequency stability measurement


6.6 Test deviation

There is no deviation from the standards referred to.

Test result

Temperature:	20°C	Humidity:	41%
Tested by:	Martin Müller	Test date:	2014-10-01

Carrier frequency stability vs. temperature

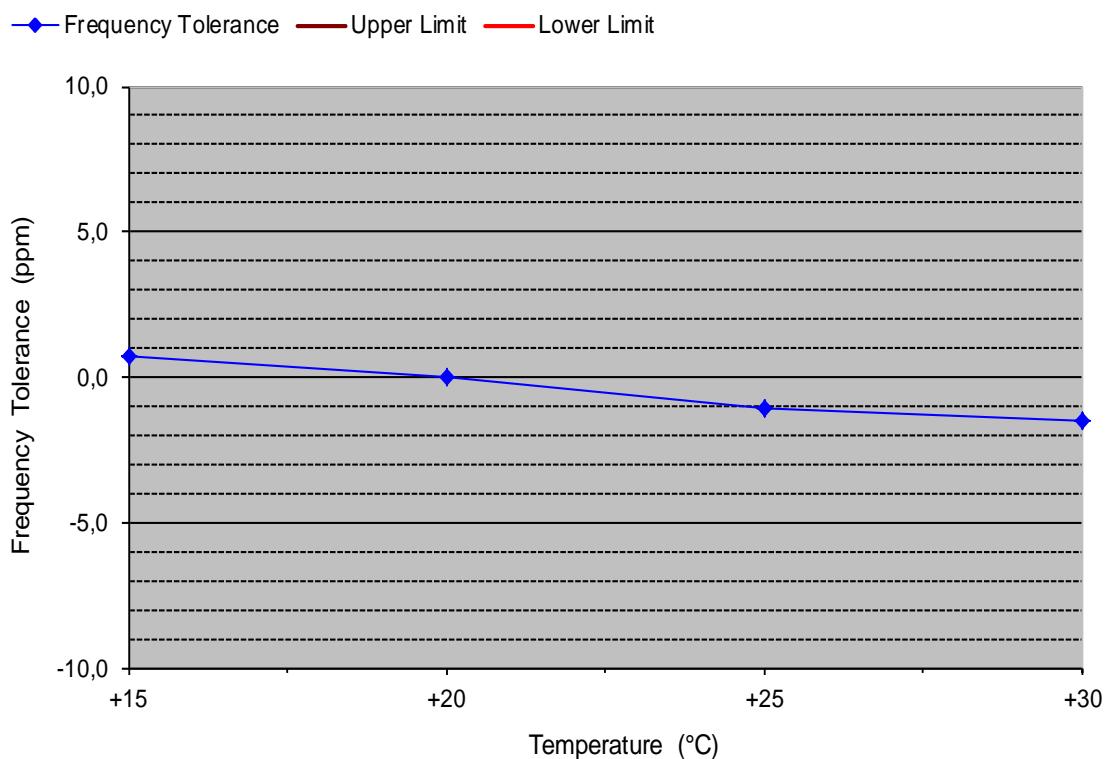

Supply voltage:	6 V	Nominal frequency:	13,562015 MHz
Temperature (°C)	Frequency (MHz)	Frequency Tolerance (Hz)	Upper Limit (ppm)
+15	13,562025	10	0,7
+20	13,562015	0	0,0
+25	13,562000	-15	-1,1
+30	13,561995	-20	-1,5
			Margin (ppm)
			99,3
			100,0
			98,9
			98,5




EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

140561-AU01+W01

Page 32 of 42

Carrier frequency stability vs. supply voltage

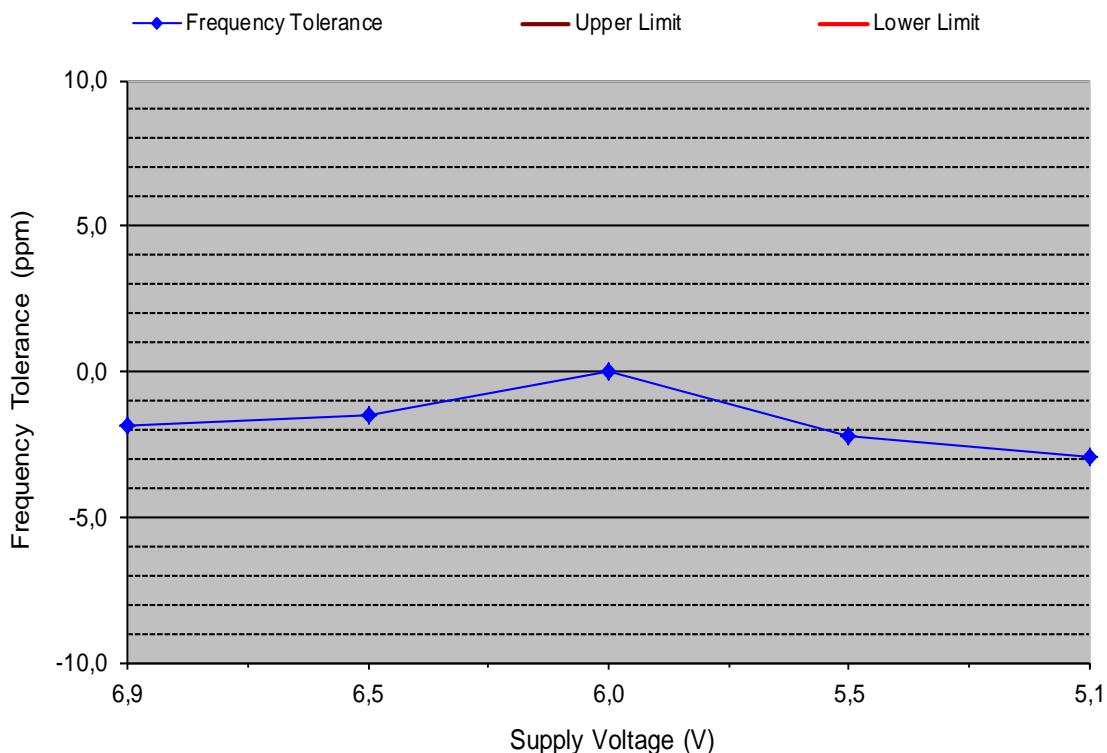

Temperature:	+20 °C	Battery End Point:	Not applicable			
Nominal frequency:	13,562015 MHz					
Supply Voltage (V)	Frequency (MHz)	Frequency Tolerance (Hz)	Frequency Tolerance (ppm)	Upper Limit (ppm)	Lower Limit (ppm)	Margin (ppm)
6,9	13,561990	-25	-1,8	+100,0	-100,0	98,2
6,5	13,561995	-20	-1,5	+100,0	-100,0	98,5
6,0	13,562015	0	0,0	+100,0	-100,0	100,0
5,5	13,561985	-30	-2,2	+100,0	-100,0	97,8
5,1	13,561975	-40	-2,9	+100,0	-100,0	97,1

7 Bandwidths

according to CFR 47 Part 2, section 2.202(a), and RSS-Gen, section 4.6

7.1 Test Location

See clause 4.1 on page 17.

7.2 Test instruments

See clause 4.2 on page 17.

7.3 Limits

The bandwidths are recorded only. There are no limits specified in CFR 47 Part 15, section 15.225, and RSS-210, Annex 2.6

7.4 Test setup

See clause 4.5 on page 20.

7.5 Test deviation

There is no deviation from the standards referred to.



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID

7.6 Test results

Temperature:	21°C	Humidity:	45%
Tested by:	Martin Müller	Test date:	2014-09-19

Occupied bandwidth (99 %)

Test procedure


When an occupied bandwidth value is not specified in the applicable RSS, the transmitted signal bandwidth to be reported is to be its 99% emission bandwidth, as calculated or measured. The transmitter shall be operated at its maximum carrier power measured under normal test conditions.

The span of the analyzer shall be set to capture all products of the modulation process, including the emission skirts. The resolution bandwidth shall be set to as close to 1% of the selected span as is possible without being below 1%. The video bandwidth shall be set to 3 times the resolution bandwidth. Video averaging is not permitted. Where practical, a sampling detector shall be used given that a peak or peak hold may produce a wider bandwidth than actual.

The trace data points are recovered and directly summed in linear terms. The recovered amplitude data points, beginning at the lowest frequency, are placed in a running sum until 0.5% of the total is reached and that frequency recorded. The process is repeated for the highest frequency data points. This frequency is recorded. The span between the two recorded frequencies is the occupied bandwidth. For this purpose the appropriate measurement function of the spectrum analyzer is used.



PS

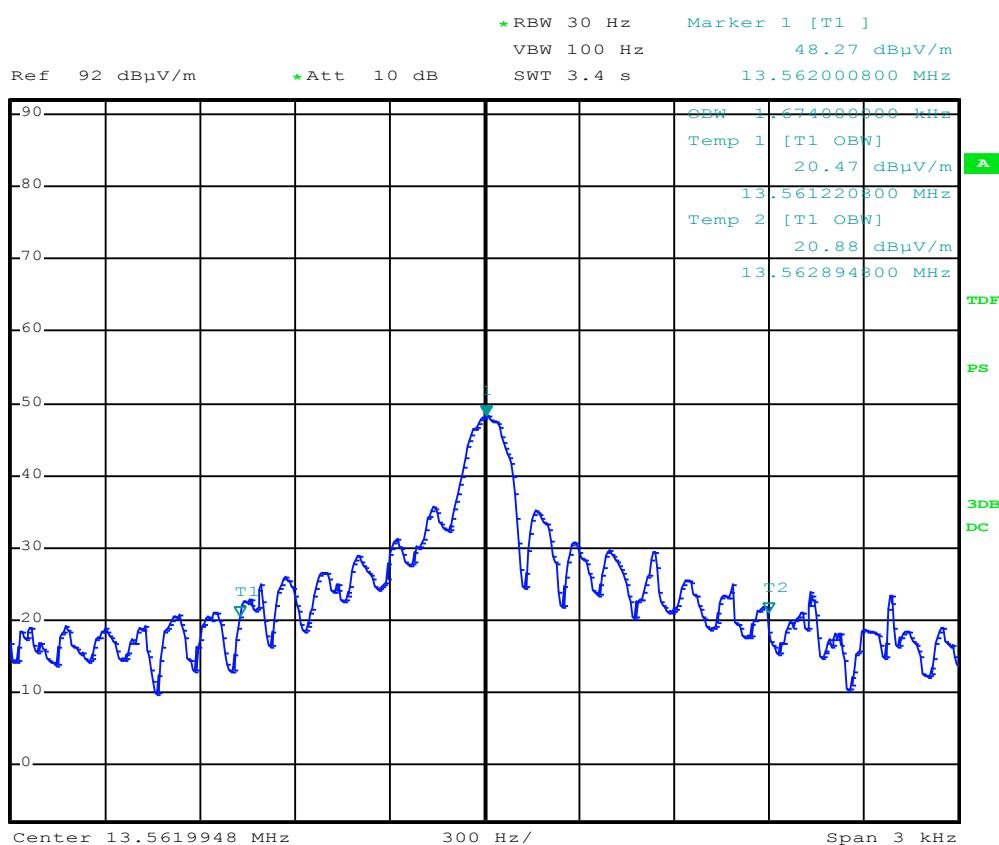


Picture 14: Occupied bandwidth (99 %)

Measured occupied bandwidth (99 %): 1.674 kHz

-6 dB emission bandwidth

Test procedure

Where indicated, the -6 dB emission bandwidth is defined as the frequency range between two points, one above and one below the carrier frequency, at which the spectral density of the emission is attenuated 6 dB below the maximum in-band spectral density of the modulated signal. Spectral density (power per unit bandwidth) is to be measured with a detector of resolution bandwidth equal to approximately 1.0% of the emission bandwidth

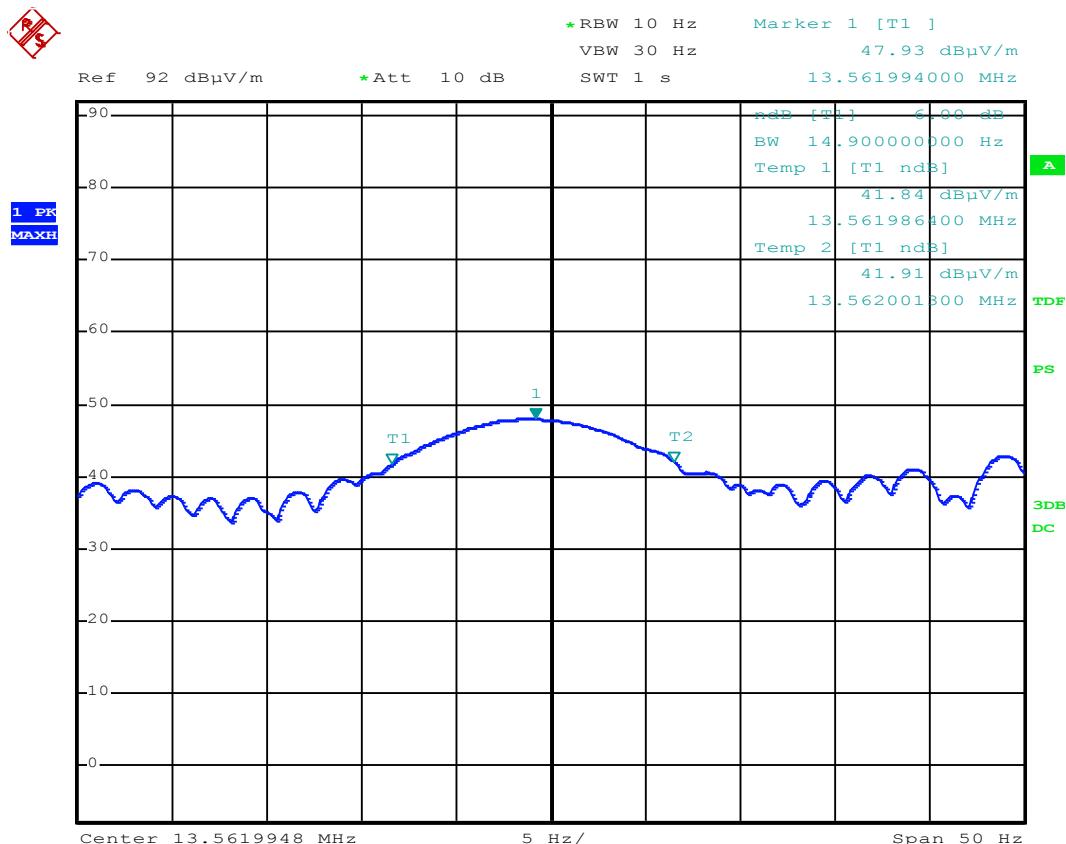


Picture 15: -6 dB emission bandwidth

Measured -6 dB emission bandwidth: 14.90 Hz

-20 dB emission bandwidth

Test procedure

Where indicated, the -20 dB emission bandwidth is defined as the frequency range between two points, one above and one below the carrier frequency, at which the spectral density of the emission is attenuated 20 dB below the maximum in-band spectral density of the modulated signal. Spectral density (power per unit bandwidth) is to be measured with a detector of resolution bandwidth equal to approximately 1.0% of the emission bandwidth.

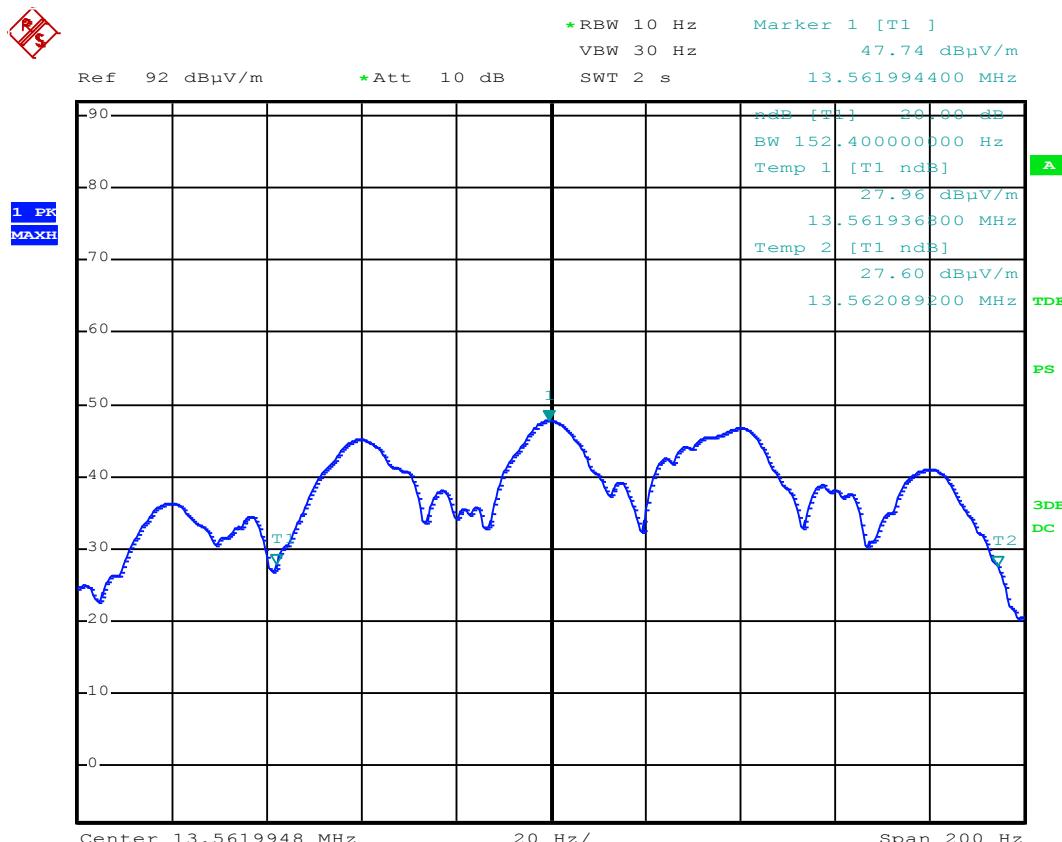

Picture 16: -20 dB emission bandwidth

Measured -20 dB emission bandwidth: 152.40 Hz

8 Equipment calibration status

Description	Modell number	Serial number	Inventory number	Next calibration
Test receiver	ESU 26	100026	W00002	2016-02
Test receiver	ESCI 3	100013	E00001	2015-12
Test receiver	ESCI 3	100328	E00552	2016-07
Test receiver	ESCS 30	825442/0002	E00003	2015-02
Test receiver	ESCS 30	845552/0008	E00551	2015-01
LISN	ESH2-Z5	881362/037	E00004	2015-03
LISN	ESH2-Z5	893406/009	E00005	2016-01
Broadband antenna	VULB 9160	9160-3050	E00011	N/A (only for pretest)
Broadband antenna	VULB 9163	9163-114	E00013	2015-09
Loop antenna	HFH2-Z2	871398/0050	E00004	2016-07
Magnetic field probe	RF-R 400-1	02-1165	E00270	N/A (see note 1)
Shielded room	P92007	B83117C1109T211	E00107	N/A
Compact Diagnostic Chamber (CDC)	VK041.0174	D62128-A502-A69-2-0006	E00026	N/A
Open area test site (OATS)	---	---	E00354	see note 2
Climatic chamber 990 I	VC 4100	59566102680010	C00014	2015-01

Table 1: Equipment calibration status

Note 1: Used for relative measurements only (see test instruments for "Carrier frequency stability", clause 6.2)

Note 2: Expiration date of measurement facility registration by
 - FCC (registration number 221458): 2017-04
 - Industry Canada (test site number 3472A-1): 2015-10

9 Measurement uncertainty

Description	Max. deviation	k=
Conducted emission AMN (9kHz to 30 MHz)	± 3.8 dB	2
Radiated emission open field (3 m) (30 MHz to 300 MHz) (300MHz to 1 GHz)	± 5.4 dB ± 5.9 dB	2
Radiated emission absorber chamber <td>± 4.5 dB</td> <td>2</td>	± 4.5 dB	2

Table 2: Measurement uncertainty

The uncertainty stated is the expanded uncertainty obtained by multiplying the standard uncertainty by the coverage factor k. For a confidence level of 95 % the coverage factor k is 2.

10 Summary

The EMC Regulations according to the marked specifications are

KEPT

The EUT does fulfill the general approval requirements mentioned.


NOT KEPT

The EUT does not fulfill the general approval requirements mentioned.

Place, Date: Straubing, October 7th, 2014



Martin Müller
Test engineer
EMV **TESTHAUS** GmbH

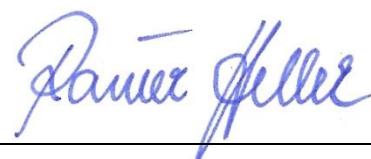

Rainer Heller
Head of EMC / radio department
EMV **TESTHAUS** GmbH

11 Revision History

Date	Description	Person	Revision
2014-10-07	First edition	M. Müller	- - - -

Template used: A_1.0_FCC 15.225_EN_PB



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.0

Esterline | LRE Medical GmbH
Aspect-Reader™
Laboratory Equipment with RFID