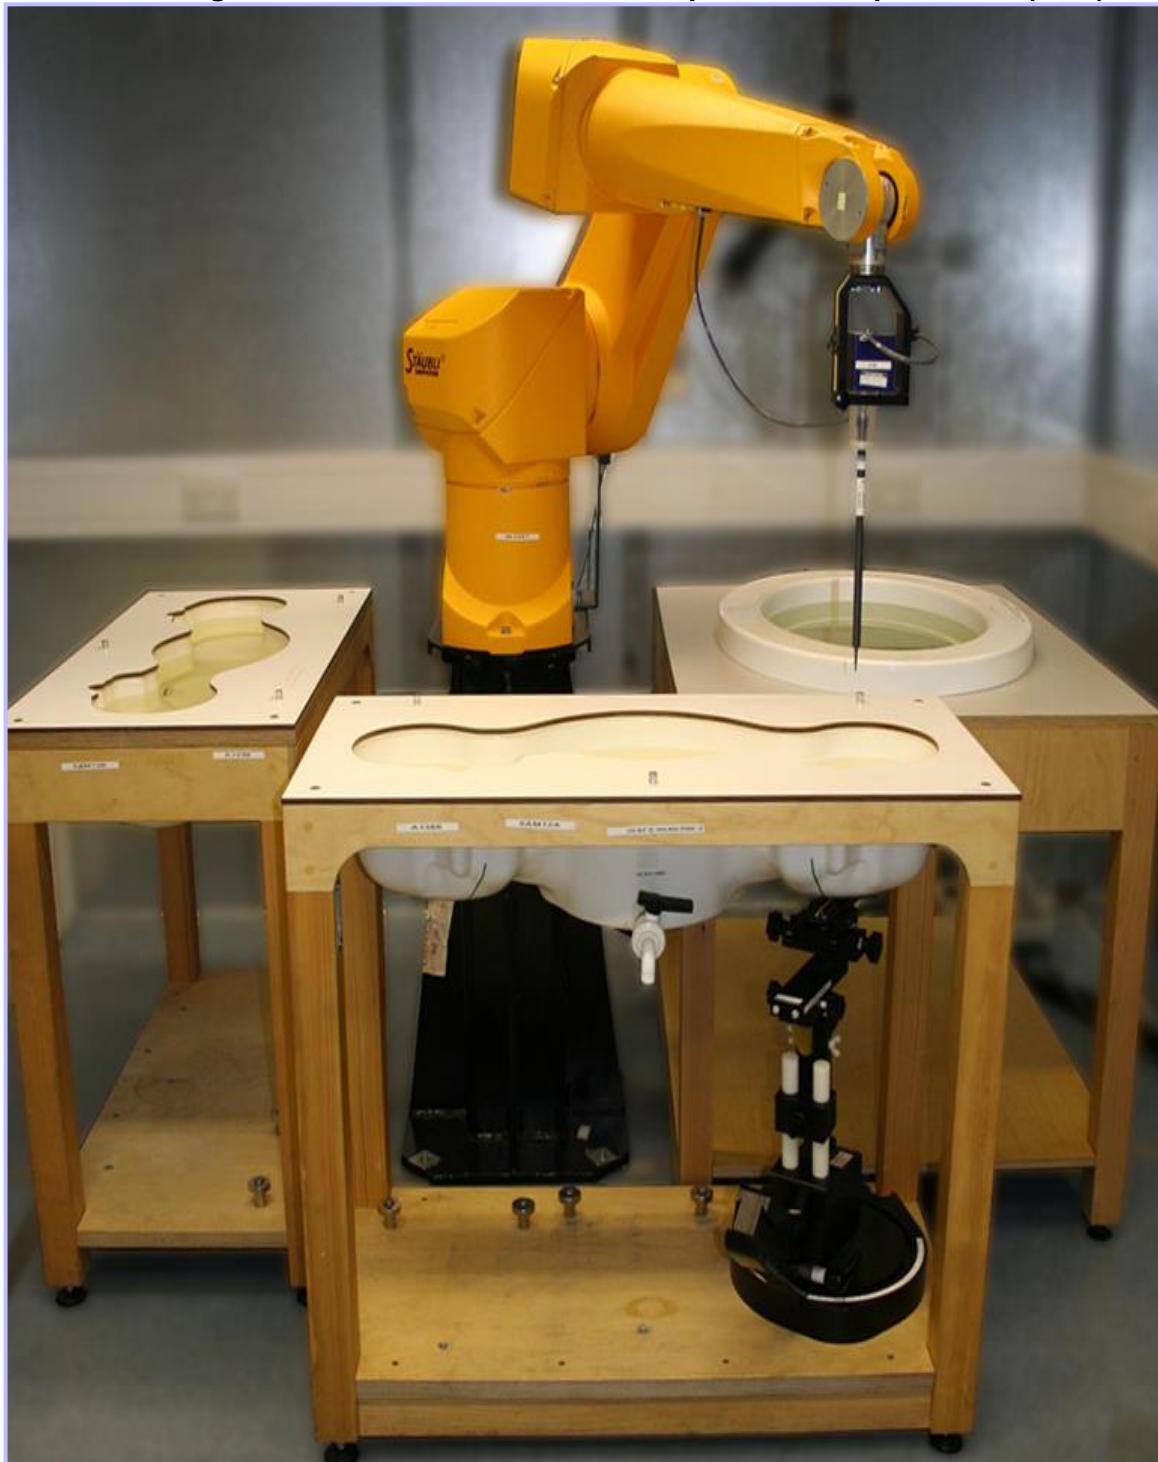


12. Appendixes

12.1. Photos and Ports Location

| Photo Reference Number | Title |
|-------------------------------|---|
| 001 | Test configuration for the measurement of Specific Absorption Rate (SAR) |
| 002 | Touch Left (Host Device) |
| 003 | Touch Right (Host Device) |
| 004 | Front of Host Device Facing Phantom at 10mm Separation |
| 005 | Back of Host Device Facing Phantom at 10mm Separation |
| 006 | Touch Left of Host Device with Sleeve (Linea Pro 5 Case) |
| 007 | Touch Right of Host Device with Sleeve (Linea Pro 5 Case) |
| 008 | Front of Host Device with Sleeve (Linea Pro 5 Case) Facing Phantom at 10mm Separation |
| 009 | Back of Host Device with Sleeve (Linea Pro 5 Case) Facing Phantom at 10mm Separation |
| 010 | Front View of Host Device |
| 011 | Back View of Host Device |
| 012 | Front View of Sleeve (Linea Pro 5 Case) |
| 013 | Back View of Sleeve (Linea Pro 5 Case) |
| 014 | Internal View of Sleeve (Linea Pro 5 Case) |
| 015 | Front View of Host Device + Sleeve (Linea Pro 5 Case) Attached |

001: Test configuration for the measurement of Specific Absorption Rate (SAR)

002: Touch Left (Host Device)

003: Touch Right (Host Device)

004: Front of Host Device Facing Phantom at 10mm Separation



005: Back of Host Device Facing Phantom at 10mm Separation



006: Touch Left of Host Device with Sleeve (Linea Pro 5 Case)

007: Touch Right of Host Device with Sleeve (Linea Pro 5 Case)



008: Front of Host Device with Sleeve (Linea Pro 5 Case) Facing Phantom at 10mm Separation



009: Back of Host Device with Sleeve (Linea Pro 5 Case) Facing Phantom at 10mm Separation



010: Front View of Host Device



011: Back View of Host Device



012: Front View of Sleeve (Linea Pro 5 Case)



013: Back View of Sleeve (Linea Pro 5 Case)



014: Internal View of Sleeve (Linea Pro 5 Case)



Note: The 'Internal View of EUT' photo is supplied by customer.

015: Front View of Host Device + Sleeve (Linea Pro 5 Case) Attached

