ipecs™ LAB

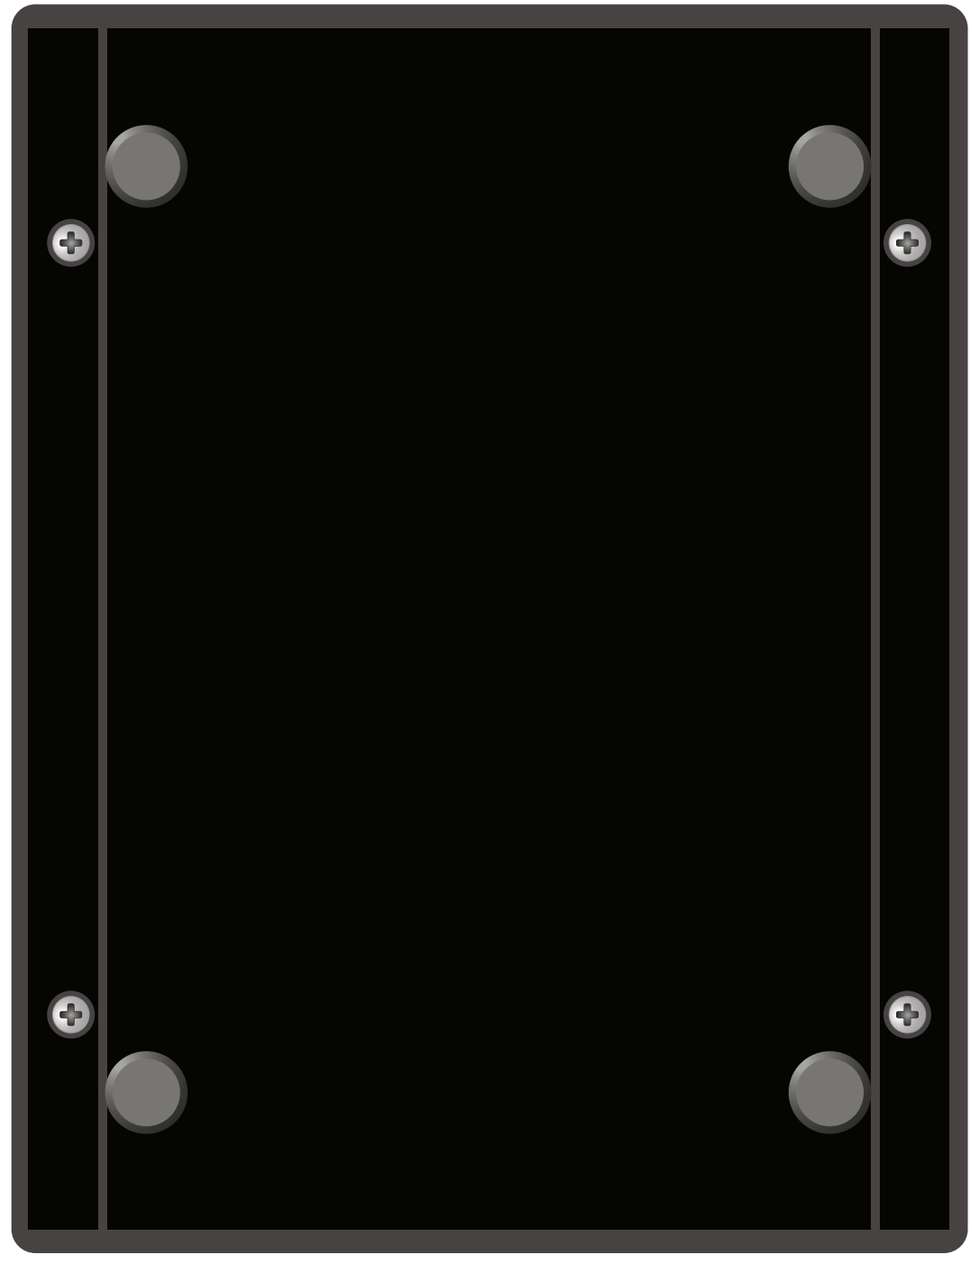

ipecs™ LAB
DCM

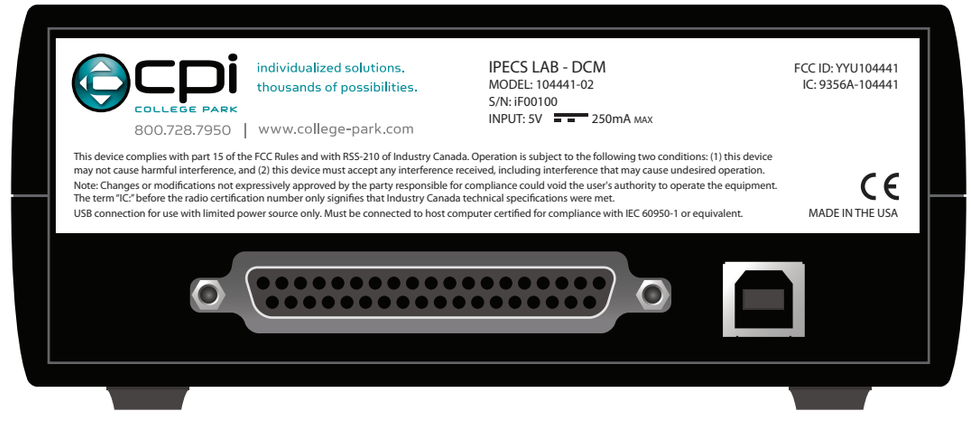
cpi
COLLEGE PARK
individualized solutions.
thousands of possibilities.
800.728.7950 | www.college-park.com
IPECS LAB - DCM
MODEL: 104441-02
S/N: iF00100
INPUT: 5V 250mA MAX
FCC ID: YYU104441
IC: 9356A-104441
This device complies with part 15 of the FCC Rules and with RSS-210 of Industry Canada. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.
Note: Changes or modifications not expressively approved by the party responsible for compliance could void the user's authority to operate the equipment.
The term "IC:" before the radio certification number only signifies that Industry Canada technical specifications were met.
USB connection for use with limited power source only. Must be connected to host computer certified for compliance with IEC 60950-1 or equivalent.
CE
MADE IN THE USA