### **FCC SAR TEST REPORT**

For

**Product Name: Mobile Internet Device** Brand Name: HKC, Pioneer, ODYS, MEDIACOM, EXPER, ZEKI, Xelio, Proscan, KLU, exper, Teach pad, artes, Advance, plaisio, XENO,

> **Smart Touch, GHIA** Model No.: A072G

Series No: A072D,R071A,P07CR,R1,A79,A072D-BK,TBT-7R1-K,M-MP710GO,H7S,H7G,H7D,TBDG773B,Pedi,plus,Opos,A072A,A072B,A072C,A072E,A072F,A072T, R072B, R072C, MV072B, MV072C, MV072D, MV072A, AXXXXX(where X would be any arabian number or letters or blank or symbols) **Test Report Number:** 

> C131009S04-SF-R1 Issued for

HuiKe Electronics (Shenzhen) Co., Ltd. Building 1,2,3, Huike Industrial Park, Minying Industrial Zone, ShuiTian, ShiYan, Bao'an, Shenzhen, China

Issued by

Compliance Certification Services Inc.

**Kun shan Laboratory** 

No.10 Weiye Rd., Innovation park, Eco&Tec, Development Zone, Kunshan City, Jiangsu, China

TEL: 86-512-57355888

FAX: 86-512-57370818



Note: This report shall not be reproduced except in full, without the written approval of Compliance Certification Services Inc. This document may be altered or revised by Compliance Certification Services Inc. personnel only, and shall be noted in the revision section of the document. The client should not use it to claim product endorsement by A2LA or any government agencies. The test results in the report only apply to the tested sample.

Date of Issue :November 1, 2013

# **Revision History**

Revision	REPORT NO.	Date	Page Revised	Contents
Original	C131009S04-SF	October 24, 2013	N/A	N/A
1	C131009S04-SF-R1	November 1, 2013	19	Change the IEEE standards to KDB 865664
1	C131009S04-SF-R1	November 1, 2013	6	Add the chart of the target power value with tolerant
1	C131009S04-SF-R1	November 1, 2013	24	shown the distance of antenna to all edges
1	C131009S04-SF-R1	November 1, 2013	26	Add the repeated SAR testing and Related imformation

### **TABLE OF CONTENTS**

1.	CERTIFICATE OF COMPLIANCE (SAR EVALUATION)	4
2.	EUT DESCRIPTION	5
3.	MAXIMUM RF OUTPUT POWER AMONG PRODUCTION UNITS	6
4.	REQUIREMENTS FOR COMPLIANCE TESTING DEFINED BY THE FCC	6
5.	TEST METHODOLOGY	6
6.	TEST CONFIGURATION	6
7.	DOSIMETRIC ASSESSMENT SETUP	7
	7.1 MEASUREMENT SYSTEM DIAGRAM	8
	7.2 SYSTEM COMPONENTS	9
8.	EVALUATION PROCEDURES	12
9.	MEASUREMENT UNCERTAINTY	16
10.	EXPOSURE LIMIT	17
11.	EUT ARRANGEMENT	18
12.	MEASUREMENT RESULTS	19
	12.1 TEST LIQUIDS CONFIRMATION	19
	12.2 LIQUID MEASUREMENT RESULTS	20
	12.3 SYSTEM PERFORMANCE CHECK	21
	12.4 EUT CONDUCTED POWER	23
	12.5 SAR TEST CONFIGURATIONS	24
	12.6 SAR MEASUREMENT RESULTS	26
	12.7 TEST RECORDS FOR BODY WORN SAR TEST	
	12.8 SAR MULTI XMITER ASSESSMENT	
_	EUT PHOTO	_
14.	EQUIPMENT LIST & CALIBRATION STATUS	31
15.	FACILITIES	32
16.	REFERENCES	32
17.	ATTACHMENTS	33
App	pendix A: Plots of Performance Check	34
App	pendix B: DASY Calibration Certificate	37
A	andiv C. Diata of CAD Toot Beaut	ca

# 1. CERTIFICATE OF COMPLIANCE (SAR EVALUATION)

Product Name:	Mobile Internet Device						
Brand Name:	HKC, Pioneer, ODYS, MEDIACOM,EXPER,ZEKI,Xelio,Proscan, KLU, exper, Teach pad, artes, Advance, plaisio, XENO, Smart Touch, GHIA						
Model Name.:	A072G						
Series No:	A072D,R071A,P07CR,R1,A79,A072D-BK,TBT-7R1-K,M-MP710GO,H7S,H7G,H7D,TBDG773B,Pedi,plus,Opos,A072A,A072B,A072C, A072E,A072F,A072T, R072B, R072C,MV072B, MV072C, MV072D,MV072A, AXXXXX (where X would be any arabian number or letters or blank or symbols)						
Device Category:	pory: PORTABLE DEVICES						
Exposure Category:	GENERAL POPULATION/UNCONTROLLED EXPOSURE						
Date of Test:	October 14, 2013&October 31, 2013						
Applicant:	Building 1,2,3, Huike Industrial Park, Minying Industrial Zone, ShuiTian,						
Applicant:  Manufacturer:							
	Building 1,2,3, Huike Industrial Park, Minying Industrial Zone, ShuiTian, ShiYan, Bao'an, Shenzhen, China  HuiKe Electronics (Shenzhen) Co., Ltd.  Building 1,2,3, Huike Industrial Park, Minying Industrial Zone, ShuiTian,						
Manufacturer: Application Type:	Building 1,2,3, Huike Industrial Park, Minying Industrial Zone, ShuiTian, ShiYan, Bao'an, Shenzhen, China  HuiKe Electronics (Shenzhen) Co., Ltd. Building 1,2,3, Huike Industrial Park, Minying Industrial Zone, ShuiTian, ShiYan, Bao'an, Shenzhen, China						
Manufacturer: Application Type:	Building 1,2,3, Huike Industrial Park, Minying Industrial Zone, ShuiTian, ShiYan, Bao'an, Shenzhen, China  HuiKe Electronics (Shenzhen) Co., Ltd. Building 1,2,3, Huike Industrial Park, Minying Industrial Zone, ShuiTian, ShiYan, Bao'an, Shenzhen, China  Certification						
Manufacturer: Application Type:	Building 1,2,3, Huike Industrial Park, Minying Industrial Zone, ShuiTian, ShiYan, Bao'an, Shenzhen, China  HuiKe Electronics (Shenzhen) Co., Ltd. Building 1,2,3, Huike Industrial Park, Minying Industrial Zone, ShuiTian, ShiYan, Bao'an, Shenzhen, China  Certification  PPLICABLE STANDARDS AND TEST PROCEDURES						
Manufacturer: Application Type:	Building 1,2,3, Huike Industrial Park, Minying Industrial Zone, ShuiTian, ShiYan, Bao'an, Shenzhen, China  HuiKe Electronics (Shenzhen) Co., Ltd. Building 1,2,3, Huike Industrial Park, Minying Industrial Zone, ShuiTian, ShiYan, Bao'an, Shenzhen, China  Certification  PPLICABLE STANDARDS AND TEST PROCEDURES  TEST RESULT						
Manufacturer: Application Type:	Building 1,2,3, Huike Industrial Park, Minying Industrial Zone, ShuiTian, ShiYan, Bao'an, Shenzhen, China  HuiKe Electronics (Shenzhen) Co., Ltd. Building 1,2,3, Huike Industrial Park, Minying Industrial Zone, ShuiTian, ShiYan, Bao'an, Shenzhen, China  Certification  PPLICABLE STANDARDS AND TEST PROCEDURES  TEST RESULT  No non-compliance noted						

The device was tested by Compliance Certification Services Inc. in accordance with the measurement methods and procedures specified in FCC KDB 865664. The test results in this report apply only to the tested sample of the stated device/equipment. Other similar device/equipment will not necessarily produce the same results due to production tolerance and measurement uncertainties.

Approved by:

left fang

Tested by:

Jeff.fang RF Manager

Compliance Certification Services Inc.

Kevin. Hua

Kevin.hua Test Engineer

Compliance Certification Services Inc.

## 2. EUT DESCRIPTION

Product Name:	Mobile Internet Device
Brand Name:	HKC, Pioneer, ODYS, MEDIACOM, EXPER, ZEKI, Xelio, Proscan, KLU, exper, Teach pad, artes, Advance, plaisio, XENO, Smart Touch, GHIA
Model Name.:	A072G
Series No:	A072D,R071A,P07CR,R1,A79,A072D-BK,TBT-7R1-K,M-MP710GO,H7S, H7G,H7D,TBDG773B,Pedi,plus,Opos,A072A,A072B,A072C, A072E, A072F, A072T, R072B, R072C,MV072B, MV072C, MV072D,MV072A, AXXXXX (where X would be any arabian number or letters or blank or symbols)
Model Discrepancy:	Only for market segment
FCC ID:	ZFN-A072D
Device Category:	Production unit
Frequency Range:	WLAN 2.4GHz: 2412 ~ 2462 MHz
Max. Transmit Power: (Conducted average power)	802.11b:14.83 dBm 802.11g:11.62 dBm 802.11 20n HT20:10.86 dBm 802.11 40n HT40:10.47 dBm
Max.Reported SAR(1g):	Body: 802.11b: 0.966 W/kg
Modulation Technique:	802.11b: DSSS (CCK, DQPSK, DBPSK) 802.11g: DSSS (CCK, DQPSK,DBPSK)+OFDM (QPSK, BPSK, 16-QAM, 64-QAM) IEEE 802.11n: OFDM(MCS 0-7)
Accessories:	Power supply and ADP(rating): Model No.:JY-05200 Input:: 100-240V,50-60Hz,0.3A Ouput: 5V 2.0A Brand : Mcnair Model: MLP386997 Capacitance: 3500mAh
Antenna Specification:	WLAN: Fixed Internal Antenna
Operating Mode:	Maximum continuous output

## 3. MAXIMUM RF OUTPUT POWER AMONG PRODUCTION UNITS

Mode	The Turn-up Maximum Power(Customer Declared)(dBm)	Range	Measured Conduct Maximum Power(dBm)
IEEE 802.11b	14+/-1	13-15	14.83
IEEE 802.11g	11+/-1	10-12	11.62
IEEE 802.11n(20M) 2.4G	10+/-1	9-11	10.86
IEEE 802.11n(40M) 2.4G	10+/-1	9-11	10.47

## 4. REQUIREMENTS FOR COMPLIANCE TESTING DEFINED BY THE FCC

The US Federal Communications Commission has released the report and order "Guidelines for Evaluating the Environmental Effects of RF Radiation", ET Docket No. 93-62 in August 1996. The order requires routine SAR evaluation prior to equipment authorization of portable transmitter devices, including portable telephones. For consumer products, the applicable limit is 1.6 mW/g for an uncontrolled environment and 8.0 mW/g for an occupational/controlled environment as recommended by the ANSI/IEEE standard C95.1-1999. According to the FCC KDB 865664, the device should be evaluated at maximum output power (radiated from the antenna) under "worstcase" conditions for normal or intended use, incorporating normal antenna operating positions, device peak performance frequencies and positions for maximum RF energy coupling.

## 5. TEST METHODOLOGY

The Specific Absorption Rate (SAR) testing specification, method and procedure for this Mobile Phone is in accordance with the following standards:

□ IEEE C95.1-1999

☐ IEEE 1528-2003

☑ KDB 248227 D01v01r02 SAR Measurement Procedures for 802.11 a/b/g Transmitters

Mobile and Portable Device RF Exposure Procedures and Equipment

**Authorization Polices** 

X KDB 616217 D04v01r01 SAR Evaluation Considerations for Laptop, Notebook, Netbook and

**Tablet Computers** 

KDB 865664 D01v01r01 SAR Measurement Requirements for 100 MHz to 6 GHz

### 6. TEST CONFIGURATION

During WLAN SAR testing EUT is configured with the WLAN continuous TX tool, and the transmission duty factor was monitored on the spectrum analyzer with zero-span setting

For WLAN SAR testing, WLAN engineering test software installed on the EUT can provide continuous transmitting RF signal.

Date of Issue :November 1, 2013


## 7. DOSIMETRIC ASSESSMENT SETUP

These measurements were performed with the automated near-field scanning system DASY 5 from ATTENNESSA. The system is based on a high precision robot (working range greater than 0.9 m), which positions the probes with a positional repeatability of better than ± 0.02 mm. Special E- and H-field probes have been developed for measurements close to material discontinuity, the sensors of which are directly loaded with a Schottky diode and connected via highly resistive lines to the data acquisition unit. The SAR measurements were conducted with the E-field PROBE EX3DV4 (manufactured by SPEAG), designed in the classical triangular configuration and optimized for dosimetric evaluation. The probe has been calibrated according to the procedure described in [7] with accuracy of better than ±10%. The spherical isotropy was evaluated with the procedure described in [8] and found to be better than ±0.25 dB. The phantom used was the SAM Twin Phantom as described in FCC supplement C, IEE P1528 and CENELEC EN 62209.

The Tissue simulation liquid used for each test is listed below.

Ingredients	Frequency (MHz)										
(% by weight)	450		835		915		1900		2450		
Tissue Type	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body	
Water	38.56	51.16	41.45	52.4	41.05	56.0	54.9	40.4	62.7	73.2	
Salt (NaCl)	3.95	1.49	1.45	1.4	1.35	0.76	0.18	0.5	0.5	0.04	
Sugar	56.32	46.78	56.0	45.0	56.5	41.76	0.0	58.0	0.0	0.0	
HEC	0.98	0.52	1.0	1.0	1.0	1.21	0.0	1.0	0.0	0.0	
Bactericide	0.19	0.05	0.1	0.1	0.1	0.27	0.0	0.1	0.0	0.0	
Triton X-100	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	36.8	0.0	
DGBE	0.0	0.0	0.0	0.0	0.0	0.0	44.92	0.0	0.0	26.7	
Dielectric Constant	43.42	58.0	42.54	56.1	42.0	56.8	39.9	54.0	39.8	52.5	
Conductivity (S/m)	0.85	0.83	0.91	0.95	1.0	1.07	1.42	1.45	1.88	1.78	

### 7.1 MEASUREMENT SYSTEM DIAGRAM

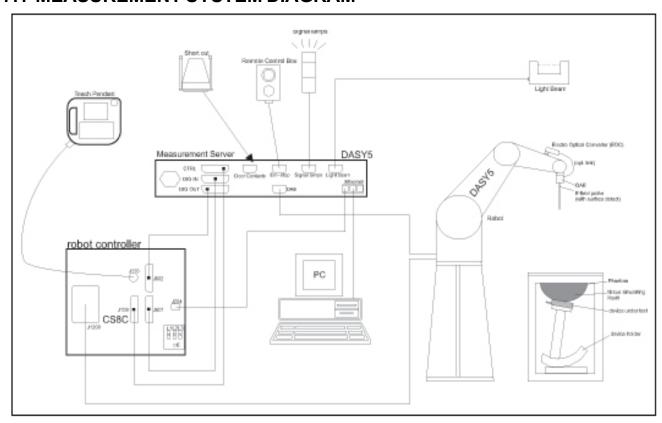

### The DASY5 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (St"aubli RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion between optical and electrical of the signals for the digital communication to the DAE and for the analog signal from the optical surface detection. The EOC is connected to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
- A computer operating Windows 7.
- DASY5 software.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The SAM twin phantom enabling testing left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- Tissue simulating liquid mixed according to the given recipes.
- Validation dipole kits allowing validating the proper functioning of the system.

### 7.2 SYSTEM COMPONENTS



The DASY5 measurement server is based on a PC/104 CPU board with a 400MHz intel ULV celeron, 128MB chip-disk and 128 MB RAM. The necessary circuits for communication with either the DAE4(or DAE3) electronic box as well as the 16-bit AD-converter system for optical detection and digital I/O interface are contained on the DASY5 I/O-board, which is directly connected to the PC/104 bus of the CPU board.

The measurement server performs all real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operation.



The PC-operating system cannot interfere with these time critical processes. All connections are supervised by a watchdog, and disconnection of any of the cables to the measurement server will automatically disarm the robot and disable all program-controlled robot movements. Furthermore, the measurement server is equipped with two expansion slots which are reserved for future applications. Please note that the expansion slots do not have a standardized pinout and therefore only the expansion cards provided by SPEAG can be inserted. Expansion cards from any other supplier could seriously damage the measurement server. Calibration: No calibration required.

### **Data Acquisition Electronics (DAE)**



The data acquisition electronics (DAE4) consists of a highly sensitive electrometer grade preamplifier with auto-zeroing, a channel and gainswitching multiplexer, a fast 16 bit AD converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock. The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection. The input impedance of the DAE4 box is 200MOhm; the inputs are symmetrical and floating. Common mode rejection is above 80 dB.

### EX3DV4 Isotropic E-Field Probe for Dosimetric Measurements



Construction: Symmetrical design with triangular core

Built-in shielding against static charges

PEEK enclosure material (resistant to organic solvents,

e.g., DGBE)

**Calibration:** Basic Broad Band Calibration in air: 10-3000 MHz.

Conversion Factors (CF) for HSL 900 and HSL 1800 CF-Calibration for other liquids and frequencies upon

request.

Frequency: 10 MHz to > 6 GHz; Linearity: ± 0.2 dB (30 MHz to 3

GHz)

**Directivity:** ± 0.3 dB in HSL (rotation around probe axis)

± 0.5 dB in HSL (rotation normal to probe axis)

**Dynamic Range:** 10 μW/g to > 100 mW/g; Linearity: ± 0.2 dB

(noise: typically  $< 1 \mu W/g$ )

Report No: C131009S04-SF-R1 FCCID: ZFN-A072D

Date of Issue : November 1, 2013

**Dimensions:** Overall length: 337 mm (Tip: 9 mm)

Tip diameter: 2.5 mm (Body: 10 mm) Distance from probe tip to dipole centers:

Application: High precision dosimetric measurements

in any exposure scenario (e.g., very strong gradient fields). Only probe which enables compliance testing for frequencies up to 6

GHz with precision of better 30%.




Interior of probe

### SAM Twin Phantom

### Construction:

The shell corresponds to the specifications of the Specific Anthropomorphic Mannequin (SAM) phantom defined in IEEE 1528-200X, CENELEC 50360 and IEC 62209. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents evaporation of the liquid. Reference markings on the phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points with the robot.



Height: 850mm; Length: 1000mm; Width: Dimensions:

750mm

## SAM Phantom (ELI4 v4.0)

### **Description Construction:**

Phantom for compliance testing of handheld and body-mounted wireless devices in the frequency range of 30 MHz to 6 GHz. ELI4 is fully compatible with the latest draft of the standard IEC 62209 Part II and all known tissue simulating liquids. ELI4 has been optimized regarding its performance and can be integrated into our standard phantom tables. A cover prevents evaporation of the liquid. Reference markings on the phantom allow installation of the complete setup, including all predefined phantom positions and measurement grids, by teaching three points. The phantom is supported by software version DASY4/DASY5.5 and higher and is compatible with all SPEAG dosimetric probes and dipoles

Shell Thickness:  $2.0 \pm 0.2 \text{ mm (sagging: <1\%)}$ 

Filling Volume: Approx. 25 liters

Dimensions: Major ellipse axis: 600 mm

Minor axis: 400 mm 500mm



FCCID: ZFN-A072D

Date of Issue :November 1, 2013

### Device Holder for SAM Twin Phantom

**Construction:** In combination with the Twin SAM Phantom, the Mounting Device (made from POM) enables the rotation of the mounted transmitter in spherical coordinates, whereby the rotation point is the ear opening. The devices can be easily and accurately positioned according to IEC, IEEE, CENELEC, FCC or other specifications. The device holder can be locked at different phantom locations (left head, right head, and flat phantom).



### System Validation Kits for SAM Twin Phantom

Construction: Symmetrical dipole with I/4 balun Enables

measurement of feedpoint impedance with NWA Matched for use near flat phantoms filled with brain simulating solutions Includes distance

holder and tripod adaptor.

Frequency: 900,1800,2450,5800 MHz

Return loss: > 20 dB at specified validation position **Power capability:** > 100 W (f < 1GHz); > 40 W (f > 1GHz)

Dimensions:

D835V2: dipole length: 161 mm; overall height: 340 mm D1800V2: dipole length: 72.5 mm; overall height: 300 mm D1900V2: dipole length: 67.7 mm; overall height: 300 mm D2450V2: dipole length: 51.5 mm; overall height: 290 mm D5GHzV2: dipole length: 20.6 mm; overall height: 300mm



### System Validation Kits for ELI4 phantom

Construction: Symmetrical dipole with I/4 balun Enables

> measurement of feedpoint impedance with NWA Matched for use near flat phantoms filled with brain simulating solutions Includes distance

holder and tripod adaptor.

Frequency: 900, 1800, 2450, 5800 MHz

Return loss: > 20 dB at specified validation position **Power capability:** > 100 W (f < 1GHz); > 40 W (f > 1GHz)

Dimensions:

D835V2: dipole length: 161 mm; overall height: 340 mm D1800V2: dipole length: 72.5 mm; overall height: 300 mm D1900V2: dipole length: 67.7 mm; overall height: 300 mm D2450V2: dipole length: 51.5 mm; overall height: 290 mm D5GHzV2: dipole length: 20.6 mm; overall height: 300 mm



## 8. EVALUATION PROCEDURES

### **DATA EVALUATION**

The DASY 5 post processing software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters: - Sensitivity Norm<sub>i</sub>, a<sub>i0</sub>, a<sub>i1</sub>, a<sub>i2</sub>

> - Conversion factor ConvF<sub>i</sub> - Diode compression point dcpi

Device parameters: - Frequency - Crest factor cf

Media parameters: - Conductivity σ

- Density

These parameters must be set correctly in the software. They can be found in the component documents or be imported into the software from the configuration files issued for the DASY 5 components. In the direct measuring mode of the multi-meter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

= Compensated signal of channel i(i = x, y, z)

= Input signal of channel i (i = x, y, z)

= Crest factor of exciting field (DASY 5 particular point) (DASY 5 particular point) (DASY 5 parameter) dcp<sub>i</sub> = Diode compression point (DASY 5 parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes:

$$E_{i} = \sqrt{\frac{V_{i}}{Norm_{i} \cdot ConvF}}$$

H-field probes:

$$H_i = \sqrt{Vi} \cdot \frac{a_{i10} + a_{i11}f + a_{i12}f^2}{f}$$

= Compensated signal of channel i(i = x, y, z)

 $Norm_i$  = Sensor sensitivity of channel i (i = x, y, z)

 $\mu V/(V/m)^2$  for E0field Probes

ConvF = Sensitivity enhancement in solution

= Sensor sensitivity factors for H-field probes aii

f = Carrier frequency (GHz)

Εi = Electric field strength of channel i in V/m

Hi = Magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with SAR = local specific absorption rate in mW/g

 $E_{tot}$  = total field strength in V/m

= conductivity in [mho/m] or [Siemens/m]

= equivalent tissue density in g/cm<sup>3</sup>

Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid.

The power flow density is calculated assuming the excitation field as a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770}$$
 or  $P_{pwe} = H_{tot}^2 \cdot 37.7$ 

with  $P_{pwe}$  = Equivalent power density of a plane wave in mW/cm<sup>2</sup>

 $E_{tot}$  = total electric field strength in V/m

= total magnetic field strength in A/m  $H_{tot}$ 

FCCID: ZFN-A072D

### **SAR EVALUATION PROCEDURES**

The procedure for assessing the peak spatial-average SAR value consists of the following steps:

### **Power Reference Measurement**

The reference and drift jobs are useful jobs for monitoring the power drift of the device under test in the batch process. Both jobs measure the field at a specified reference position, at a selectable distance from the phantom surface. The reference position can be either the selected section's grid reference point or a user point in this section. The reference job projects the selected point onto the phantom surface, orients the probe perpendicularly to the surface, and approaches the surface using the selected detection method.

### Area Scan

The area scan is used as a fast scan in two dimensions to find the area of high field values, before doing a finer measurement around the hot spot. The sophisticated interpolation routines implemented in DASY 5 software can find the maximum locations even in relatively coarse grids. The scan area is defined by an editable grid. This grid is anchored at the grid reference point of the selected section in the phantom. When the area scan's property sheet is brought-up, grid was at to 15 mm by 15 mm and can be edited by a user.

### **Zoom Scan**

Zoom scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The default zoom scan measures 5 x 5 x 7 points within a cube whose base faces are centered around the maximum found in a preceding area scan job within the same procedure. If the preceding Area Scan job indicates more then one maximum, the number of Zoom Scans has to be enlarged accordingly (The default number inserted is 1).

### **Power Drift measurement**

The drift job measures the field at the same location as the most recent reference job within the same procedure, and with the same settings. The drift measurement gives the field difference in dB from the reading conducted within the last reference measurement. Several drift measurements are possible for one reference measurement. This allows a user to monitor the power drift of the device under test within a batch process. In the properties of the Drift job, the user can specify a limit for the drift and have DASY 5 software stop the measurements if this limit is exceeded.

The Z Scan job measures points along a vertical straight line. The line runs along the Z-axis of a one-dimensional grid. A user can anchor the grid to the current probe location. As with any other grids, the local Z-axis of the anchor location establishes the Z-axis of the grid.

FCCID: ZFN-A072D

### **SPATIAL PEAK SAR EVALUATION**

The procedure for spatial peak SAR evaluation has been implemented according to the IEEE1529 standard. It can be conducted for 1 g and 10 g.

The DASY 5 system allows evaluations that combine measured data and robot positions, such as:

- · maximum search
- extrapolation
- · boundary correction
- · peak search for averaged SAR

During a maximum search, global and local maximum searches are automatically performed in 2-D after each Area Scan measurement with at least 6 measurement points. It is based on the evaluation of the local SAR gradient calculated by the Quadratic Shepard's method. The algorithm will find the global maximum and all local maxima within -2 dB of the global maxima for all SAR distributions.

### **Extrapolation**

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. Several measurements at different distances are necessary for the extrapolation.

Extrapolation routines require at least 10 measurement points in 3-D space. They are used in the Cube Scan to obtain SAR values between the lowest measurement points and the inner phantom surface. The routine uses the modified Quadratic Shepard's method for extrapolation. For a grid using 5x5x7 measurement points with 5mm resolution amounting to 343 measurement points, the uncertainty of the extrapolation routines is less than 1% for 1 g and 10 g cubes.

### **Boundary effect**

For measurements in the immediate vicinity of a phantom surface, the field coupling effects between the probe and the boundary influence the probe characteristics. Boundary effect errors of different dosimetric probe types have been analyzed by measurements and using a numerical probe model. As expected, both methods showed an enhanced sensitivity in the immediate vicinity of the boundary. The effect strongly depends on the probe dimensions and disappears with increasing distance from the boundary. The sensitivity can be approximately given as:

$$S \approx S_o + S_b exp(-\frac{z}{a})cos(\pi \frac{z}{\lambda})$$

Since the decay of the boundary effect dominates for small probes (a $<<\lambda$ ), the cos-term can be omitted. Factors Sb (parameter Alpha in the DASY 5 software) and a (parameter Delta in the DASY 5 software) are assessed during probe calibration and used for numerical compensation of the boundary effect. Several simulations and measurements have confirmed that the compensation is valid for different field and boundary configurations.

This simple compensation procedure can largely reduce the probe uncertainty near boundaries. It works well as long as:

- the boundary curvature is small
- the probe axis is angled less than 30 to the boundary normal
- the distance between probe and boundary is larger than 25% of the probe diameter
- the probe is symmetric (all sensors have the same offset from the probe tip)

Since all of these requirements are fulfilled in a DASY 5 system, the correction of the probe boundary effect in the vicinity of the phantom surface is performed in a fully automated manner via the measurement data extraction during post processing.

## 9. MEASUREMENT UNCERTAINTY

UNCERTAINTY BUDGE ACCORDING TO IEEE 1528-2003									
Error Description	Uncertainty Value ±%	Probability distribution	Divisor	C₁1g	Standard unc.(1g) ±%	V <sub>1</sub> or V <sub>eff</sub>			
Measurement System	2 0000 = 70				(- <b>3</b> ) = /-				
Probe calibration	±5.5	normal	1	1	±5.5	∞			
Axial isotropy of probe	±4.7	rectangular	√3	0.7	±1.9	∞			
Hemispherical Isotropy of probe	±9.6	rectangular	√3	0.7	±3.9	∞			
Probe linearity	±4.7	rectangular	√3	1	±2.7	∞			
Detection Limit	±1.0	rectangular	√3	1	±0.6	∞			
Boundary effects	±1.0	rectangular	√3	1	±0.6	∞			
Readout electronics	±0.3	normal	1	1	±0.3	∞			
Response time	±0.8	rectangular	√3	1	±0.5	∞			
Integration time	±2.6	rectangular	√3	1	±1.5	∞			
Probe positioning	±2.9	rectangular	√3	1	±1.7	∞			
Probe positioner	±0.4	rectangular	√3	1	±0.2	∞			
RF ambient Noise	±3.0	rectangular	√3	1	±1.7	∞			
RF ambient Reflections	±3.0	rectangular	√3	1	±1.7	∞			
Max.SAR Eval	±1.0	rectangular	√3	1	±0.6	∞			
Test Sample Related									
Device positioning	±2.9	normal	1	1	±2.9	145			
Device holder uncertainty	±3.6	normal	1	1	±3.6	5			
Power drift	±5.0	rectangular	√3	1	±2.9	∞			
Phantom and Set up									
Phantom uncertainty	±4.0	rectangular	√3	1	±2.3	∞			
Liquid conductivity(target)	±5.0	rectangular	√3	0.64	±1.8	∞			
Liquid conductivity(meas.)	±2.5	rectangular	1	0.64	±1.6	∞			
Liquid permittivity(target)	±5.0	rectangular	√3	0.6	±1.7	∞			
Liquid permittivity(meas.)	±2.5	rectangular	1	0.6	±1.5	∞			
Combined Standard Uncertainty	,				±10.7	387			
Coverage Factor for 95%		kp=2							
Expanded Standard Uncertainty					±21.4				

Table: Worst-case uncertainty for DASY5 assessed according to IEEE1528-2003.

The budge is valid for the frequency range 300 MHz to 6G Hz and represents a worst-case analysis.

Report No: C131009S04-SF-R1

Date of Issue :November 1, 2013

### **EXPOSURE LIMIT 10**.

(A). Limits for Occupational/Controlled Exposure (W/kg)

Whole-Body	Partial-Body	Hands, Wrists, Feet and Ankles
0.4	8.0	20.0

(B). Limits for General Population/Uncontrolled Exposure (W/kg)

Whole-Body	Partial-Body	Hands, Wrists, Feet and Ankles
0.08	1.6	4.0

Note: Whole-Body SAR is averaged over the entire body, partial-body SAR is averaged over any 10 gram of tissue defined as a tissue volume in the shape of a cube. SAR for hands, wrists, feet and ankles is averaged over any 1 grams of tissue defined as a tissue volume in the shape of a cube.

Population/Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure.

Occupational/Controlled Environments are defined as locations where there is exposure that may be incurred by people who are aware of the potential for exposure, (i.e. as a result of employment or occupation).

> **NOTE** GENERAL POPULATION/UNCONTROLLED EXPOSURE **PARTIAL BODY LIMIT** 1.6 W/kg

## **EUT ARRANGEMENT**

This EUT was tested in two different positions. They are rear side of tablet and Edge 3.In these positions, the surface of EUT is touching with phantom 0cm.

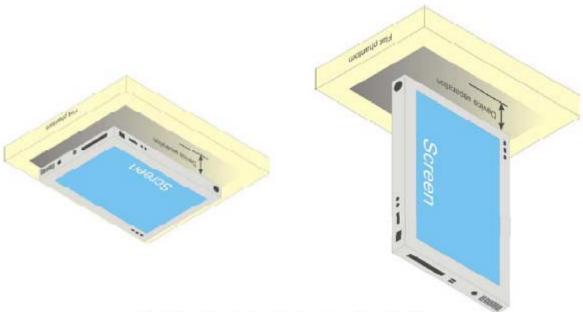


Fig 8.1 Illustration for Lap-touching Position

### **12**. **MEASUREMENT RESULTS**

### 12.1 **TEST LIQUIDS CONFIRMATION**

### SIMULATED TISSUE LIQUID PARAMETER CONFIRMATION

The dielectric parameters were checked prior to assessment using the HP85070C dielectric probe kit. The dielectric parameters measured are reported in each correspondent section.

### KDB865664 RECOMMENDED TISSUE DIELECTRIC PARAMETERS

The tissue dielectric parameters recommended by the KDB865664 have been incorporated in the following table

Target Frequency	He	ad	Body		
(MHz)	ε <sub>r</sub>	σ (S/m)	ε <sub>r</sub>	σ (S/m)	
150	52.3	0.76	61.9	0.80	
300	45.3	0.87	58.2	0.92	
450	43.5	0.87	56.7	0.94	
835	41.5	0.90	55.2	0.97	
900	41.5	0.97	55.0	1.05	
915	41.5	0.98	55.0	1.06	
1450	40.5	1.20	54.0	1.30	
1610	40.3	1.29	53.8	1.40	
1800-2000	40.0	1.40	53.3	1.52	
2450	39.2	1.80	52.7	1.95	
3000	38.5	2.40	52.0	2.73	
5800	35.3	5.27	48.2	6.00	

(ε<sub>r</sub> = relative permittivity, σ = conductivity and ρ = 1000 kg/m<sup>3</sup>)

### 12.2 LIQUID MEASUREMENT RESULTS

The following table give the recipes for tissue simulating liquid:

### For Head:

Ī	Frequency		Sugar					Conductivity	Permittivity
	(MHz)	(%)	(%)	(%)	(%)	(%)	(%)	( <del>o</del> )	$(\varepsilon_{\rm r})$
	2450	55.00	0	0	0	0	45.00	1.80	39.20

### For Body:

Frequency (MHz)	Water (%)	Sugar (%)	Salt (%)	Cellulose (%)	Preventol (%)	DGBE (%)	Conductivity (σ)	Permittivity $(\epsilon_r)$
2450	65.33	0	0	0	0	23.54	1.95	52.70

The following table give the targets for tissue simulating liquid:

### For Head:

Frequency (MHz)	Conductivity (σ)	+/- 5% Range	Permittivity (εr)	+/- 5% Range
2450	1.80	1.71~1.89	39.20	37.24~41.16

### For Body:

Frequency (MHz)	Conductivity (σ)	+/- 5% Range	Permittivity (εr)	+/- 5% Range
2450	1.95	1.85~2.05	52.70	50.06~55.33

### The following table show the measuring results for simulating liquid:

Liquid Type	Liquid Temp. (°C)	Parameters	Target	Measured	Deviation (%)	Limited (%)	Measured Date
Body2450	21.8	Permitivity(ε)	52.70	50.42	-4.33	± 5	2013-10-14
B00y2430	21.0	Conductivity(σ)	1.95	2.01	3.08	± 5	2013-10-14
Body2450 21.8		Permitivity(ε)	52.70	50.53	-4.12	± 5	2013-10-31
Body2450	21.0	Conductivity(σ)	1.95	1.98	1.54	± 5	2013-10-31


Date of Issue : November 1, 2013

### 12.3 SYSTEM PERFORMANCE CHECK

The system performance check is performed prior to any usage of the system in order to guarantee reproducible results. The system performance check verifies that the system operates within its specifications of  $\pm 10\%$ . The system performance check results are tabulated below. And also the corresponding SAR plot is attached as well in the SAR plots files.

### SYSTEM PERFORMANCE CHECK MEASUREMENT CONDITIONS

- The measurements were performed in the flat section of the SAM twin phantom filled with head and body simulating liquid of the following parameters.
- The DASY5 system withan E-fileld probe EX3DV4 SN: 3798 was used for the measurements.
- The dipole was mounted on the small tripod so that the dipole feed point was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15 mm (below 1 GHz) and 10 mm (above 1 GHz) from dipole center to the simulating liquid surface.
- The coarse grid with a grid spacing of 10mm was aligned with the dipole.
- Special 7x7x7 fine cube was chosen for cube integration (dx= 5 mm, dy= 5 mm, dz= 5 mm).
- Distance between probe sensors and phantom surface was set to 2 mm.
- The dipole input power was 1W±3%.
- The results are normalized to 1 W input power.

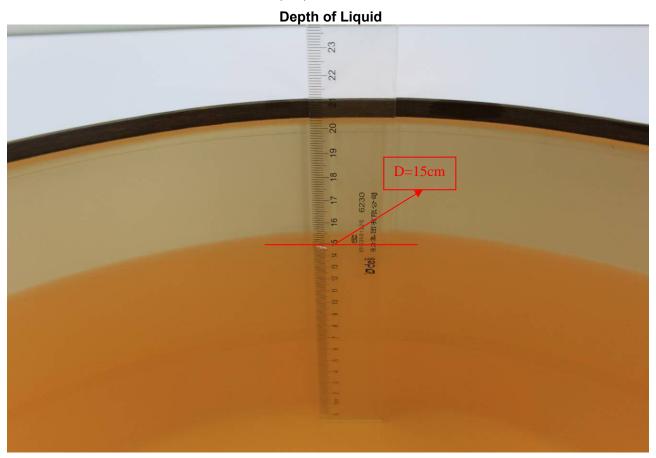

Note: For SAR testing, the depth is 15cm shown above

Date of Issue :November 1, 2013

## SYSTEM PERFORMANCE CHECK RESULTS

Liquid Type	Ambient Temp. (°C)		Input Power (W)	Measured SAR1g (W/Kg)	Target	1W Normalized SAR1g(W/Kg)	Deviation (%)	Limited (%)	Date
Body2450	23.4	21.8	0.25	13.70	51.50	54.80	6.41	± 10	2013-10-14
Body2450	23.4	21.8	0.25	13.69	51.50	54.76	6.33	± 10	2013-10-31

### 12.4 EUT CONDUCTED POWER

### WLAN Conducted output power(dBm):

			Average power(dBm)
Mode	Channel	Frequence	Date Rate(bps)
			1M
	1	2412 MHZ	14.67
802.11 b	6	2437 MHZ	14.83
	11	2462 MHZ	14.59

			Average power(dBm)
Mode	Channel	Frequence	Date Rate(bps)
			6M
	1	2412 MHZ	11.62
802.11 g	6	2437 MHZ	11.51
	11	2462 MHZ	11.55

Mode			Average power(dBm)
	Channel	Frequence	Date Rate(bps)
			6.5M
	1	2412 MHZ	10.46
802.11 n HT20	6	2437 MHZ	10.86
	11	2462 MHZ	10.66


Mode			Average power(dBm)
	Channel	Frequence	Date Rate(bps)
			6.5M
	3	2422 MHZ	10.35
802.11 n HT40	6	2437 MHZ	10.28
	9	2452 MHZ	10.47

### Note:

- Per KDB 248227 D01 v01r02, choose the highest output power channel to test SAR and 1. determine further SAR exclusion
- 2. For each frequency band, testing at higher data rates and higher order modulations is not required when the maximum average output power for each of these configurations is less than 1/4dB higher than those measured at the lowest data rate
- 3. Per KDB 248227,11g and 11n-HT20 output power is less than 1/4 dB higher than 11b mode, the SAR test can be excluded.



### 12.5 SAR TEST CONFIGURATIONS

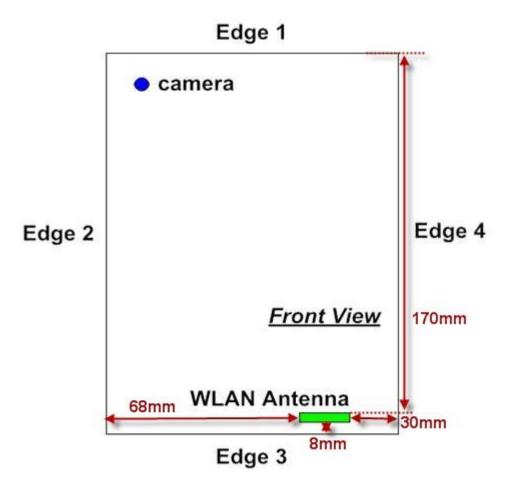

Device dimensions (H x W x D): 190 x 116 x 12 mm

Antennas	Wireless Interface
WLAN Antenna	WLAN 2.4GHz Band

Exposure	Wireless Interface	802.11 b
Position	Tune-up Maximum power (dBm)	15
	Tune-up Maximum rated power (mW)	31.62
D	Antenna to user (mm)	4
Rear Side	SAR exclusion threshold (mW)	9.61
Olde	SAR testing required?	Yes
	Antenna to user (mm)	170
Edge 1	SAR exclusion threshold	1296.1
	SAR testing required?	No
	Antenna to user (mm)	68
Edge 2	SAR exclusion threshold (mW)	276.1
	SAR testing required?	No
	Antenna to user (mm)	8
Edge 3	SAR exclusion threshold (mW)	19.2
	SAR testing required?	Yes
	Antenna to user (mm)	30
Edge 4	SAR exclusion threshold (mW)	57.7
	SAR testing required?	No

### Note:

- 1. Maximum power is the source-based time-average power and represents the maximum RF output power among production units
- 2. Per KDB 447498 D01v05r01, for larger devices, the test separation distance is determined by the closest separation between the antenna and the user.
- 3. Per KDB 447498 D01v05r01, standalone SAR test exclusion threshold is applied; If the distance of
- the antenna to theuser is < 5mm, 5mm is used to determine SAR exclusion threshold


  4. Per KDB 447498 D01v05r01, the 1-g and 10-g SAR test exclusion thresholds for 100 MHz to 6 GHz at test separation distances ≤ 50 mm are determined by:

[(max. power of channel, including tune-up tolerance, mW)/(min. test separation distance, mm)]  $\cdot [\sqrt{f(GHz)}] \le 3.0$  for 1-g SAR and  $\le 7.5$  for 10-g extremity SAR

- f(GHz) is the RF channel transmit frequency in GHz
- Power and distance are rounded to the nearest mW and mm before calculation
  - The result is rounded to one decimal place for comparison
- 5. Per KDB 447498 D01v05, at 100 MHz to 6 GHz and for test separation distances > 50 mm, the SAR test exclusion threshold is determined according to the following
- a) [Threshold at 50 mm in step 1) + (test separation distance 50 mm)·(f(MHz)/150)] mW, at 100 MHz to 1500 MHz
- b) [Threshold at 50 mm in step 1) + (test separation distance 50 mm)·10] mW at > 1500 MHz and ≤ 6 ĞĤz



### 12.6 SAR MEASUREMENT RESULTS

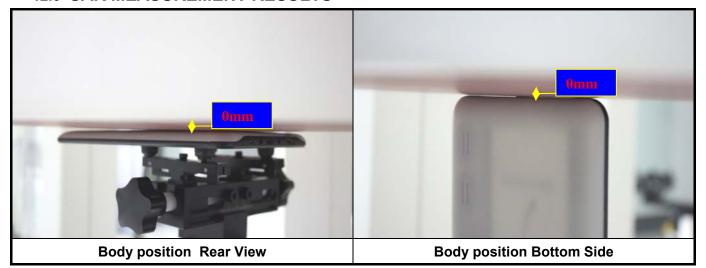

### **Body SAR Test Records**

### **WLAN 2.4GHz SAR**

Band	Mode	Test Position	Dist. (mm)	Ch.	Freq. (MHZ)	max Power (dBm)	Turn- Up Limit (dBm)	Scaled Factor	Power Drift (dB)	SAR1g (mW/g)	Scaled SAR1g (mW/g)
WLAN 2.4GHz	802.11b	Rear Side	0	1	2412	14.67	15	1.079	-0.13	0.852	0.919
WLAN 2.4GHz	802.11b	Rear Side	0	6	2437	14.83	15	1.040	0.16	0.929	0.966
WLAN 2.4GHz	802.11b	Rear Side	0	11	2462	14.59	15	1.099	0.07	0.796	0.875
WLAN 2.4GHz	802.11b	Edge 3	0	6	2437	14.83	15	1.040	0.10	0.437	0.454

### **Repeated SAR Measurement**

Band	Mode	Test Position	Dist (mm )	Ch	max Power (dBm)	Turn- Up Limit (dBm )	Scaled Factor	Power Drift (dB)	SAR1g (mW/g)	Ratio	Scaled SAR1g (mW/g)
WLAN 2.4GHz	802.11b	Rear Side	0	1	14.67	15	1.079	0.09	0.857	1.01	0.925
WLAN 2.4GHz	802.11b	Rear Side	0	6	14.83	15	1.040	0.08	0.917	1.01	0.954

### Note:

- 1. Per KDB 865664 D01v01r01, for each frequency band, repeated SAR measurement is required only when the measured SAR is ≥0.8W/kg
- 2. Per KDB 865664 D01v01r01,if the ratio among the repeated measurement is ≤1.2 and the measured SAR <1.45W/kg,only one repeated measurement is required.
- 3. The ratio is the difference in percentage between original and repeated measured SAR.
- 4. All measurement SAR result is scaled-up to account for tune-up tolerance and is compliant.

Date of Issue :November 1, 2013

### 12.7 TEST RECORDS FOR BODY WORN SAR TEST


- 1. Body-worn exposure conditions are intended to voice call operations, therefore GSM voice call mode is selected to be tested.
- 2. Per KDB 648474 D04v01, when the reported SAR for a body-worn accessory measured without a headset connected to the handset is ≤ 1.2 W/kg, SAR testing with a headset connected to the handset is not required.

### 12.8 SAR MULTI XMITER ASSESSMENT

	Applicable Combination
Simultaneous Transmission	None

# **EUT PHOTO**



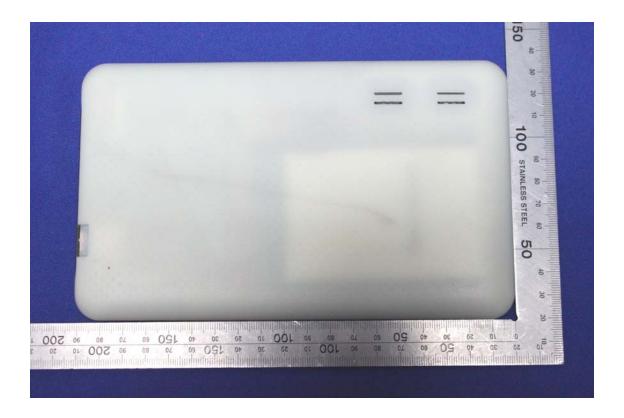









## **EQUIPMENT LIST & CALIBRATION STATUS**

Name of Equipment	Manufacturer	Type/Model	Serial Number	Last Calibration	Calibration Due
PC	HP	Core(rm)3.16G	CZCO48171H	N/A	N/A
Signal Generator	Agilent	83732B	US37101915	06/04/2013	06/03/2014
S-Parameter Network Analyzer	Agilent	E5071B	MY42301382	03/11/2013	03/10/2014
Power Meter	Agilent	E4416A	QB41292714	03/16/2013	03/15/2014
Peak & Average sensor	Agilent	E9327A	CF0001	03/16/2013	03/15/2014
E-field PROBE	SPEAG	EX3DV4	3798	07/26/2013	07/25/2014
DAE	SPEAG	DEA4	679	01/16/2013	01/15/2014
DIPOLE 2450MHZ ANTENNA	SPEAG	D2450V2	817	07/31/2013	07/30/2014
SAM PHANTOM (ELI4 v4.0)	SPEAG	QDOVA001BB	1102	N/A	N/A
ROBOT	SPEAG	TX60	F10/5E6AA1/A101	N/A	N/A
ROBOT KRC	SPEAG	CS8C	F10/5E6AA1/C101	N/A	N/A
LIQUID CALIBRATION KIT	ANTENNESSA	41/05 OCP9	00425167	N/A	N/A

Date of Issue : November 1, 2013

## 15. FACILITIES

All measurement facilities used to collect the measurement data are located at

No.10, Weiye Rd., Innovation Park, Eco & Tec. Development Part, Kunshan City, Jiangsu Province, China.

### REFERENCES 16.

- [1] Federal Communications Commission, \Report and order: Guidelines for evaluating the environ-mental effects of radiofrequency radiation", Tech. Rep. FCC 96-326, FCC, Washington, D.C. 20554, 1996.
- David L. Means Kwok Chan, Robert F. Cleveland, \Evaluating compliance with FCC guidelines for human exposure to radiofrequency electromagnetic fields, Tech. Rep., Federal Communication Commission, O\_ce of Engineering & Technology, Washington, DC, 1997.
- Thomas Schmid, Oliver Egger, and Niels Kuster, \Automated E- eld scanning system for dosimetric assessments", IEEE Transactions on Microwave Theory and Techniques, vol. 44, pp. 105{113, Jan. 1996.
- Niels Kuster, Ralph K.astle, and Thomas Schmid, \Dosimetric evaluation of mobile communications equipment with known precision", IEICE Transactions on Communications, vol. E80-B, no. 5, pp. 645{652, May 1997.
- [5] CENELEC. \Considerations for evaluating of human exposure to electromagnetic fields (EMFs) from mobile telecommunication equipment (MTE) in the frequency range 30MHz - 6GHz", Tech. Rep., CENELEC, European Committee for Electrotechnical Standardization, Brussels, 1997.
- [6] ANSI, ANSI/IEEE C95.1-1999: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz, The Institute of Electrical and Electronics Engineers, Inc., New York, NY 10017, 1992.
- [7] Katja Pokovic, Thomas Schmid, and Niels Kuster, \Robust setup for precise calibration of Eeld probes in tissue simulating liquids at mobile communications frequencies", in ICECOM 97, Dubrovnik, October 15{17, 1997, pp. 120{124.
- Katja Pokovic, Thomas Schmid, and Niels Kuster, \E- eld probe with improved isotropy in brain simulating liquids", in Proceedings of the ELMAR, Zadar, Croatia, 23(25 June, 1996, pp. 172{175.
- Volker Hombach, Klaus Meier, Michael Burkhardt, Eberhard K. uhn, and Niels Kuster, \The dependence of EM energy absorption upon human head modeling at 900 MHz", IEEE Transactions on Microwave Theory and Techniques, vol. 44, no. 10, pp. 1865{1873, Oct. 1996.
- [10] Klaus Meier, Ralf Kastle, Volker Hombach, Roger Tay, and Niels Kuster, \The dependence of EM energy absorption upon human head modeling at 1800 MHz", IEEE Transactions on Microwave Theory and Techniques, Oct. 1997, in press.
- [11] W. Gander, Computermathematik, Birkhaeuser, Basel, 1992.
- [12] W. H. Press, S. A. Teukolsky, W. T. Vetterling, and B. P. Flannery, Numerical Recepies in C, The Art of Scientific Computing, Second Edition, Cambridge University Press, 1992..Dosimetric Evaluation of Sample device, month 1998 9
- [13] NIS81 NAMAS, \The treatment of uncertainty in EMC measurement", Tech. Rep., NAMAS Executive, National Physical Laboratory, Teddington, Middlesex, England, 1994.
- [14] Barry N. Taylor and Christ E. Kuyatt, \Guidelines for evaluating and expressing the uncertainty of NIST measurement results", Tech. Rep., National Institute of Standards and Technology, 1994. Dosimetric Evaluation of Sample device, month 1998 10

Date of Issue :November 1, 2013

### **ATTACHMENTS 17**.

Exhibit	Content
1	System Performance Check Plots
2	Dipole calibration report D2450V2 SN: 817
3	Probe calibration report EX3DV4 SN3798
4	DAE calibration report DEA4 SD000D04BJ SN:1245
5	SAR Test Plots

## **APPENDIX A: PLOTS OF PERFORMANCE CHECK**

The plots are showing as followings.

Report No: C131009S04-SF-R1

FCCID: ZFN-A072D

Date of Issue :November 1, 2013

Test Laboratory: Compliance Certification Services Inc. Date: 10/14/2013

SystemPerformanceCheck-D2450\_2013.10.14

DUT: Dipole 2450 MHz D2450V2; Type: D24500V2; Serial: 817

Communication System: CW; Communication System Band: D2450 (2450.0 MHz); Frequency: 2450

MHz; Duty Cycle: 1:1

Medium parameters used: f = 2450 MHz;  $\sigma = 2.009 \text{ S/m}$ ;  $\varepsilon_r = 50.424$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Room Ambient Temperature: 23.4°C; Liquid Temperature: 21.8°C

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY Configuration:

- Probe: EX3DV4 SN3798; ConvF(7.08, 7.08, 7.08); Calibrated: 7/26/2013;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1245; Calibrated: 7/20/2013
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1102
- DASY52 52.8.5(1059);
- SEMCAD X Version 14.6.8 (7028)


System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Area Scan (8x9x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR (measured) = 18.4 W/kg

System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 90.176 V/m; Power Drift = 0.08 dB

Peak SAR (extrapolated) = 26.5 W/kg

**SAR(1 g) = 13.7 W/kg; SAR(10 g) = 6.65 W/kg** Maximum value of SAR (measured) = 20.1 W/kg

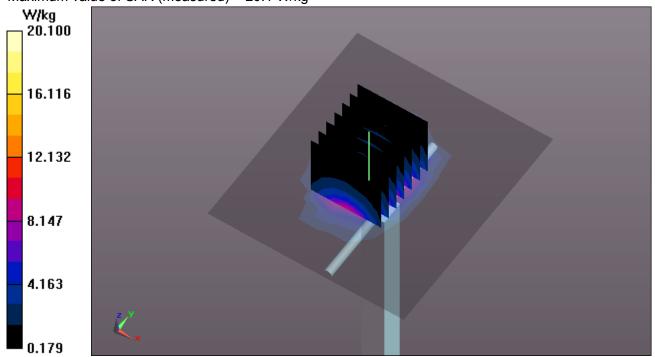

Test Laboratory: Compliance Certification Services Inc. Date: 10/31/2013

SystemPerformanceCheck-D2450\_2013.10.31

DUT: Dipole 2450 MHz D2450V2; Type: D24500V2; Serial: 817

Communication System: CW; Communication System Band: D2450 (2450.0 MHz); Frequency: 2450

MHz; Duty Cycle: 1:1

Medium parameters used: f = 2450 MHz;  $\sigma = 1.98 \text{ S/m}$ ;  $\varepsilon_r = 50.53$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Room Ambient Temperature: 23.4°C; Liquid Temperature: 21.8°C

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY Configuration:** 

- Probe: EX3DV4 SN3798; ConvF(7.08, 7.08, 7.08); Calibrated: 7/26/2013;
- Sensor-Surface: 2mm (Mechanical Surface Detection) Electronics: DAE4 Sn1245; Calibrated: 7/20/2013
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1102
- DASY52 52.8.5(1059);
- SEMCAD X Version 14.6.8 (7028)


System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Area Scan (8x9x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR (measured) = 18.4 W/kg

System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 90.176 V/m; Power Drift = 0.08 dB

Peak SAR (extrapolated) = 26.5 W/kg

SAR(1 g) = 13.69 W/kg; SAR(10 g) = 6.64 W/kgMaximum value of SAR (measured) = 19.9 W/kg

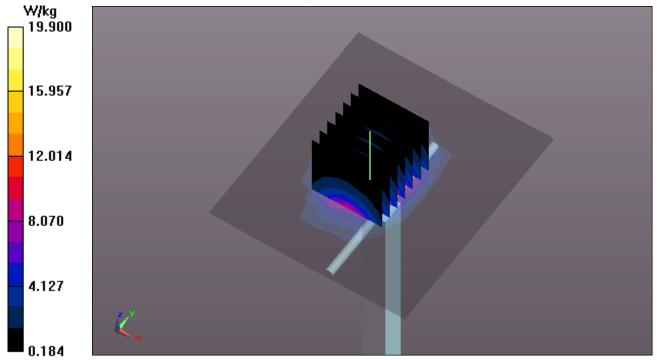

Date of Issue :November 1, 2013

	Λ	D	DE	= N	חו	IY	B.	n	V 67	/ C	ΛI	IRE	ΛТ	ION		DT	<b>IFIC</b>	ΛT	
1	н		76	=17	1U	אוי	D.	U	A31		AL	IDR	AI	IUN	ICE	: R I	ILIC	·Αι	

The DASY Calibration Certificates are showing as followings .

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client

CCS-CN (Auden)

Accreditation No.: SCS 108

C

Certificate No: D2450V2-817\_Jul13

## CALIBRATION CERTIFICATE

Object

D2450V2 - SN: 817

Calibration procedure(s)

QA CAL-05.v9

Calibration procedure for dipole validation kits above 700 MHz

Calibration date:

Dimany Standards

Approved by:

July 31, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

lina

Primary Standards	10.4	Gai Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	01-Nov-12 (No. 217-01640)	Oct-13
Power sensor HP 8481A	US37292783	01-Nov-12 (No. 217-01640)	Oct-13
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-13 (No. 217-01736)	Apr-14
Type-N mismatch combination	SN: 5047.3 / 06327	04-Apr-13 (No. 217-01739)	Apr-14
Reference Probe ES3DV3	SN: 3205	28-Dec-12 (No. ES3-3205_Dec12)	Dec-13
DAE4	SN: 601	25-Apr-13 (No. DAE4-601_Apr13)	Apr-14
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-12)	In house check: Oct-13
	Name	Function	Signature
Calibrated by:	Israe El-Naouq	Laboratory Technician	Orran C1-Dasses

Cal Data (Cadillanta No.)

Issued: July 31, 2013

Caback had Calibration

This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Katja Pokovic

Certificate No: D2450V2-817\_Jul13

Page 1 of 8

Technical Manager

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerlacher Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taretura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the size

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL ConvF

N/A

tissue simulating liquid

sensitivity in TSL / NORM x,y,z not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### Additional Documentation:

d) DASY4/5 System Handbook

## Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- · SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-817\_Jul13

Page 2 of 8

Date of Issue :November 1, 2013

#### Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

## Head TSL parameters

The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.8 ± 6 %	1.81 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	****	

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.3 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.6 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm3 (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.18 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 16.5 % (k=2)

## Body TSL parameters

e following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	50.5 ± 6 %	2.01 mho/m ± 8 %
Body TSL temperature change during test	< 0.5 °C	****	Onto.

## SAR result with Body TSL

SAR averaged over 1 cm3 (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.6 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	49.2 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5,87 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.1 W/kg ± 16.5 % (k=2)

Certificate No: D2450V2-817\_Jul13

Page 3 of 8

### Appendix

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.5 Ω + 2.9 jΩ	
Return Loss	- 27.1 dB	

## Antenna Parameters with Body TSL

Impedance, transformed to feed point	$49.7 \Omega + 4.5 j\Omega$
Return Loss	- 27.0 dB

## General Antenna Parameters and Design

Electrical Delay (one direction)	1.159 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the 'Measurement Conditions' paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG	
Manufactured on	October 23, 2007	

Certificate No: D2450V2-817\_Jul13

## DASY5 Validation Report for Head TSL

Date: 31.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 817

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz;  $\sigma = 1.81 \text{ S/m}$ ;  $\epsilon_r = 37.8$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)


### DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.52, 4.52, 4.52); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

## Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 99.781 V/m; Power Drift = 0.06 dB Peak SAR (extrapolated) = 27.7 W/kg

SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.18 W/kgMaximum value of SAR (measured) = 16.8 W/kg

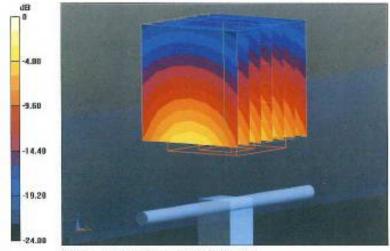

0 dB = 16.8 W/kg = 12.25 dBW/kg

## Impedance Measurement Plot for Head TSL

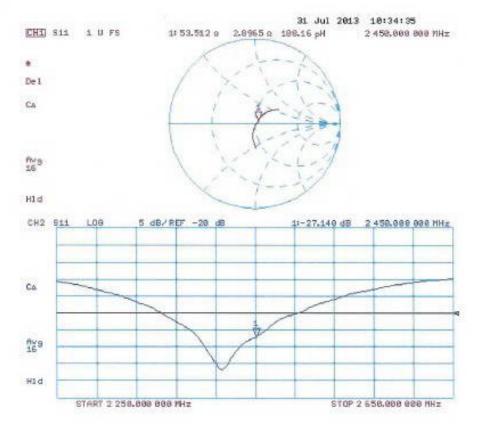

## DASY5 Validation Report for Body TSL

Date: 31.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 817

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz;  $\sigma = 2.01 \text{ S/m}$ ;  $\varepsilon_r = 50.5$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section


Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.42, 4.42, 4.42); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)


## Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 94.151 V/m; Power Drift = 0.06 dB Peak SAR (extrapolated) = 26.3 W/kg SAR(1 g) = 12.6 W/kg; SAR(10 g) = 5.87 W/kg Maximum value of SAR (measured) = 16.7 W/kg

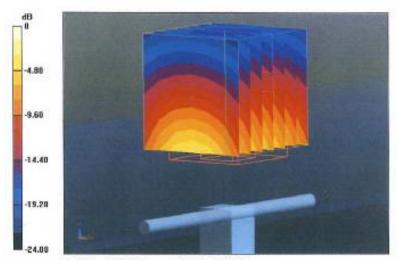

0 dB = 16.7 W/kg = 12.23 dBW/kg

## Impedance Measurement Plot for Body TSL

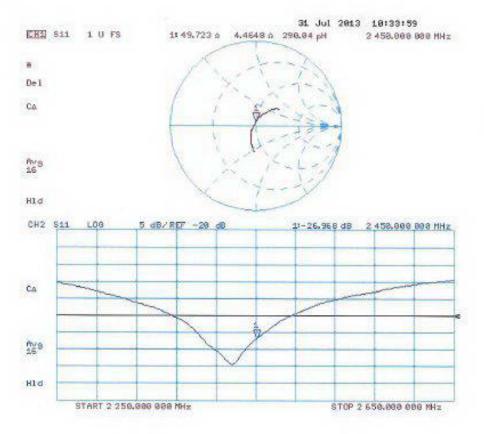

Report No: C131009S04-SF-R1

FCCID: ZFN-A072D

Date of Issue : November 1, 2013

Schmid & Partner Engineering AG

s p e a q

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 info@speag.com, http://www.speag.com

1245

## IMPORTANT NOTICE

## USAGE OF THE DAE 4

The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points:

Battery Exchange: The battery cover of the DAE4 unit is closed using a screw, over tightening the screw may cause the threads inside the DAE to wear out.

Shipping of the DAE: Before shipping the DAE to SPEAG for calibration, remove the batteries and pack the DAE in an antistatic bag. This antistatic bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside.

E-Stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements.

Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect.

DASY Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MOhm is given in the corresponding configuration file.

#### Important Note:

Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer.

#### Important Note:

Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the Estop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure.

#### Important Note:

To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE.

Schmid & Partner Engineering

TN\_BR040315AD DAE4.doc

11.12.2009

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client

CCS-CN (Auden)

Accreditation No.: SCS 108

Certificate No: DAE4-1245 Jul 13

CALIBRATION CERTIFICATE

Object

DAE4 - SD 000 D04 BM - SN: 1245

Calibration procedure(s)

QA CAL-06.v26

Calibration procedure for the data acquisition electronics (DAE)

Calibration date:

July 25, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	02-Oct-12 (No:12728)	Oct-13
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	07-Jan-13 (in house check)	In house check: Jan-14
Calibrator Box V2.1	SE UMS 006 AA 1002	07-Jan-13 (in house check)	In house check: Jan-14

Calibrated by:

Name Dominique Steffen Function Technician Signature

Approved by:

Fin Bomholt

Deputy Technical Manager

Issued: July 25, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: DAE4-1245\_Jul13

Page 1 of 5

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage

Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE

data acquisition electronics

Connector angle

information used in DASY system to align probe sensor X to the robot

coordinate system.

## Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
  - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
  - AD Converter Values with Inputs shorted: Values on the internal AD converter corresponding to zero input voltage
  - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
  - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
  - Power consumption: Typical value for information. Supply currents in various operating modes.

Certificate No: DAE4-1245\_Jul13

Page 2 of 5

## DC Voltage Measurement

A/D - Converter Resolution nominal

High Range:

1LSB =

6.1µV.

full range = -100...+300 mV full range = -1......+3mV

Low Range:

1LSB =

61nV,

DASY measurement parameters; Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	x	Y	Z
High Range	405.940 ± 0.02% (k=2)	404.664 ± 0.02% (k=2)	405.801 ± 0.02% (k=2)
Low Range	4.00386 ± 1.50% (k=2)	3.98278 ± 1.50% (k=2)	4.02487 ± 1.50% (k=2)

## Connector Angle

nnector Angle to be used in DASY system	30.5°±1°	٦
nnector Angle to be used in DASY system	30	.5°±1°

Certificate No: DAE4-1245 Jul 13

Page 3 of 5

## Appendix

## 1. DC Voltage Linearity

High Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	199992.97	-4.47	-0.00
Channel X + Input	20001.91	0.89	0.00
Channel X - Input	-19999.11	1.66	-0.01
Channel Y + Input	199994.30	-3.32	-0.00
Channel Y + Input	20001.64	0.75	0.00
Channel Y - Input	-20000.51	0.28	-0.00
Channel Z + Input	199995.90	-1.30	-0.00
Channel Z + Input	20000.30	-0.60	-0.00
Channel Z - Input	-19999.90	0.89	-0.00

Low Range	Reading (μV)	Difference (µV)	Error (%)
Channel X + Input	2001.51	0.38	0.02
Channel X + Input	201.72	0.21	0.11
Channel X - Input	-198,76	-0.28	0.14
Channel Y + Input	2000.72	-0.41	-0.02
Channel Y + Input	199.98	-1.50	-0.74
Channel Y - Input	-198.85	-0.28	0.14
Channel Z + Input	2000.21	-0.84	-0.04
Channel Z + Input	200.77	-0.56	-0.28
Channel Z - Input	-199.95	-1.29	0.65

## 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	-8.24	-10.01
	- 200	10.27	8.63
Channel Y	200	-7.32	-7.74
	- 200	6.53	6.34
Channel Z	200	-5.94	-6.42
	- 200	- 5.13	4.65

## 3. Channel separation

	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (μV)
Channel X	200	-	4.16	-2.61
Channel Y	200	8.79		3.99
Channel Z	200	9.96	7.22	-

Certificate No: DAE4-1245\_Jul13

Page 4 of 5

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15874	16183
Channel Y	16451	15694
Channel Z	15932	15717

### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	0.94	-0.24	2.04	0.48
Channel Y	-0.42	-1.91	0.54	0.47
Channel Z	-0.83	-2.62	0.57	0.60

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

#### 8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Calibration Laboratory of Schmid & Partner Engineering AG Zoughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnege Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client

CCS-CN (Auden)

Certificate No: EX3-3798\_Jul13

Accreditation No.: SCS 108

C

## CALIBRATION CERTIFICATE

Object

EX3DV4 - SN:3798

Calibration procedure(s)

QA CAL-01.v8, QA CAL-14.v3, QA CAL-23.v4, QA CAL-25.v4

Calibration procedure for dosimetric E-field probes

Calibration date:

July 26, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)\*C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	04-Apr-13 (No. 217-01733)	Apr-14
Power sensor E4412A	MY41498087	04-Apr-13 (No. 217-01733)	Apr-14
Reference 3 dB Attenuator	SN: S5054 (3c)	04-Apr-13 (No. 217-01737)	Apr-14
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-13 (No. 217-01735)	Apr-14
Reference 30 dB Attenuator	SN: S5129 (30b)	04-Apr-13 (No. 217-01738)	Apr-14
Reference Probe ES3DV2	SN: 3013	28-Dec-12 (No. ES3-3013_Dec12)	Dec-13
DAE4	SN: 660	31-Jan-13 (No. DAE4-660_Jan13)	Jan-14
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-15
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-12)	In house check: Oct-13

Calibrated by:

Name

Function

Signature

Laboratory Technician

O Diff

Approved by:

Katja Pokovic

Technical Manager

Issued: July 26, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: EX3-3798\_Jul13

Page 1 of 11

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage

Service suisse d'étalonnage Servizio svizzoro di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL NORMx,y,z ConvF tissue simulating liquid sensitivity in free space sensitivity in TSL / NORMx,y,z diode compression point

CF A, B, C, D

DCP

crest factor (1/duty\_cycle) of the RF signal modulation dependent linearization parameters

Polarization φ

φ rotation around probe axis

Polarization 9

9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

#### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- Techniques", December 2003

  b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
   NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is
  implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
  in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z; A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: EX3-3798\_Jul13

Page 2 of 11

July 26, 2013

# Probe EX3DV4

SN:3798

Manufactured: April 5, 2011

Calibrated: July 26, 2013

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: EX3-3798\_Jul13

Page 3 of 11

July 26, 2013

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3798

#### **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)	
Norm (µV/(V/m) <sup>2</sup> ) <sup>A</sup>	0.54	0.51	0.59	± 10.1 %	
DCP (mV) <sup>8</sup>	95.9	98.8	98.6		

#### **Modulation Calibration Parameters**

UID	Communication System Name		A dB	B dBõV	С	D dB	VR mV	Unc <sup>E</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	164.4	±3.0 %
		Y	0.0	0.0	1.0		168.1	
		Z	0.0	0.0	1.0		130.9	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: EX3-3798\_Jul13

A The uncertainties of NormX,Y,Z do not affect the E2-field uncertainty inside TSL (see Pages 5 and 6).

<sup>Numerical linearization parameter: uncortainty not required.

Uncortainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the</sup> 

July 26, 2013

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3798

#### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>c</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
835	41.5	0.90	9.16	9.16	9.16	0.35	0.94	± 12.0 %
900	41.5	0.97	9.01	9.01	9.01	0.35	0.93	± 12.0 %
1810	40.0	1.40	7.79	7.79	7.79	0.73	0.59	± 12.0 %
1900	40.0	1.40	7.73	7.73	7.73	0.68	0.62	± 12.0 %
2000	40.0	1.40	7.73	7.73	7.73	0.80	0.58	± 12.0 %
2450	39.2	1.80	7.08	7.08	7.08	0.66	0.62	± 12.0 %
5200	36.0	4.66	4.85	4.85	4.85	0.37	1.80	± 13.1 %
5300	35.9	4.76	4.71	4.71	4.71	0.38	1.80	± 13.1 %
5500	35.6	4.96	4.76	4.76	4.76	0.36	1.80	± 13.1 %
5600	35.5	5.07	4.51	4.51	4.51	0.42	1.80	± 13.1 %
5800	35.3	5.27	4.48	4.48	4.48	0.40	1.80	± 13.1 %

<sup>&</sup>lt;sup>5</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS

Certificate No: EX3-3798\_Jul13

of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

At frequencies below 3 GHz, the validity of tissue parameters (c and c) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (c and c) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (c and c) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

July 26, 2013

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3798

#### Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity F	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
835	55.2	0.97	9.27	9.27	9.27	0.49	0.84	± 12.0 %
900	55.0	1.05	9.11	9.11	9.11	0.80	0.62	± 12.0 %
1810	53.3	1.52	7.45	7.45	7.45	0.37	88.0	± 12.0 %
1900	53.3	1.52	7.32	7.32	7.32	0.37	0.86	± 12.0 %
2000	53.3	1.52	7.54	7.54	7.54	0.29	1.01	± 12.0 %
2450	52.7	1.95	7.08	7.08	7.08	0.80	0.57	± 12.0 %
5200	49.0	5.30	4.38	4.38	4.38	0.41	1.90	± 13.1 %
5300	48.9	5.42	4.22	4.22	4.22	0.41	1.90	± 13.1 %
5500	48.6	5.65	3.93	3.93	3.93	0.46	1.90	± 13.1 %
5600	48.5	5.77	3.92	3.92	3.92	0.38	1.90	± 13.1 %
5800	48.2	6.00	4.24	4.24	4.24	0.46	1.90	± 13.1 %

Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS


Certificate No: EX3-3798\_Jul13

of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

At frequencies below 3 GHz, the validity of tissue parameters (c and o) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (c and o) is restricted to ± 5%. The uncertainty is the RSS of the CorwF uncertainty for indicated target tissue parameters.

July 26, 2013

# Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

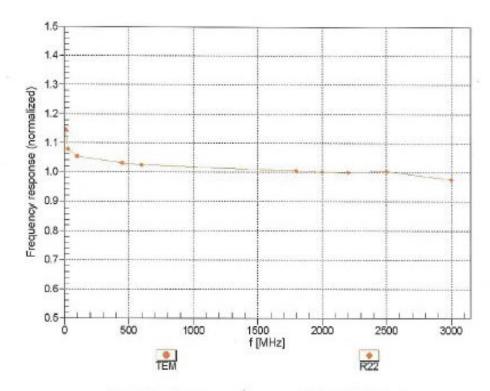

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Certificate No: EX3-3798\_Jul13

Page 7 of 11


July 26, 2013


## Receiving Pattern (φ), 9 = 0°

f=600 MHz,TEM



f=1800 MHz,R22




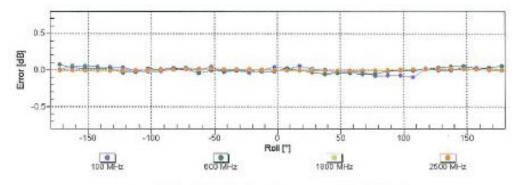


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

July 26, 2013

# Dynamic Range f(SAR<sub>head</sub>) (TEM cell, f = 900 MHz)

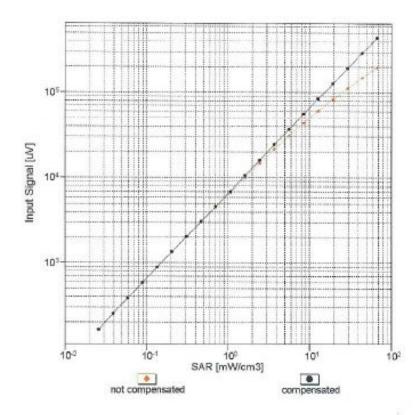

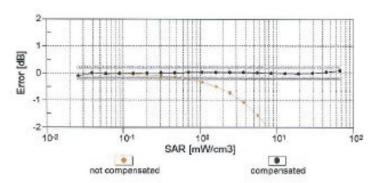


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: EX3-3798\_Jul13


Page 9 of 11


July 26, 2013

## Conversion Factor Assessment

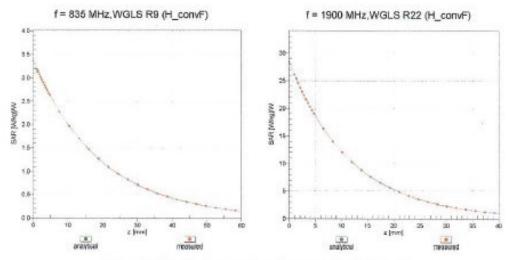

## Deviation from Isotropy in Liquid Error (¢, 9), f = 900 MHz

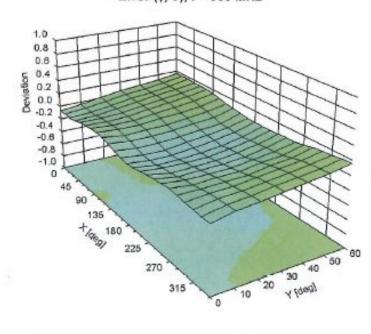



Certificate No: EX3-3798\_Jul13

Page 10 of 11

July 26, 2013

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3798

#### Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-42.4
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	2 mm

Certificate No: EX3-3798\_Jul13

Page 11 of 11

Date of Issue :November 1, 2013

## **APPENDIX C: PLOTS OF SAR TEST RESULT**

The plots are showing in the file named Appendix C Plots of SAR Test Result

**END REPORT**