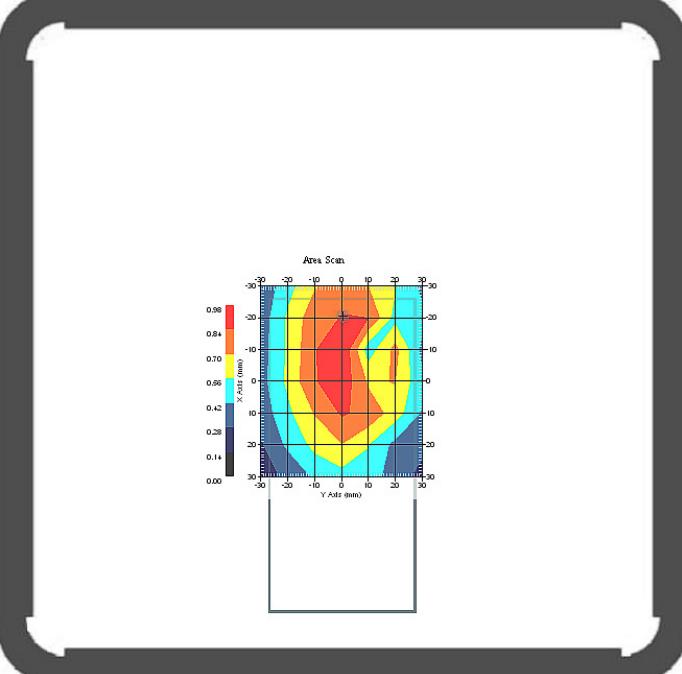
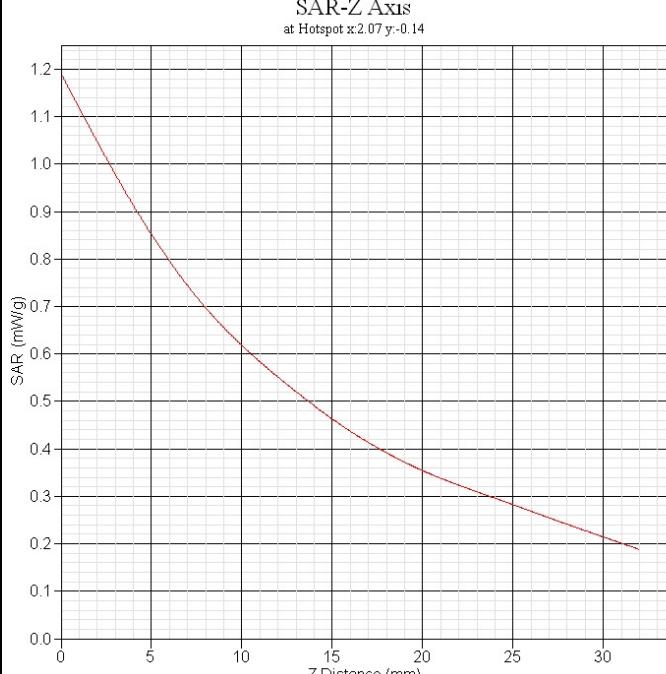
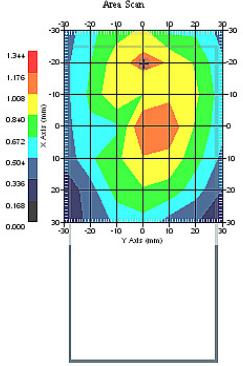
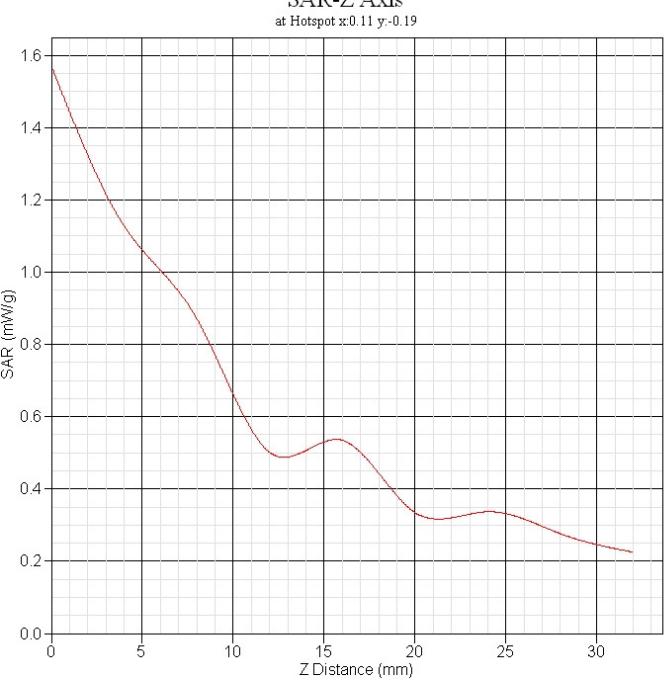
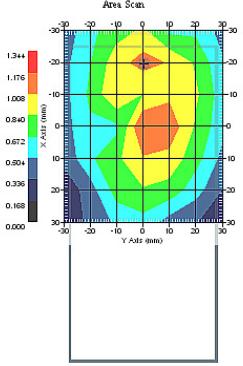
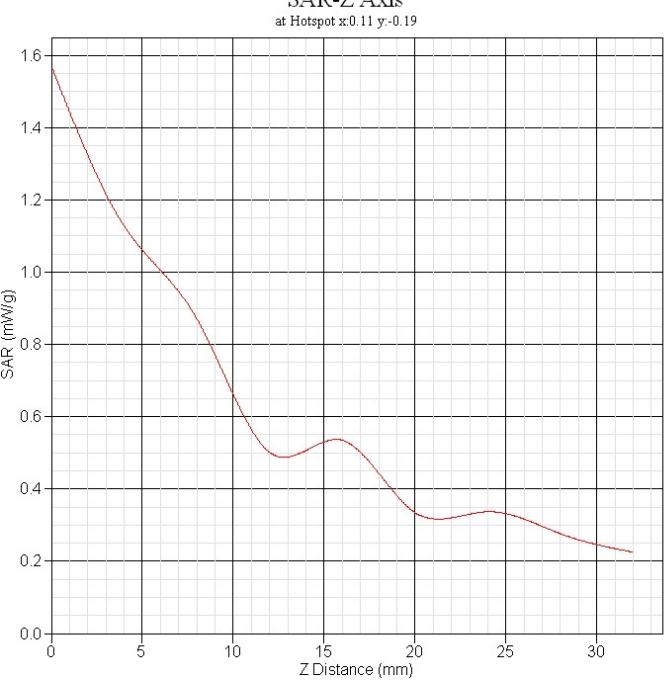
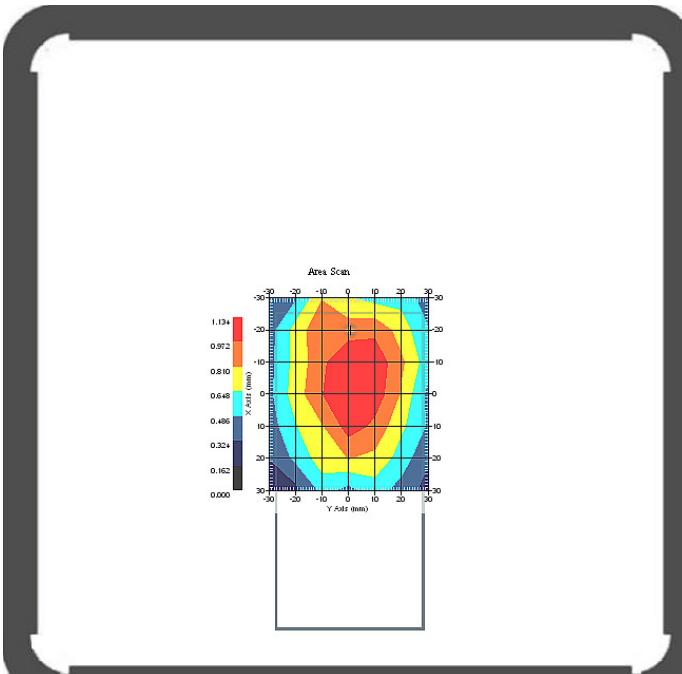
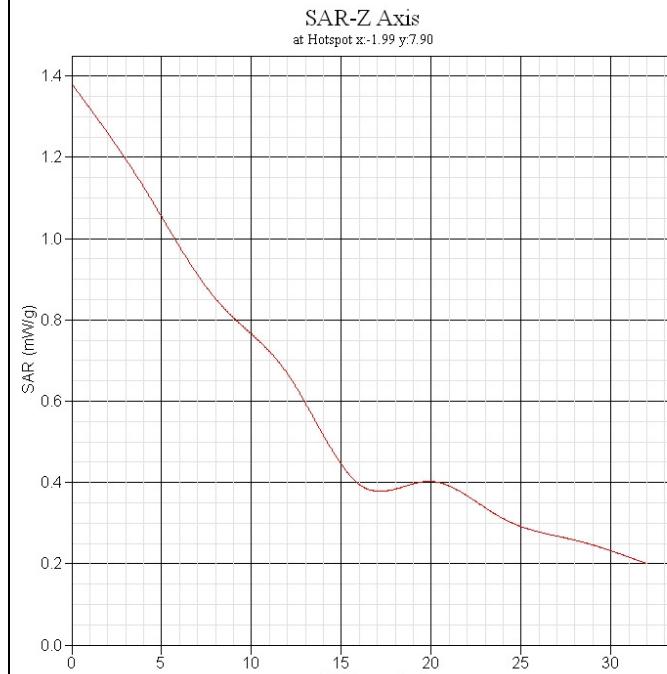
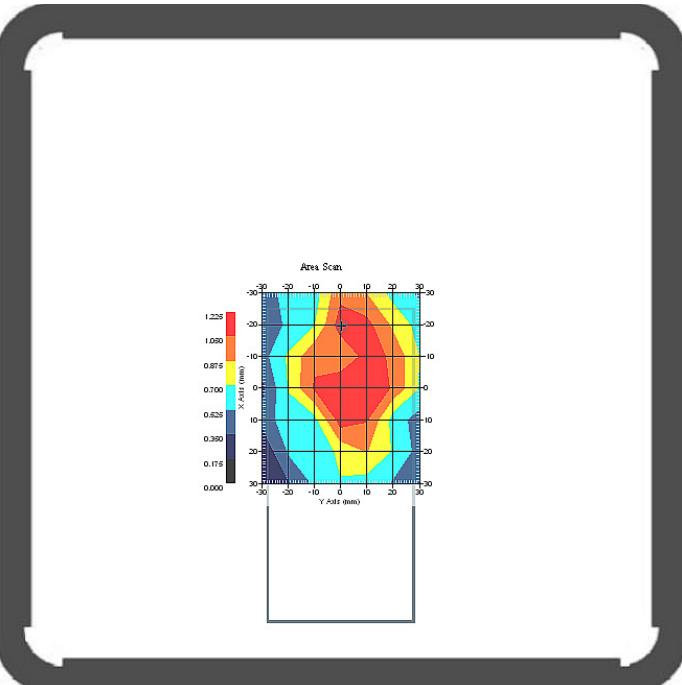
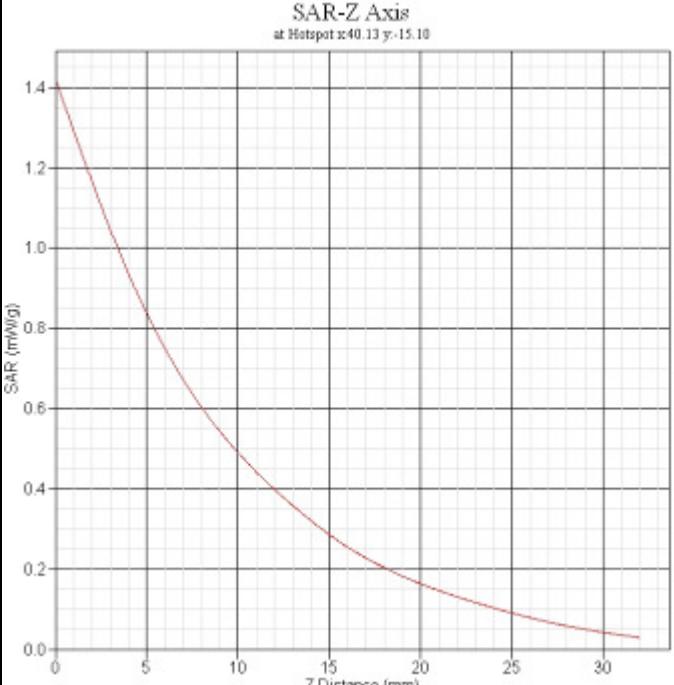




GSM850 body Back CH128	
Frequency(MHz)	824.2
Relative permittivity(real part)	53.36
Conductivity(S/m)	0.95
Variation(%)	1.450
Duty Cycle Factor	8
Crest factor	8
Conversion Factor	6.4
Probe Sensitivity	1.20 1.20 1.20 μ V/(V/m)2
Data	2013-04-15
	 <p>SAR-Z Axis at Hotspot x:2.07 y:-0.14</p>
SAR 1g(W/kg)	0.749
SAR 10g(W/kg)	0.513

GSM850 body Back CH190																					
Frequency(MHz)	836.6																				
Relative permittivity(real part)	53.36																				
Conductivity(S/m)	0.95																				
Variation(%)	2.171																				
Duty Cycle Factor	8																				
Crest factor	8																				
Conversion Factor	6.4																				
Probe Sensitivity	1.20 1.20 1.20 μ V/(V/m)2																				
Data	2013-04-15																				
	 <p>SAR-Z Axis at Hotspot x:0.11 y:-0.19</p> <table border="1"> <caption>Approximate data points from the SAR-Z Axis graph</caption> <thead> <tr> <th>Z Distance (mm)</th> <th>SAR (mW/g)</th> </tr> </thead> <tbody> <tr><td>0</td><td>1.60</td></tr> <tr><td>2</td><td>1.40</td></tr> <tr><td>5</td><td>1.05</td></tr> <tr><td>10</td><td>0.65</td></tr> <tr><td>12</td><td>0.50</td></tr> <tr><td>15</td><td>0.55</td></tr> <tr><td>20</td><td>0.35</td></tr> <tr><td>25</td><td>0.32</td></tr> <tr><td>30</td><td>0.25</td></tr> </tbody> </table>	Z Distance (mm)	SAR (mW/g)	0	1.60	2	1.40	5	1.05	10	0.65	12	0.50	15	0.55	20	0.35	25	0.32	30	0.25
Z Distance (mm)	SAR (mW/g)																				
0	1.60																				
2	1.40																				
5	1.05																				
10	0.65																				
12	0.50																				
15	0.55																				
20	0.35																				
25	0.32																				
30	0.25																				
SAR 1g(W/kg)	1.071																				
SAR 10g(W/kg)	0.753																				



GSM850 body Back CH190(repeat)	
Frequency(MHz)	836.6
Relative permittivity(real part)	53.36
Conductivity(S/m)	0.95
Variation(%)	2.171
Duty Cycle Factor	8
Crest factor	8
Conversion Factor	6.4
Probe Sensitivity	1.20 1.20 1.20 μ V/(V/m)2
Data	2013-04-15
	
SAR 1g(W/kg)	1.058
SAR 10g(W/kg)	0.742



GSM850 body Back CH251	
Frequency(MHz)	848.8
Relative permittivity(real part)	53.36
Conductivity(S/m)	0.95
Variation(%)	-2.567
Duty Cycle Factor	8
Crest factor	8
Conversion Factor	6.4
Probe Sensitivity	1.20 1.20 1.20 μ V/(V/m)2
Data	2013-04-15
	
SAR 1g(W/kg)	0.895
SAR 10g(W/kg)	0.583

GSM850 body Back CH190+earphone	
Frequency(MHz)	836.6
Relative permittivity(real part)	53.36
Conductivity(S/m)	0.95
Variation(%)	-4.429
Duty Cycle Factor	8
Crest factor	8
Conversion Factor	6.4
Probe Sensitivity	1.20 1.20 1.20 μ V/(V/m)2
Data	2013-04-15
	
SAR 1g(W/kg)	0.970
SAR 10g(W/kg)	0.737

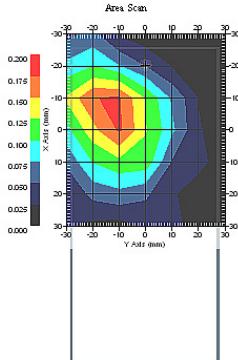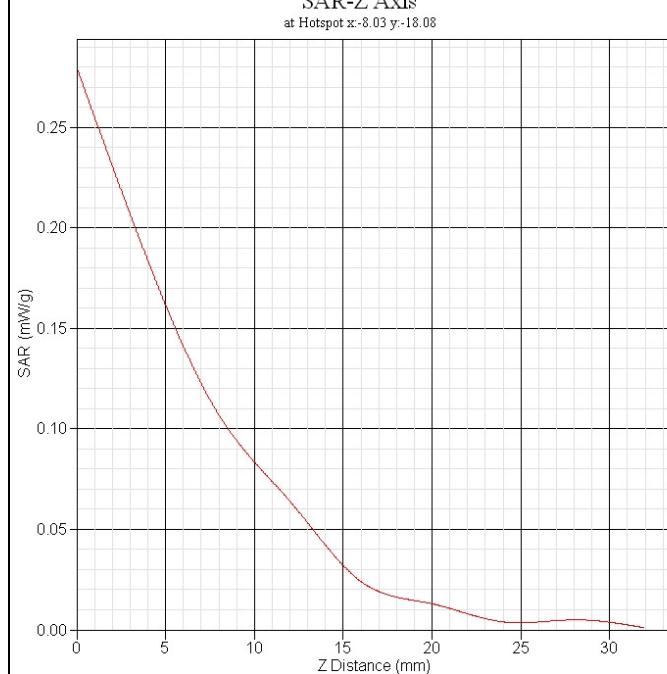
GPRS1900 body Front CH512	
Frequency(MHz)	1850.2
Relative permittivity(real part)	52.91
Conductivity(S/m)	1.50
Variation(%)	-3.398
Duty Cycle Factor	8
Crest factor	8
Conversion Factor	5.4
Probe Sensitivity	1.20 1.20 1.20 μ V/(V/m)2
Data	2013-04-15
	
SAR 1g(W/kg)	0.161
SAR 10g(W/kg)	0.079

GPRS1900 body Back CH512	
Frequency(MHz)	1850.2
Relative permittivity(real part)	52.91
Conductivity(S/m)	1.50
Variation(%)	-1.246
Duty Cycle Factor	8
Crest factor	8
Conversion Factor	5.4
Probe Sensitivity	1.20 1.20 1.20 μ V/(V/m)2
Data	2013-04-15
SAR 1g(W/kg)	0.532
SAR 10g(W/kg)	0.264

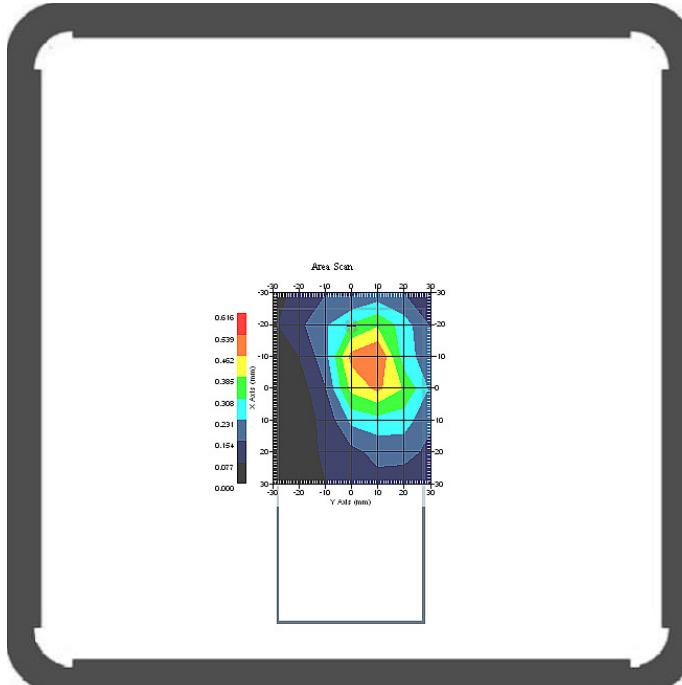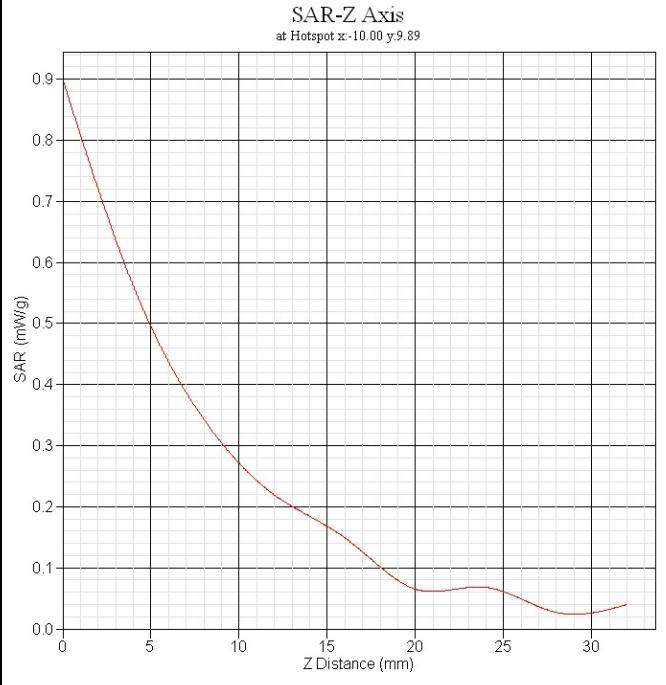GPRS1900 body Back CH512+earphone	
Frequency(MHz)	1850.2
Relative permittivity(real part)	52.91
Conductivity(S/m)	1.50
Variation(%)	-1.720
Duty Cycle Factor	8
Crest factor	8
Conversion Factor	5.4
Probe Sensitivity	1.20 1.20 1.20 μ V/(V/m)2
Data	2013-04-15
	
SAR 1g(W/kg)	0.452
SAR 10g(W/kg)	0.226

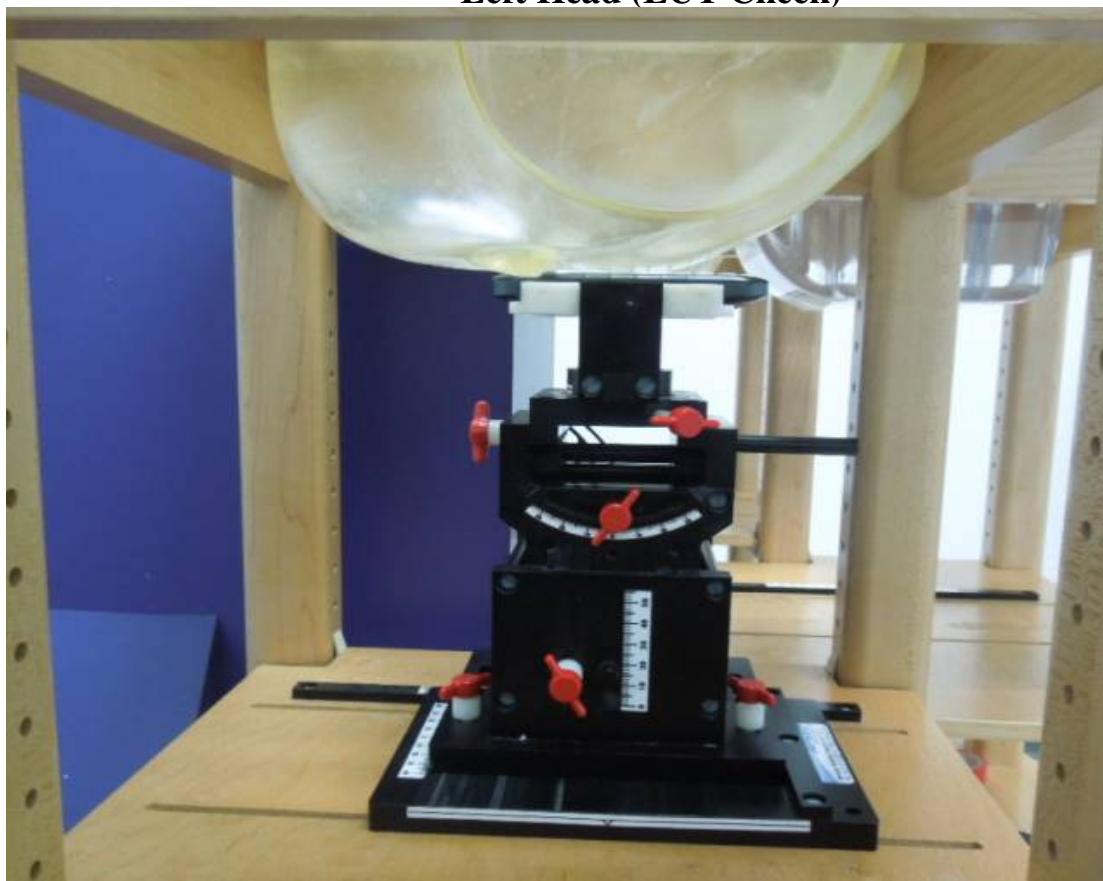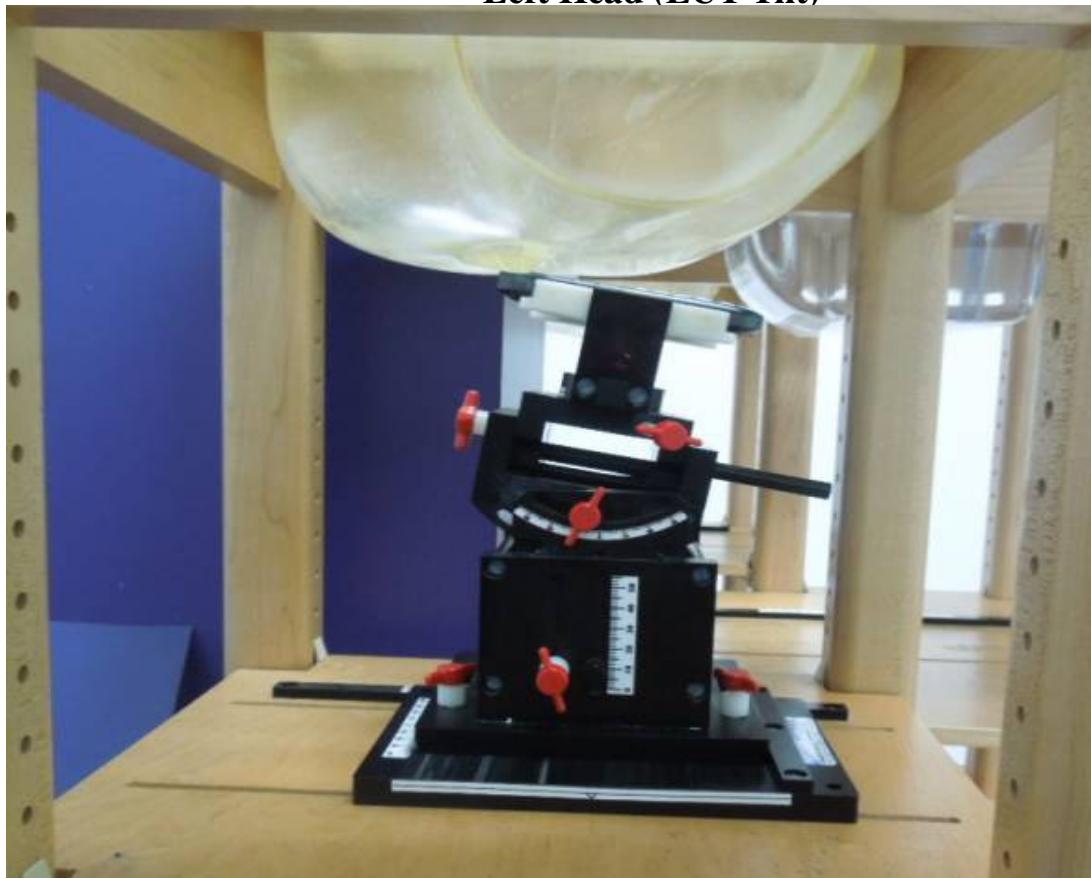SAR Test Photographs**Left Head (EUT Cheek)****Left Head (EUT Tilt)**

Right Head (EUT Cheek)**Right Head (EUT Tilt)**

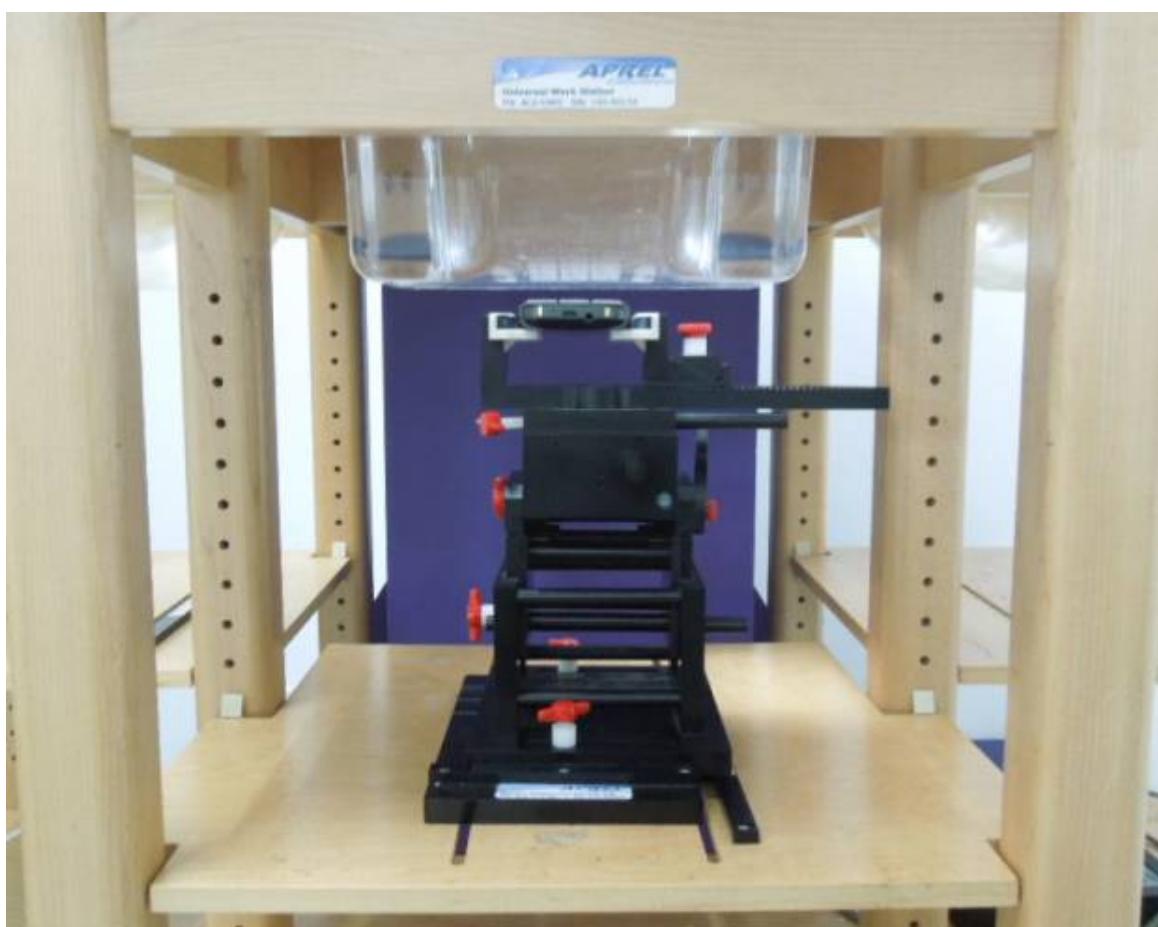Body Back (1.5cm)**Body Front (1.5cm)**



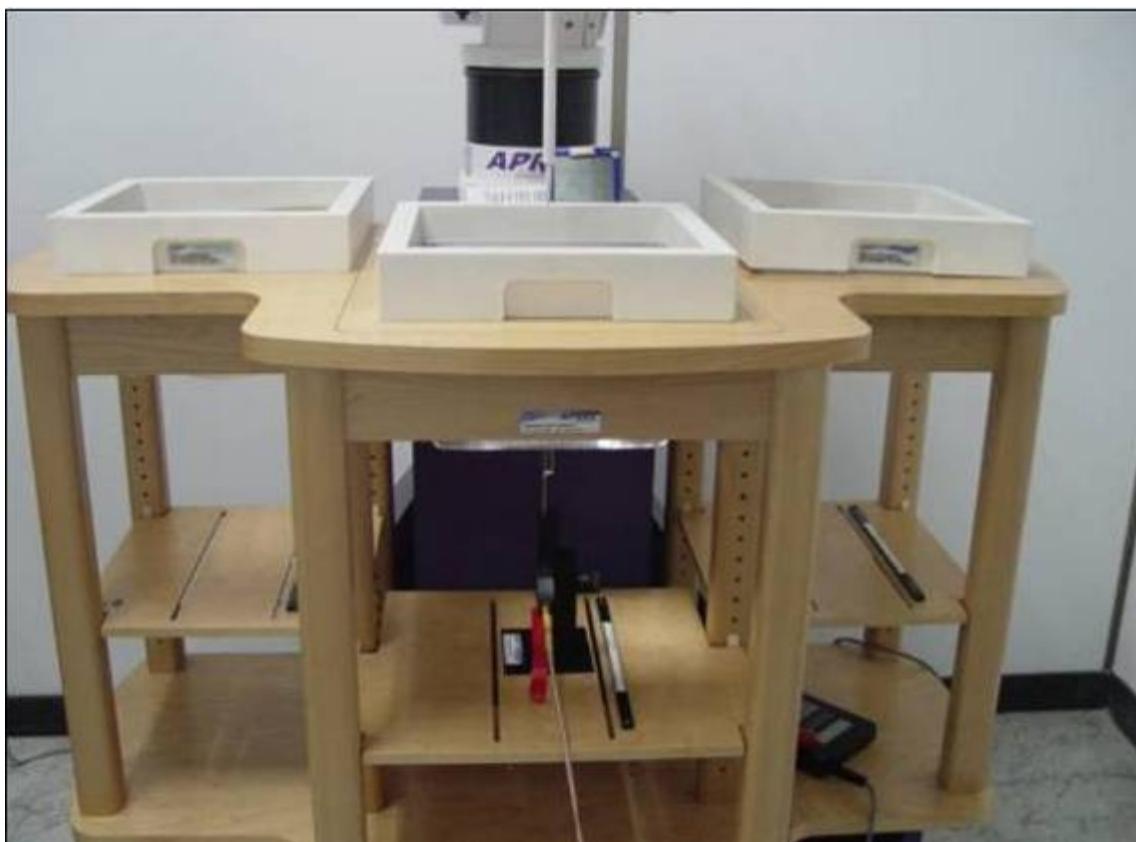
Body Back (1.5cm)+earphone**Validation**

Photo of Liquid Height for Head SAR**Photo of Liquid Height for Body SAR**

EUT

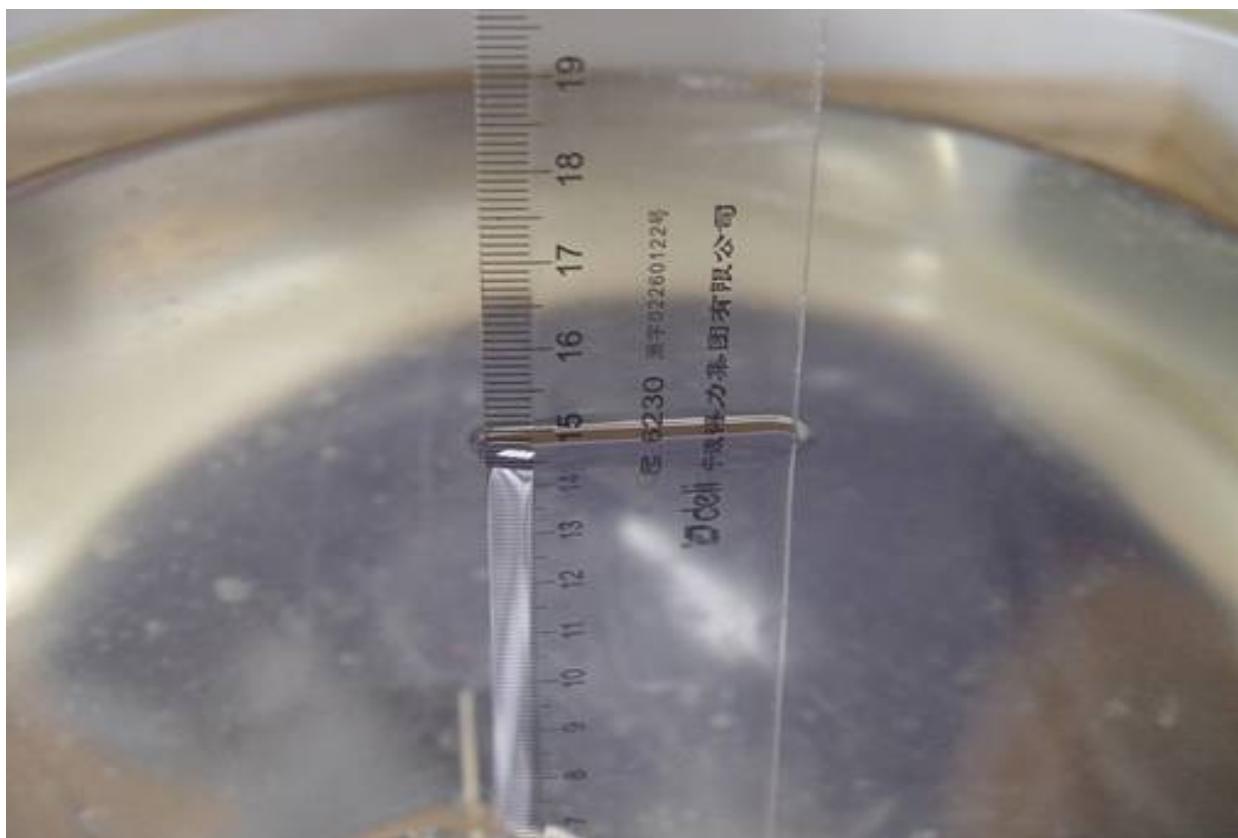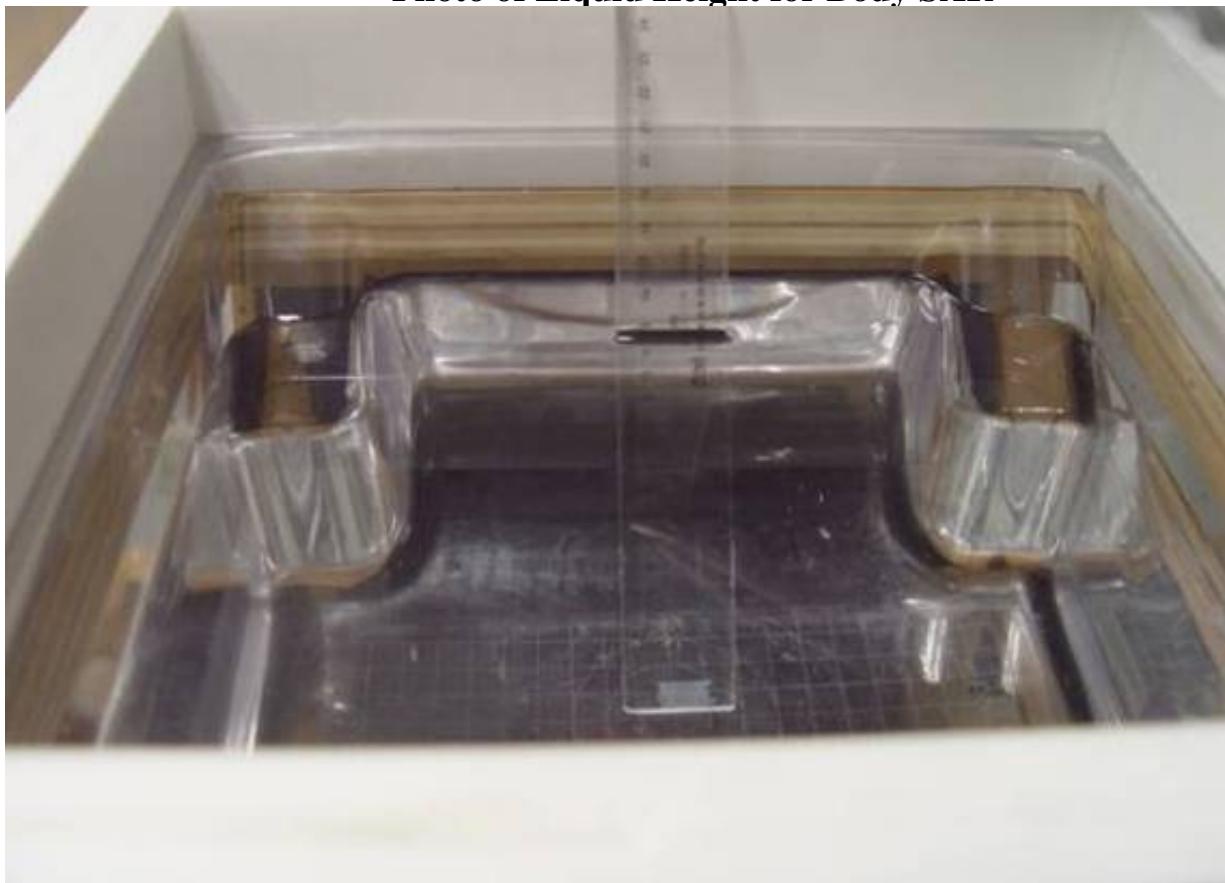


<Justification of the extended calibration>


Referring to KDB 450824, if dipoles are verified in return loss(<-20dB,within 20% of prior calibration),and in impedance(within 5 ohm of prior calibration),the annual calibration is not necessary and the calibration interval can be extended.

Date of Measurement	835 Head					
	Return-Loss (dB)	Delta (%)	Real Impedance(ohm)	Delta (ohm)	Imaginary Impedance(ohm)	Delta (ohm)
5.17.2011	-26.655		51.666		-3.088	
6.28.2012	-26.669	-0.05	52.536	0.87	-4.2203	-1.1323

The return loss is <-20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration.


Therefore the verification result should support extended calibration.

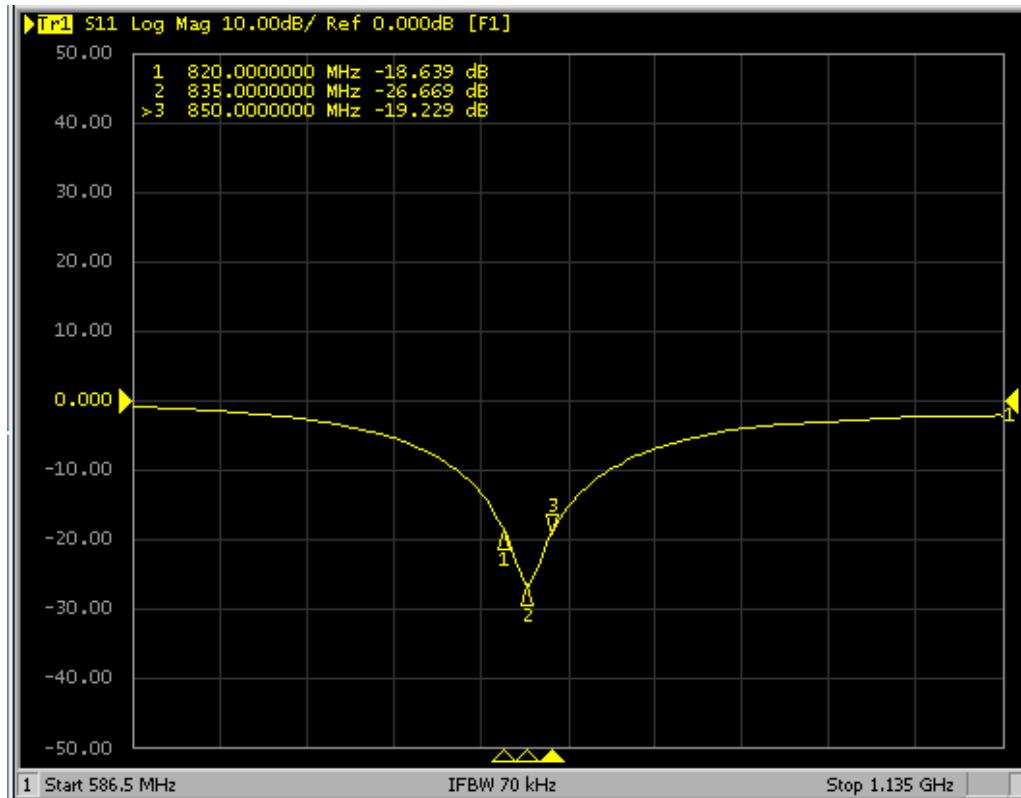


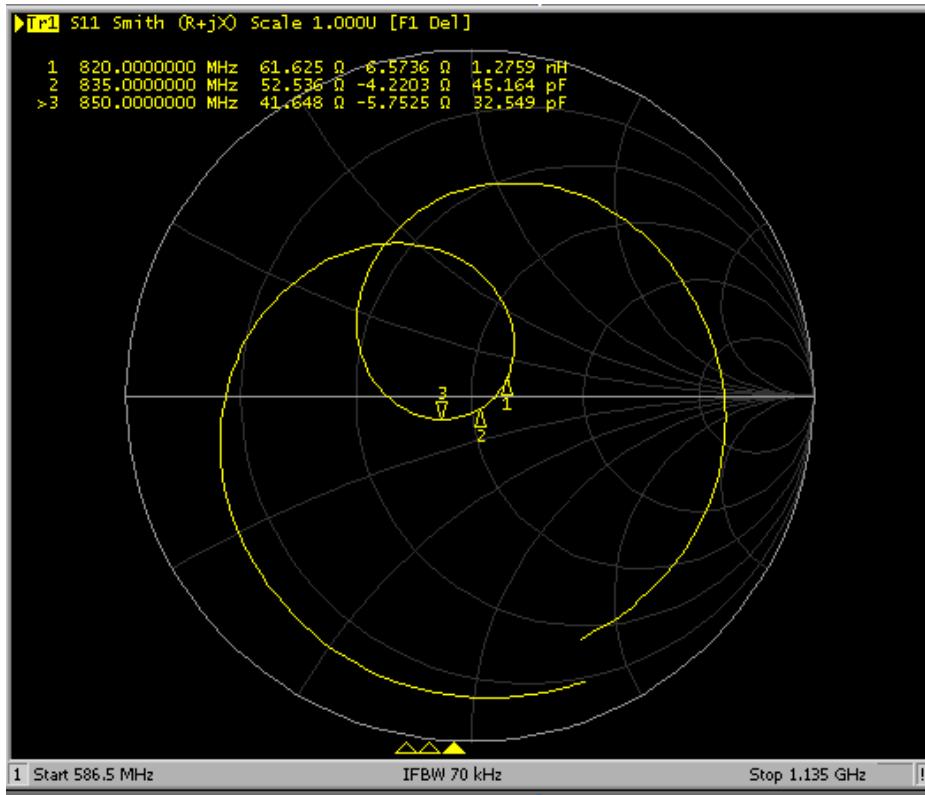

835 Body						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance(ohm)	Delta (ohm)	Imaginary Impedance(ohm)	Delta (ohm)
5.17.2011	-22.106		57.482		-2.174	
6.28.2012	-22.595	-2.21	54.711	-2.771	-6.5731	-4.3991


The return loss is <-20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

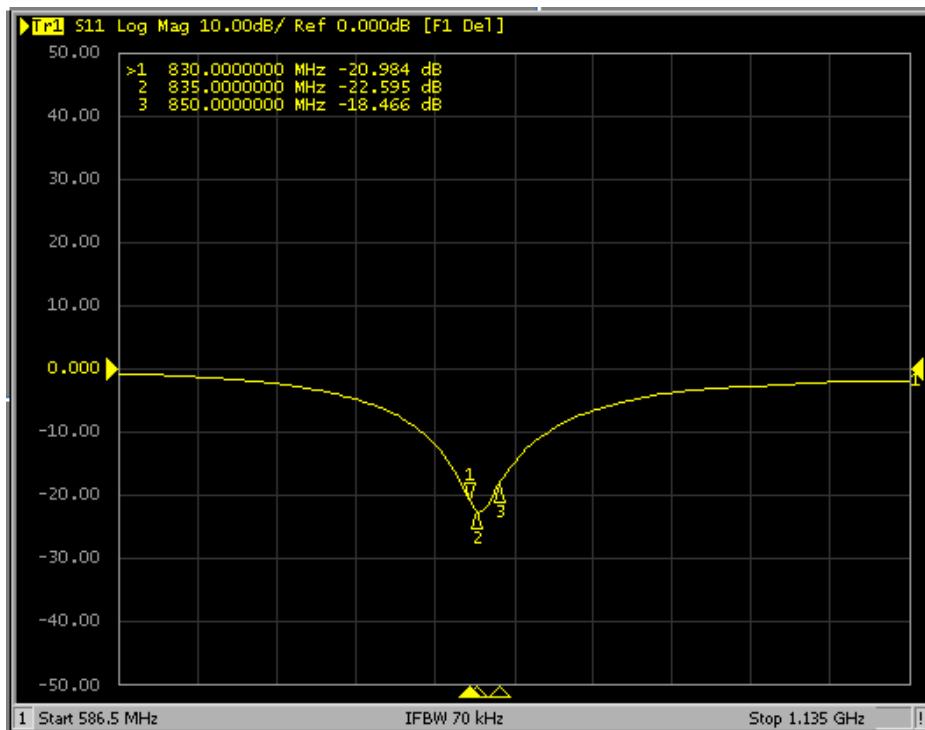


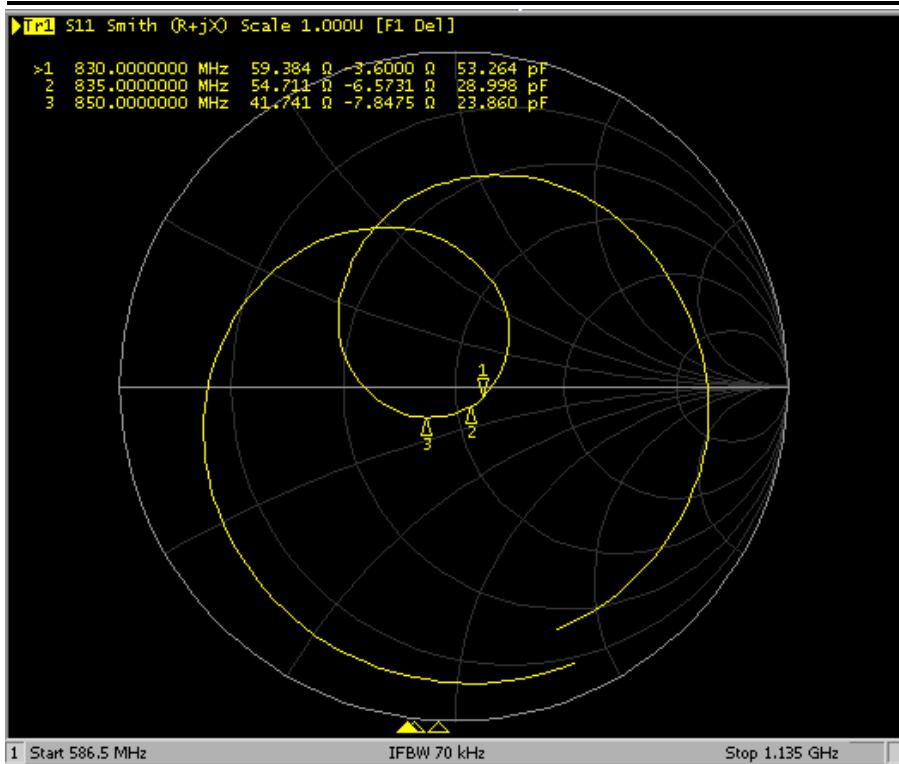

1900 Head						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance(ohm)	Delta (ohm)	Imaginary Impedance(ohm)	Delta (ohm)
5.16.2011	-31.943		51.262		-1.179	
6.28.2012	-33.275	-4.17	49.302	-1.96	-2.1682	-0.9892



The return loss is <-20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

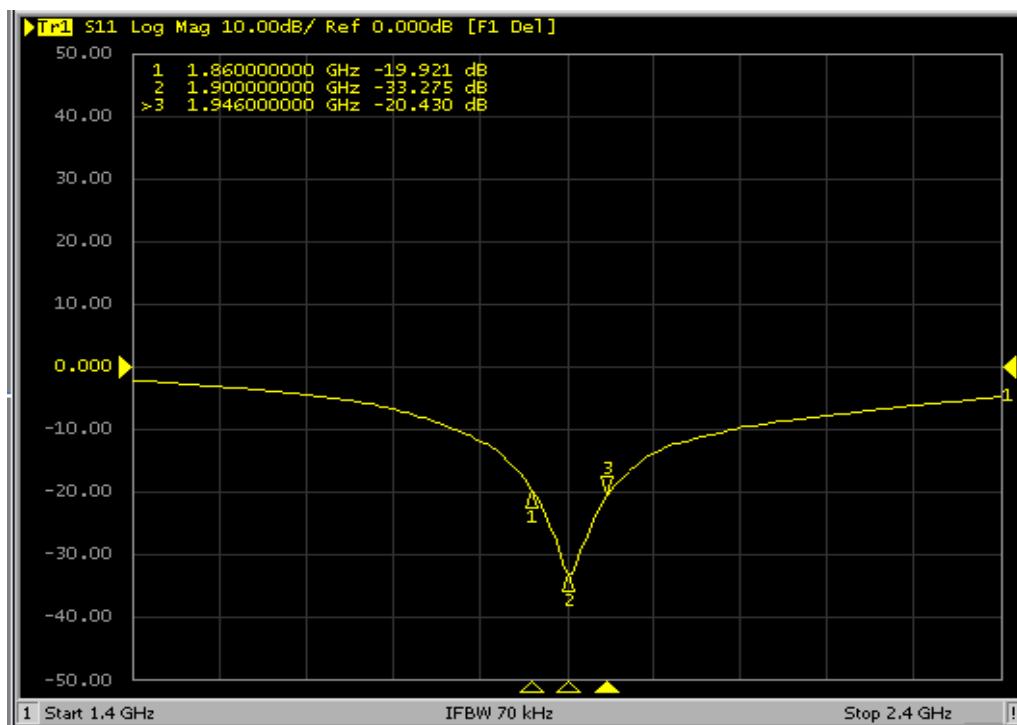

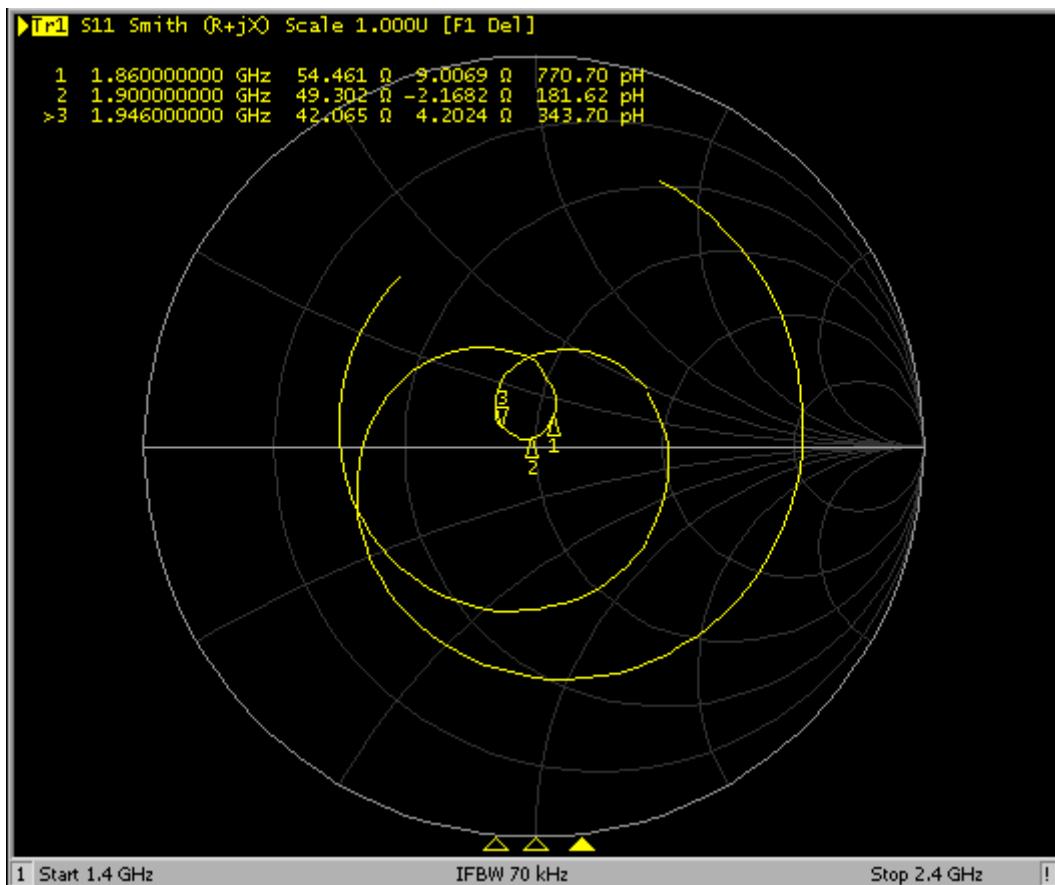

1900 Body						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance(ohm)	Delta (ohm)	Imaginary Impedance(ohm)	Delta (ohm)
5.16.2011	-25.099		53.750		-3.685	
6.28.2012	-25.606	-2.02	50.197	-3.553	-5.6096	-1.9246

The return loss is <-20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

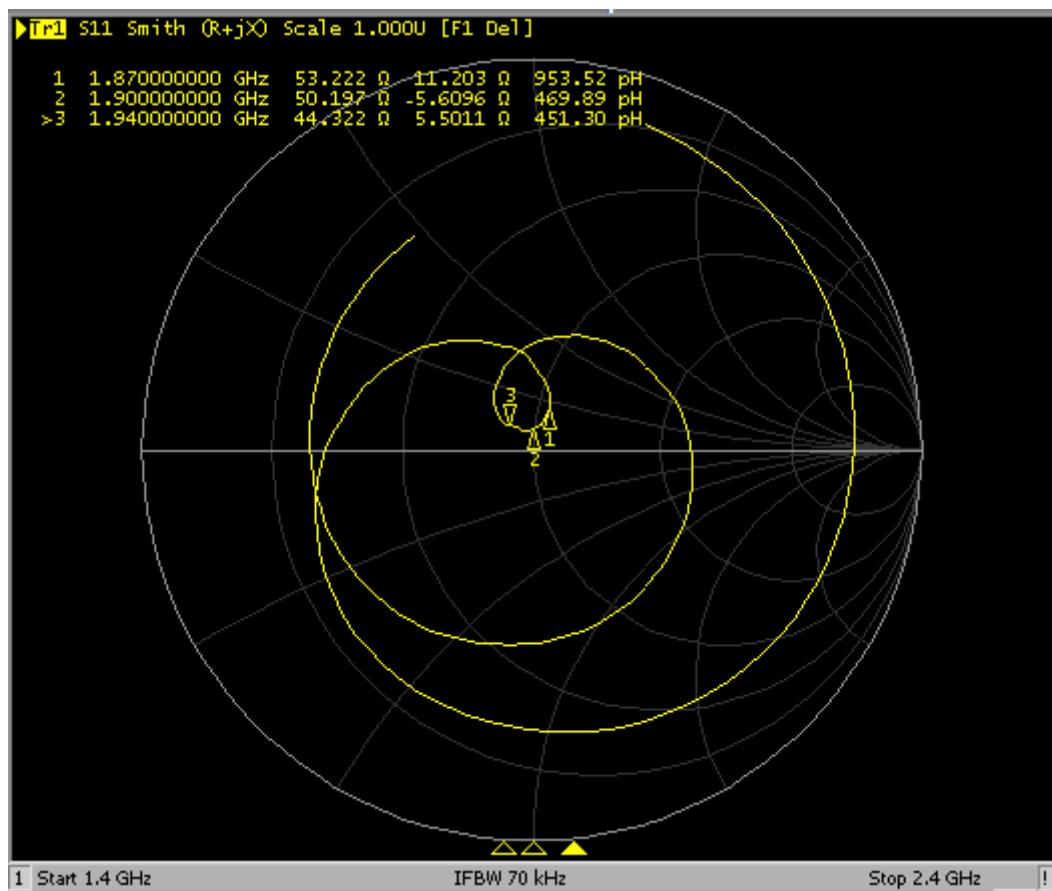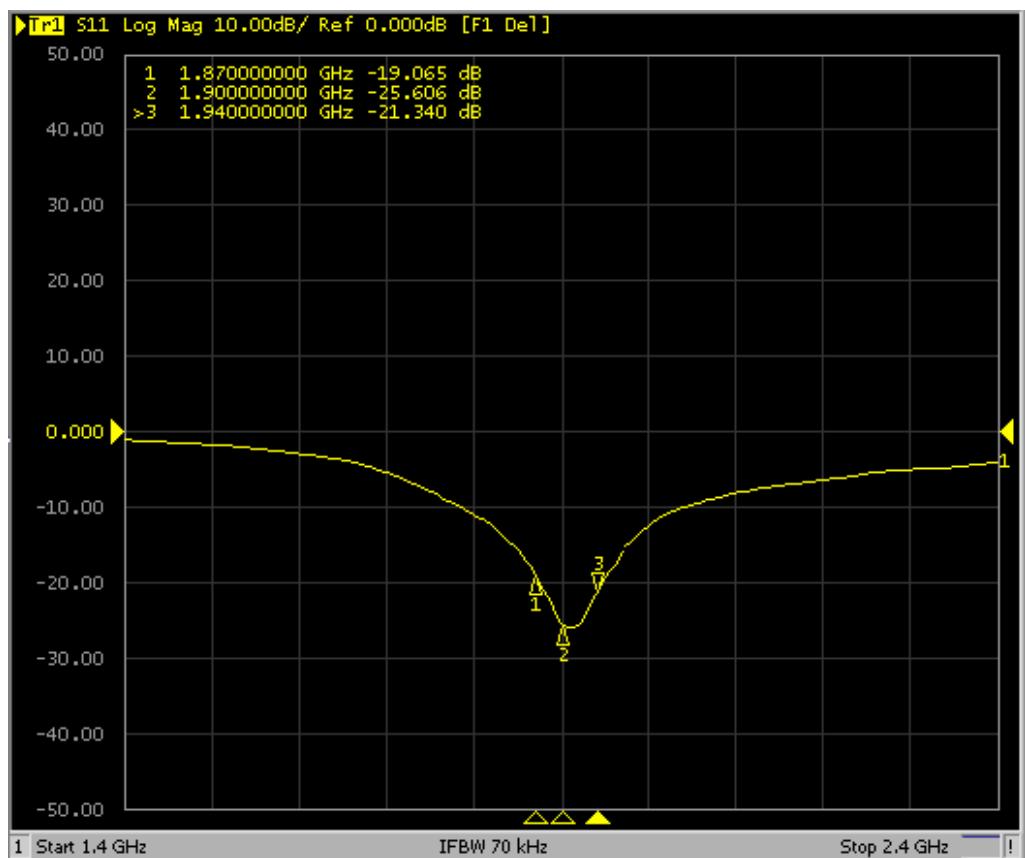

NCL CALIBRATION LABORATORIES**Calibration File No.: PC 1432****Client.: IAC****C E R T I F I C A T E O F C A L I B R A T I O N**

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe

Record of Calibration

Head and Body

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 500-00273

Calibration Procedure: D01-032-E020-V2, D22-012-Tissue, D28-002-Dipole
Project No: ISL-E020-5695

Calibrated: 1st October 2012Released on: 5th October 2012

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By:



Art Brennan, Quality Manager

NCL CALIBRATION LABORATORIES303 Terry Fox Drive, Suite 102
Kanata, Ontario
CANADA K2K 3J1Division of APREL
TEL: (613) 435-8300
FAX: (613) 435-8306

NCL Calibration Laboratories

Division of APREL Inc.

Introduction

This Calibration Report reproduces the results of the calibration performed in line with the references listed below. Calibration is performed using accepted methodologies as per the references listed below. Probes are calibrated for air, and tissue and the values reported are the results from the physical quantification of the probe through meteorgical practices.

Calibration Method

Probes are calibrated using the following methods.

<1000MHz

TEM Cell for sensitivity in air

Standard phantom using temperature transfer method for sensitivity in tissue

>1000MHz

Waveguide* method to determine sensitivity in air and tissue

*Waveguide is numerically (simulation) assessed to determine the field distribution and power

The boundary effect for the probe is assessed using a standard flat phantom where the probe output is compared against a numerically simulated series of data points

References

- o IEEE Standard 1528 (2003) including Amendment 1
IEEE Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques
- o EN 62209-1 (2006)
Human Exposure to RF Fields from hand-held and body-mounted wireless communication devices - Human models. Instrumentation, and procedures-Part 1: Procedure to measure the Specific Absorption Rate (SAR) for hand-held mobile wireless devices
- o IEC 62209-2 Ed. 1.0 (2010-03)
Human exposure to RF fields from hand-held and body-mounted wireless devices - Human models, instrumentation, and procedures - Part 2: specific absorption rate (SAR) for wireless communication devices (30 MHz - 6 GHz)
- o TP-D01-032-E020-V2 E-Field probe calibration procedure
- o D22-012-Tissue dielectric tissue calibration procedure
- o D28-002-Dipole procedure for validation of SAR system using a dipole
- o IEEE 1309 Draft Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9kHz to 40GHz

Page 2 of 10

This page has been reviewed for content and attested to on Page 2 of this document.

NCL Calibration Laboratories
Division of APREL Inc.

Conditions

Probe 500-00273 was a recalibration.

"The probe was received in good working order, although at 1900MHz the uncertainty was higher than our standard (see note")

Ambient Temperature of the Laboratory: 22 °C +/- 1.5°C
Temperature of the Tissue: 21 °C +/- 1.5°C
Relative Humidity: < 60%

Primary Measurement Standards

Instrument	Serial Number	Cal due date
Power meter Anritsu MA2408A	90025437	Nov.5, 2012
Power Sensor Anritsu MA2481D	103555	Nov 5 2012
Attenuator HP 8495A (70dB)	1944A10711	Sept. 13, 2013
Network Analyzer Anritsu MT8801C	MB11855	Feb. 7, 2013

Secondary Measurement Standards

Signal Generator Agilent E4438C -506 MY55182336 June 6, 2013

Attestation

The below named signatories have conducted the calibration and review of the data which is presented in this calibration report.

We the undersigned attest that to the best of our knowledge the calibration of this subject has been accurately conducted and that all information contained within the results pages have been reviewed for accuracy.



Art Brennan, Quality Manager



Dan Brooks, Test Engineer

NCL Calibration Laboratories
Division of APREL Inc.

Probe Summary

Probe Type: E-Field Probe E020
Serial Number: 500-00273
Frequency: As presented on page 5
Sensor Offset: 1.56
Sensor Length: 2.5
Tip Enclosure: Composite*
Tip Diameter: < 2.9 mm
Tip Length: 55 mm
Total Length: 289 mm

*Resistive to recommended tissue recipes per IEEE-1528

Sensitivity in Air

Channel X: 1.2 μ V/(V/m)²
Channel Y: 1.2 μ V/(V/m)²
Channel Z: 1.2 μ V/(V/m)²

Diode Compression Point: 95 mV

NCL Calibration Laboratories

Division of APREL Inc.

Calibration for Tissue (Head H, Body B)

Frequency	Tissue Type	Measured Epsilon	Measured Sigma	Calibration Uncertainty	Tolerance Uncertainty for 5%*	Conversion Factor
450 H	Head	X	X	X	X	X
450 B	Body	X	X	X	X	X
750 H	Head	X	X	X	X	X
750 B	Body	X	X	X	X	X
850 H	Head	42.86	0.95	3.5	3.4	6.5
850 B	Body	53.71	1.04	3.5	3.4	6.4
900 H	Head	41.5	0.99	3.5	3.4	6.1
900 B	Body	53.25	1.04	3.5	3.4	6.3
1450 H	Head	X	X	X	X	X
1450 B	Body	X	X	X	X	X
1500 H	Head	X	X	X	X	X
1500 B	Body	X	X	X	X	X
1640 H	Head	X	X	X	X	X
1640 B	Body	X	X	X	X	X
1750 H	Head	X	X	X	X	X
1750 B	Body	X	X	X	X	X
1800 H	Head	36.85	1.35	3.5	2.7	5.5
1800 B	Body	52.38	1.5	3.5	2.7	5.4
1900 H	Head	38.21	1.46	3.5	2.7	5.7
1900 B	Body	52.1	1.59	3.5	2.7	5.4
2000 H	Head	X	X	X	X	X
2000 B	Body	X	X	X	X	X
2100 H	Head	39.8	1.49	3.5	2.9	5.0
2100 B	Body	53.0	1.58	3.5	2.9	4.9
2300 H	Head	X	X	X	X	X
2300 B	Body	X	X	X	X	X
2450 H	Head	38.2	1.84	3.5	3.5	4.65
2450 B	Body	50.63	1.99	3.5	3.5	4.4
2600 H	Head	X	X	X	X	X
2600 B	Body	X	X	X	X	X
3000 H	Head	X	X	X	X	X
3000 B	Body	X	X	X	X	X
3600 H	Head	X	X	X	X	X
3600 B	Body	X	X	X	X	X
5200 H	Head	X	X	X	X	X
5200 B	Body	X	X	X	X	X
5600 H	Head	X	X	X	X	X
5600 B	Body	X	X	X	X	X
5800 H	Head	X	X	X	X	X
5800 B	Body	X	X	X	X	X

NCL Calibration Laboratories
Division of APREL Inc.

Boundary Effect:

Uncertainty resulting from the boundary effect is less than 2.1% for the distance between the tip of the probe and the tissue boundary, when less than 0.58mm.

Spatial Resolution:

The spatial resolution uncertainty is less than 1.5% for 4.9mm diameter probe.
The spatial resolution uncertainty is less than 1.0% for 2.5mm diameter probe.

DAQ-PAQ Contribution

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

Boundary Effect:

For a distance of 0.58mm the worst case evaluated uncertainty (increase in the probe sensitivity) is less than 2.1%.

NOTES:

*The maximum deviation from the centre frequency when comparing the lower to upper range is listed.

**1800MHz Head was evaluated at close to the 10% allowable deviation; the deviation has now been normalized to within 2%.

***1800MHz Body was evaluated at close to the 10% allowable deviation; the deviation has now been normalized to within 2%.


****1900MHz Body was evaluated at close to the 10% allowable deviation; the deviation has now been normalized to within 2%.

*****2450MHz Head was evaluated at close to the 10% allowable deviation; the deviation has now been normalized to within 2%.

*****2450MHz Body was evaluated at close to the 10% allowable deviation; the deviation has now been normalized to within 2%.



NCL Calibration Laboratories
Division of APREL Inc.

Receiving Pattern Air

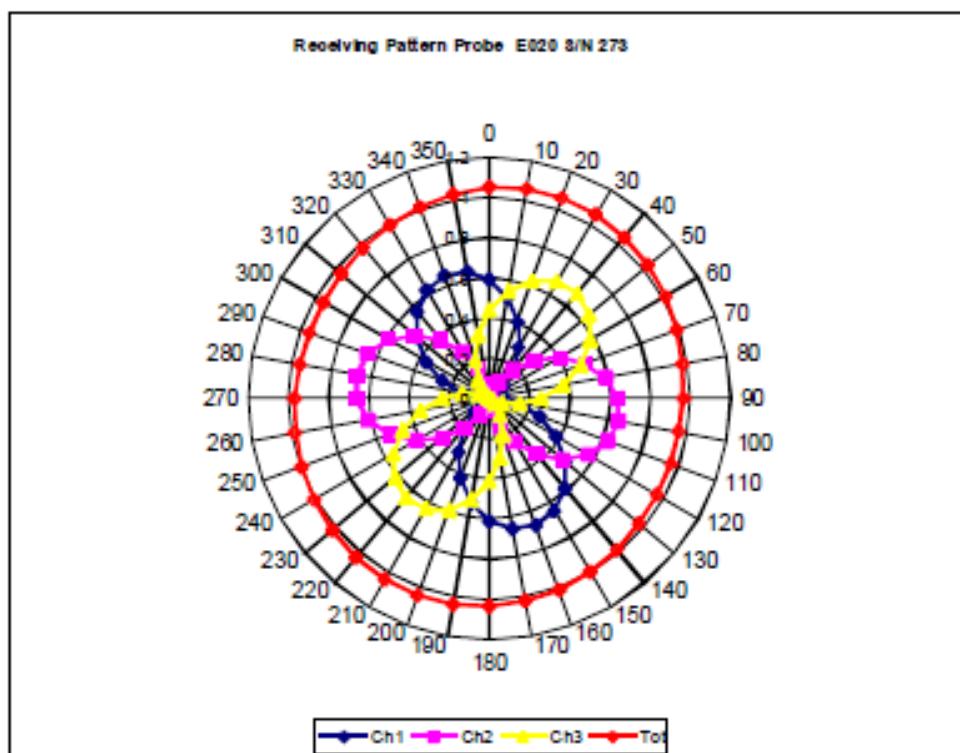

NCL Calibration Laboratories
Division of APREL Inc.


Isotropy Error Air

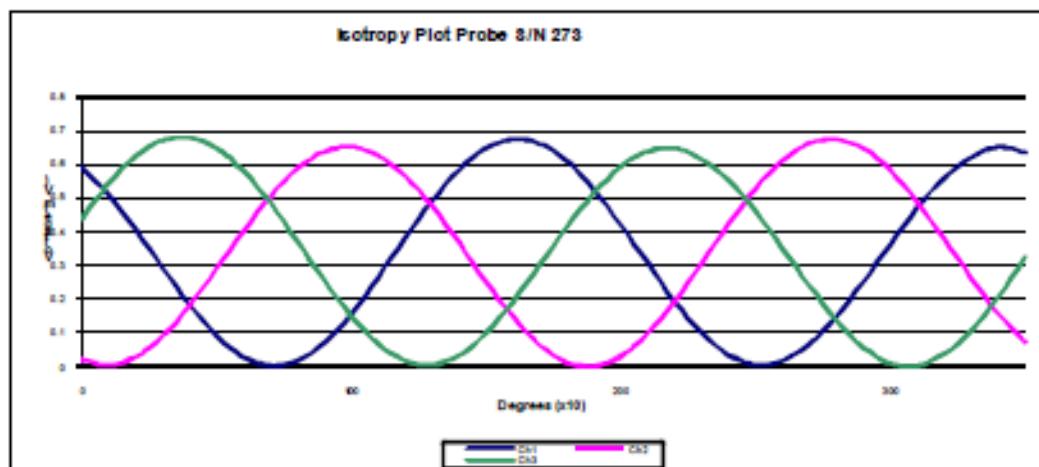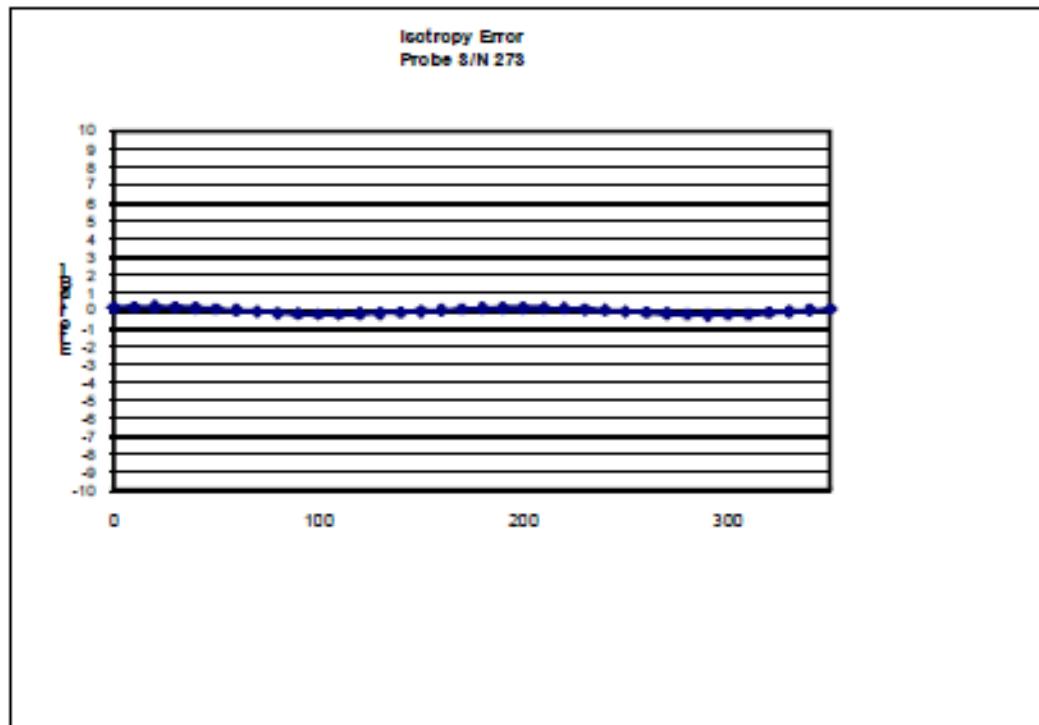

Isotropicity Tissue: 0.10 dB


NCL Calibration Laboratories
Division of APREL Inc.

Dynamic Range

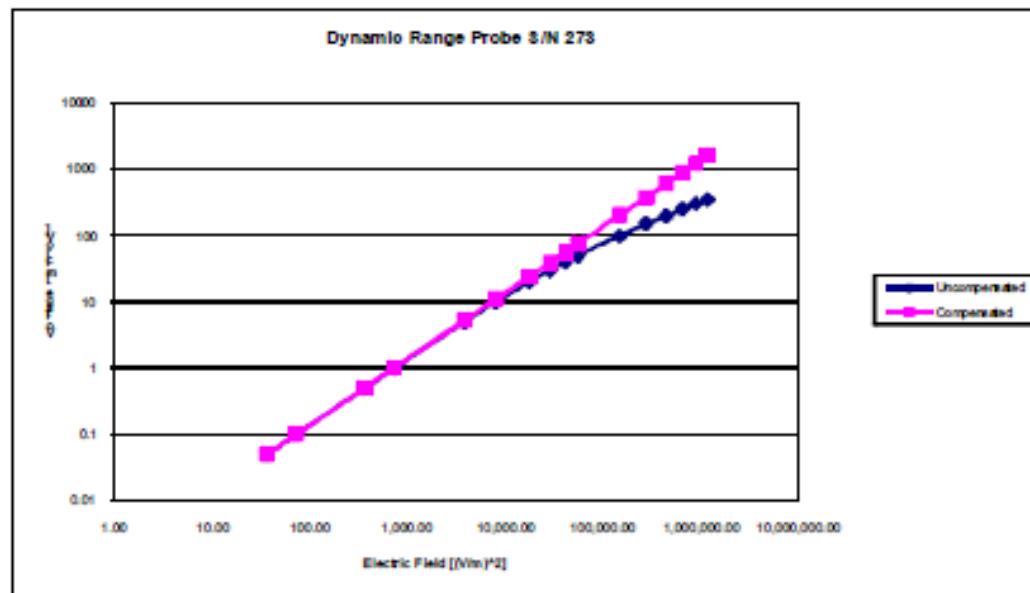

NCL Calibration Laboratories
Division of APREL Inc.

Video Bandwidth

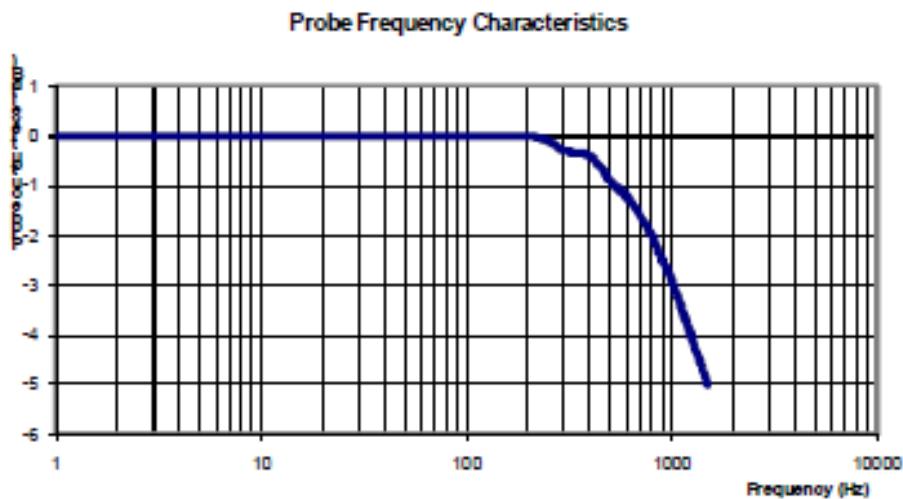

Video Bandwidth at 500 Hz: 1 dB
Video Bandwidth at 1.02 KHz: 3 dB

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\INCL\Calibration Equipment\Instrument List May 2012.

Page 10 of 10
This page has been reviewed for content and attested to on Page 2 of this document.

NCL CALIBRATION LABORATORIES

Calibration File No: DC-1217/18
Project Number: SGL-IAC-DC-5582-93

C E R T I F I C A T E O F C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.

Validation Dipole
835MHz Head & Body

Manufacturer: APREL Laboratories

Part number: ALS-D-835-S-2

Frequency: 835MHz


Serial No: 180-00556

Customer: IAC

Calibrated: 17th May 2011
Released on: 27th May 2011

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By:

**NCL CALIBRATION LABORATORIES**

303 Terry Fox Drive, Suite 102
Kanata, Ontario
CANADA K2K 3J1

Division of APREL
TEL: (613) 435-8300
FAX: (613) 435-8306

NCL Calibration Laboratories
Division of APREL Inc.


Conditions

Dipole 180-00556 was a re-calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C
Temperature of the Tissue: 21 °C +/- 0.5°C

Dipoles are calibrated on the ALSAS-10U with a feed power normalized to 1Watt.

We the undersigned attest that to the best of our knowledge the calibration of this device has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



Stuart Nicol



C. Teodorian

Primary Measurement Standards

Instrument	Serial Number	Cal due date
Power meter Anritsu MA2408A	90025437	Nov.4, 2010
Power Sensor Anritsu MA2481D	103555	Nov 4, 2010
Attenuator HP 8495A (70dB)	1944A10711	Sept. 14, 2010
Network Analyzer Anritsu MT8801C	MB11855	Feb. 8, 2011

Secondary Measurement Standards

Signal Generator Agilent E4438C -506 MY55182336 June 7, 2011

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Inc.

Calibration Results Summary

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

Mechanical Dimensions

Length: 161.0 mm
Height: 89.8 mm


Electrical Specification 835MHz

Tissue Type	Return Loss:	Impedance:	SWR:
Head	-26.655	51.666	1.102U
Body	-22.106	57.482	1.177U

System Validation Results

Tissue	Frequency	1 Gram	10 Gram	Peak
Head	835 MHz	9.590	6.003	15.013
Body	835 MHz	9.981	6.006	15.013

835MHz

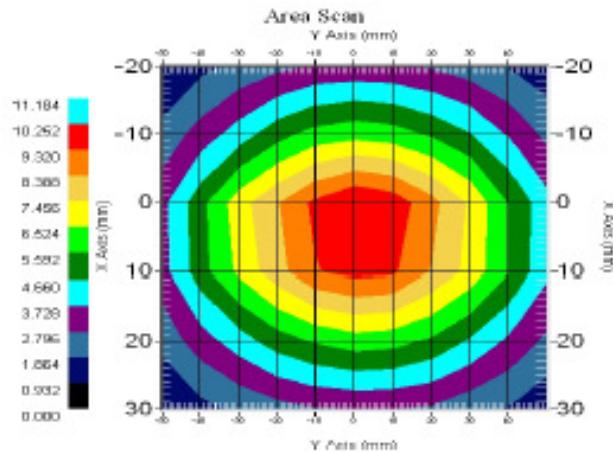

This page has been reviewed for content and attested to by signature within this document.

3

NCL Calibration Laboratories

Division of APREL Inc.

Introduction

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018-ALSAS. The results contained within this report are for Validation Dipole 190-00606. The calibration routine consisted of a three-step process. Step 1 was a mechanical verification of the dipole to ensure that it meets the mechanical specifications. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALSAS-10U, along with APREL E-030 130 MHz to 26 GHz E-Field Probe Serial Number 215.

References

- o IEEE Standard 1528 (2003) including Amendment 1
IEEE Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques
- o EN 62209-1 (2006)
Human Exposure to RF Fields from hand-held and body-mounted wireless communication devices - Human models, instrumentation, and procedures-Part 1: Procedure to measure the Specific Absorption Rate (SAR) for hand-held mobile wireless devices
- o IEC 62209-2 Ed. 1.0 (2010-03)
Human exposure to RF fields from hand-held and body-mounted wireless devices - Human models, instrumentation, and procedures - Part 2: specific absorption rate (SAR) for wireless communication devices (30 MHz - 6 GHz)
- o TP-D01-032-E020-V2 E-Field probe calibration procedure
- o D22-012-Tissue dielectric tissue calibration procedure
- o D28-002-Dipole procedure for validation of SAR system using a dipole
- o IEEE 1309 Draft Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9kHz to 40GHz

Conditions

Dipole 190-00606 was a re-calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C
Temperature of the Tissue: 20 °C +/- 0.5°C

This page has been reviewed for content and attested to by signature within this document.

4


NCL Calibration Laboratories
Division of APREL Inc.

Electrical Calibration


Electrical Specification 835MHz

Tissue Type	Measured Epsilon	Measured Sigma
Head	41.09	0.89
Body	53.15	0.95

Head Tissue

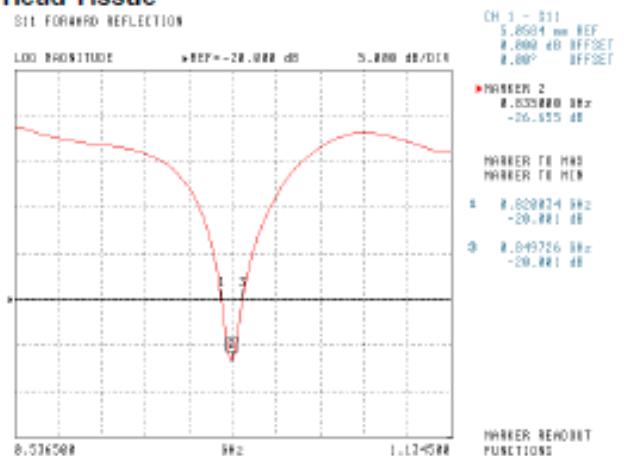

Body Tissue

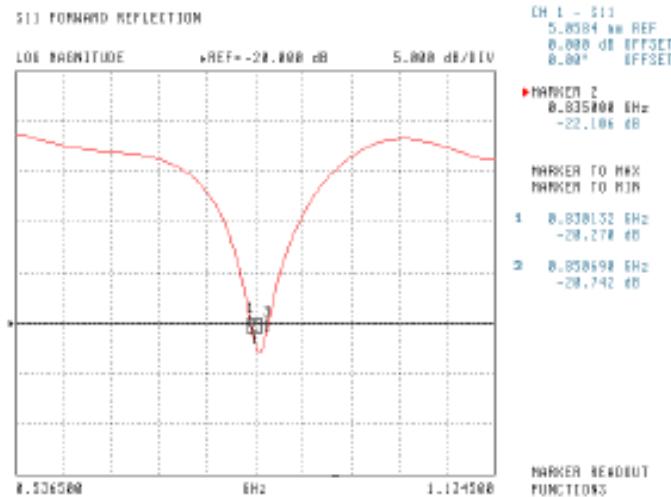

This page has been reviewed for content and attested to by signature within this document.



5

NCL Calibration Laboratories

Division of APREL Inc.

**Electrical Specification 835MHz
Impedance**

Tissue Type	Measured Epsilon	Measured Sigma
Head	41.09	0.89
Body	53.15	0.95

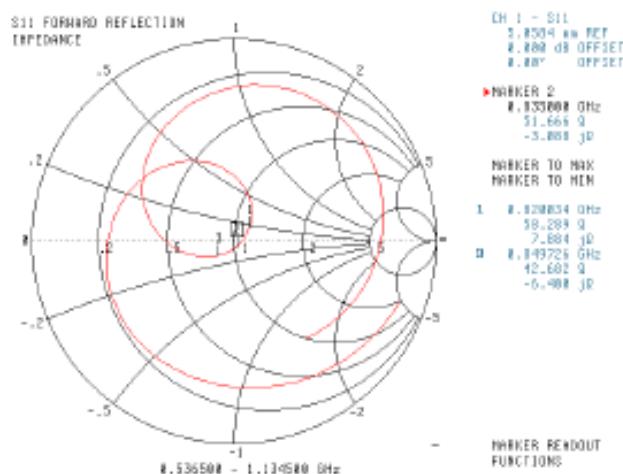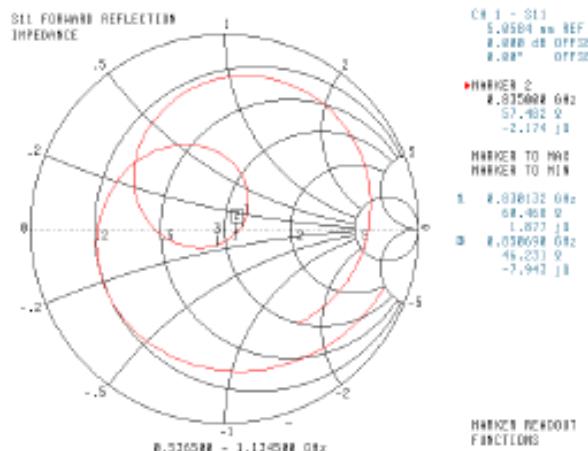
Head Tissue**Body Tissue**

NCL Calibration Laboratories
Division of APREL Inc.


Electrical Specification 835MHz
Standing Wave Ratio

Tissue Type	Measured Epsilon	Measured Sigma
Head	41.09	0.89
Body	53.15	0.95

Head Tissue

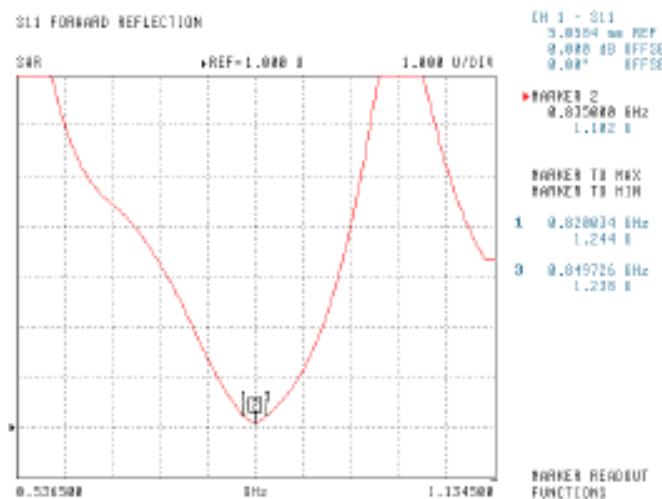

Body Tissue

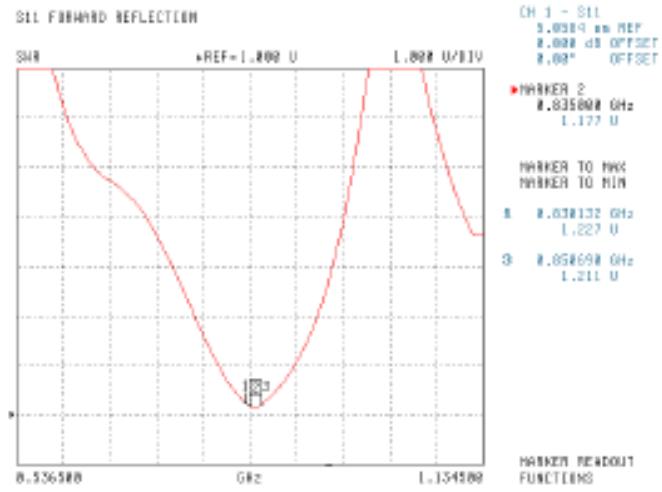

This page has been reviewed for content and attested to by signature within this document.

7

NCL Calibration Laboratories
Division of APREL Inc.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2011.

This page has been reviewed for content and attested to by signature within this document.

8

NCL CALIBRATION LABORATORIES

Calibration File No: DC-1224/5
Project Number: SGL-IAC-DC-5582-93

C E R T I F I C A T E O F C A L I B R A T I O N

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.


Validation Dipole
1900MHz Head & Body

Manufacturer: APREL Laboratories
Part number: ALS-D-1900-S-2
Frequency: 1900MHz
Serial No: 210-00707

Customer: IAC

Calibrated: 16th May 2011
Released on: 27th May 2011

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: 

NCL CALIBRATION LABORATORIES

303 Terry Fox Drive, Suite 102
Kanata, Ontario
CANADA K2K 3J1

Division of APREL
TEL: (613) 435-8300
FAX: (613) 435-8306

NCL Calibration Laboratories
Division of APREL Inc.


Conditions

Dipole 210-00707 was a new dipole taken from stock.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C
Temperature of the Tissue: 21 °C +/- 0.5°C

Dipoles are calibrated on the ALSAS-10U with a feed power normalized to 1Watt.

We the undersigned attest that to the best of our knowledge the calibration of this device has been accurately conducted and that all information contained within this report has been reviewed for accuracy.



Stuart Nicol



C. Teodorian

Primary Measurement Standards

Instrument	Serial Number	Cal due date
Power meter Anritsu MA2408A	190025437	Nov.4, 2010
Power Sensor Anritsu MA2481D	103555	Nov 4, 2010
Attenuator HP 8495A (70dB)	1944A10711	Sept. 14, 2010
Network Analyzer Anritsu MT8801C	MB11855	Feb. 8, 2011

Secondary Measurement Standards

Signal Generator Agilent E4438C -506 MY55182336 June 7, 2011

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Inc.

Calibration Results Summary

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

Mechanical Dimensions


Length: 67.1 mm
Height: 38.9 mm

Electrical Specification 1900MHz

Tissue Type	Return Loss:	Impedance:	SWR:
Head	-31.943	51.262	1.055U
Body	-25.099	57.750	1.119U

System Validation Results

Tissue	Frequency	1 Gram	10 Gram	Peak
Head	1900 MHz	39.378	19.668	77.268
Body	1900 MHz	39.654	19.668	77.268

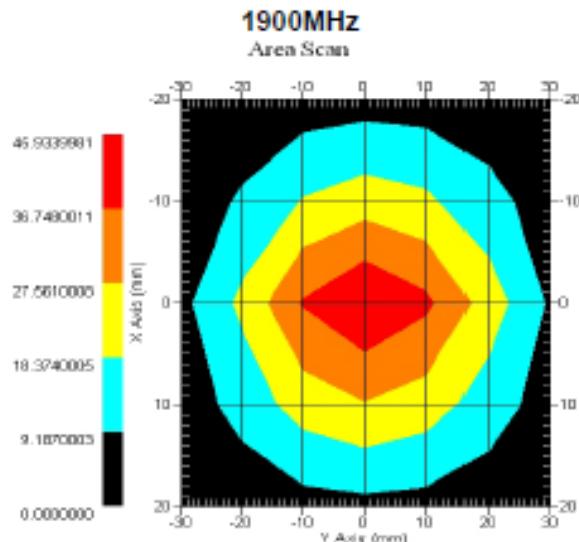

This page has been reviewed for content and attested to by signature within this document.

3

NCL Calibration Laboratories

Division of APREL Inc.

Introduction

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018-ALSAS. The results contained within this report are for Validation Dipole 200-00657. The calibration routine consisted of a three-step process. Step 1 was a mechanical verification of the dipole to ensure that it meets the mechanical specifications. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALSAS-10U, along with APREL E-030 130 MHz to 26 GHz E-Field Probe Serial Number 215.

References

- o IEEE Standard 1528 (2003) including Amendment 1
IEEE Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques
- o EN 62209-1 (2006)
Human Exposure to RF Fields from hand-held and body-mounted wireless communication devices - Human models, instrumentation, and procedures-Part 1: Procedure to measure the Specific Absorption Rate (SAR) for hand-held mobile wireless devices
- o IEC 62209-2 Ed. 1.0 (2010-03)
Human exposure to RF fields from hand-held and body-mounted wireless devices - Human models, instrumentation, and procedures - Part 2: specific absorption rate (SAR) for wireless communication devices (30 MHz - 6 GHz)
- o TP-D01-032-E020-V2 E-Field probe calibration procedure
- o D22-012-Tissue dielectric tissue calibration procedure
- o D28-002-Dipole procedure for validation of SAR system using a dipole
- o IEEE 1309 Draft Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9kHz to 40GHz

Conditions

Dipole 200-00657 was a re-calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C
Temperature of the Tissue: 20 °C +/- 0.5°C

This page has been reviewed for content and attested to by signature within this document.

4


NCL Calibration Laboratories
Division of APREL Inc.

Electrical Calibration


Electrical Specification 1900MHz

Tissue Type	Measured Epsilon	Measured Sigma
Head	38.12	1.41
Body	51.52	1.57

Head Tissue

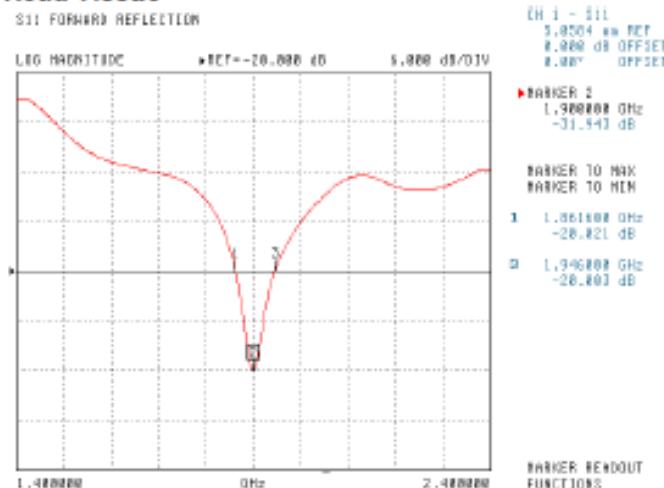

Body Tissue

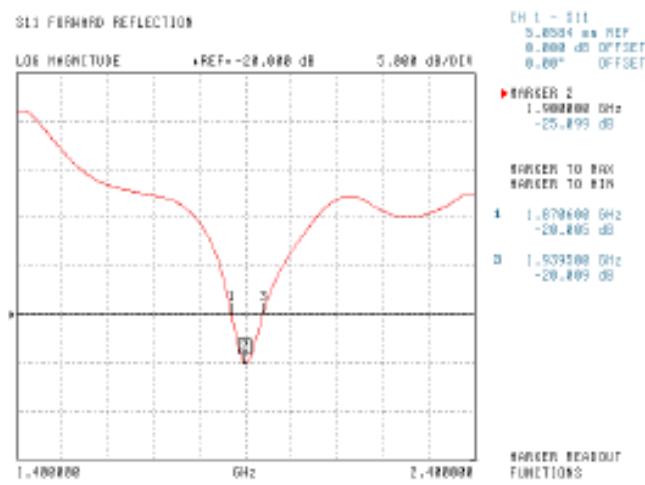


This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Inc.


Electrical Specification 1900MHz
Impedance

Tissue Type	Measured Epsilon	Measured Sigma
Head	38.12	1.41
Body	51.52	1.57

Head Tissue

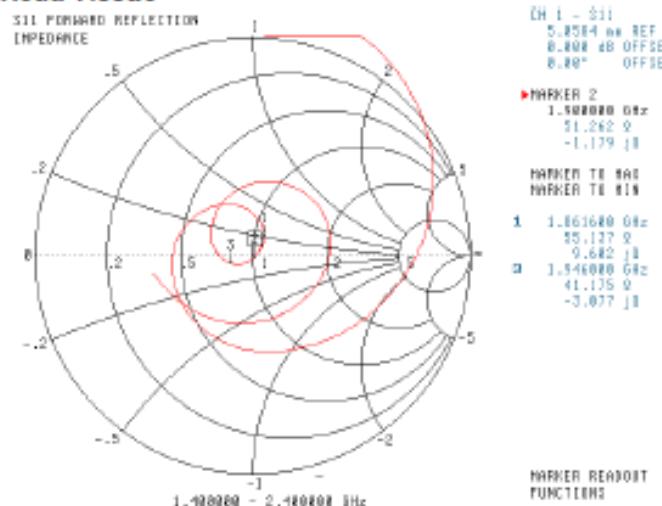

Body Tissue

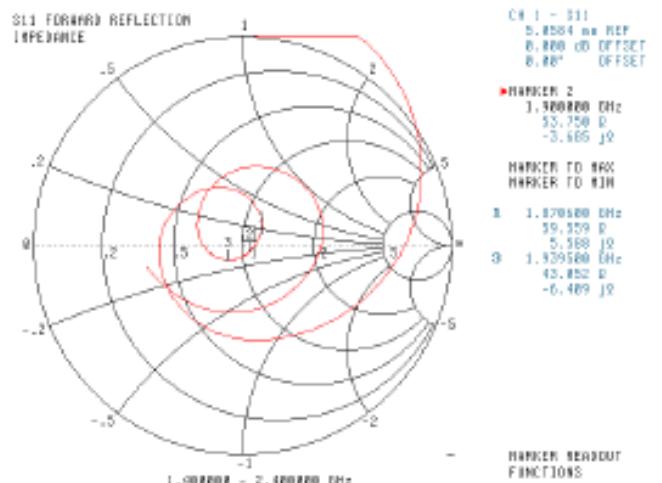



This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories

Division of APREL Inc.

**Electrical Specification 1900MHz
Standing Wave Ratio**

Tissue Type	Measured Epsilon	Measured Sigma
Head	38.12	1.41
Body	51.52	1.57

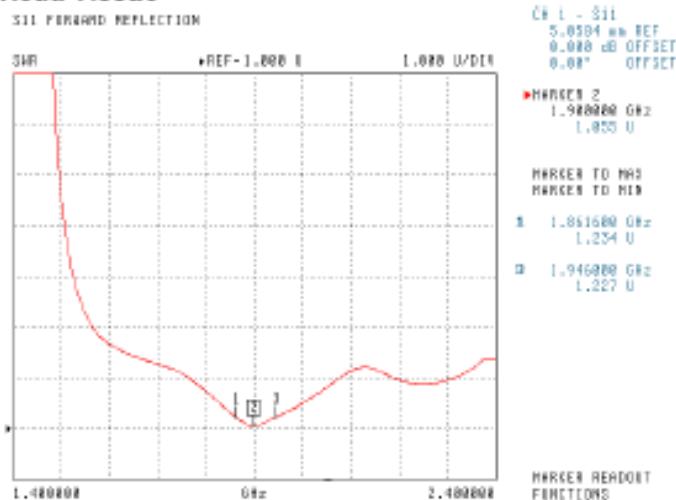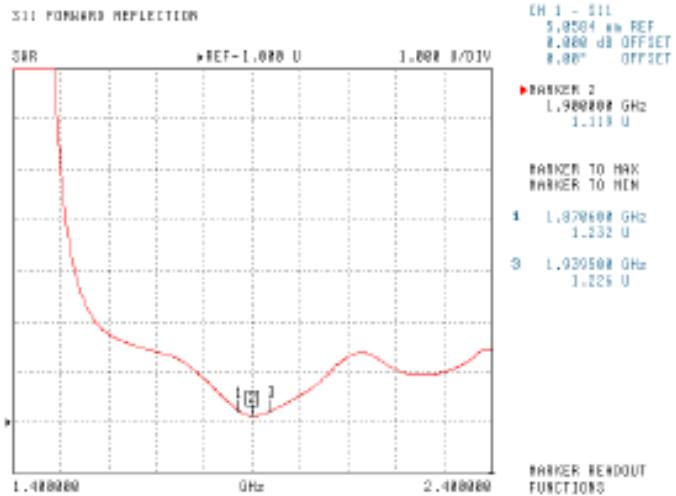Head Tissue**Body Tissue**

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories
Division of APREL Inc.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2011.

This page has been reviewed for content and attested to by signature within this document.

8